

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
 Data File : PD086820.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 23:11
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4016

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:43:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:36:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.885	70624372	427.2E6	38.801	37.322
27)	SA Decachlor...	9.092	8.091	199.5E6	929.9E6	75.931	73.234
Target Compounds							
2)	A alpha-BHC	4.008	3.399	144.7E6	681.8E6	41.876	38.202
3)	MA gamma-BHC...	4.340	3.736	140.9E6	629.0E6	41.215	37.791
4)	MA Heptachlor	4.940	4.092	138.4E6	639.1E6	40.536	37.367
9)	A Endosulfan I	6.087	5.259	116.7E6	535.8E6	39.702	37.112
13)	MA Dieldrin	6.359	5.526	264.9E6	1145.8E6	81.640	75.132
14)	MA Endrin	6.587	5.802	218.2E6	1027.5E6	81.752	74.581
16)	A 4,4'-DDD	6.717	5.943	191.5E6	902.5E6	81.682	74.937
17)	MA 4,4'-DDT	7.034	6.198	200.0E6	971.2E6	81.571	75.151
20)	A Methoxychlor	7.506	6.770	522.6E6	2052.3E6	387.494	353.365


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 23:11
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:43:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:36:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

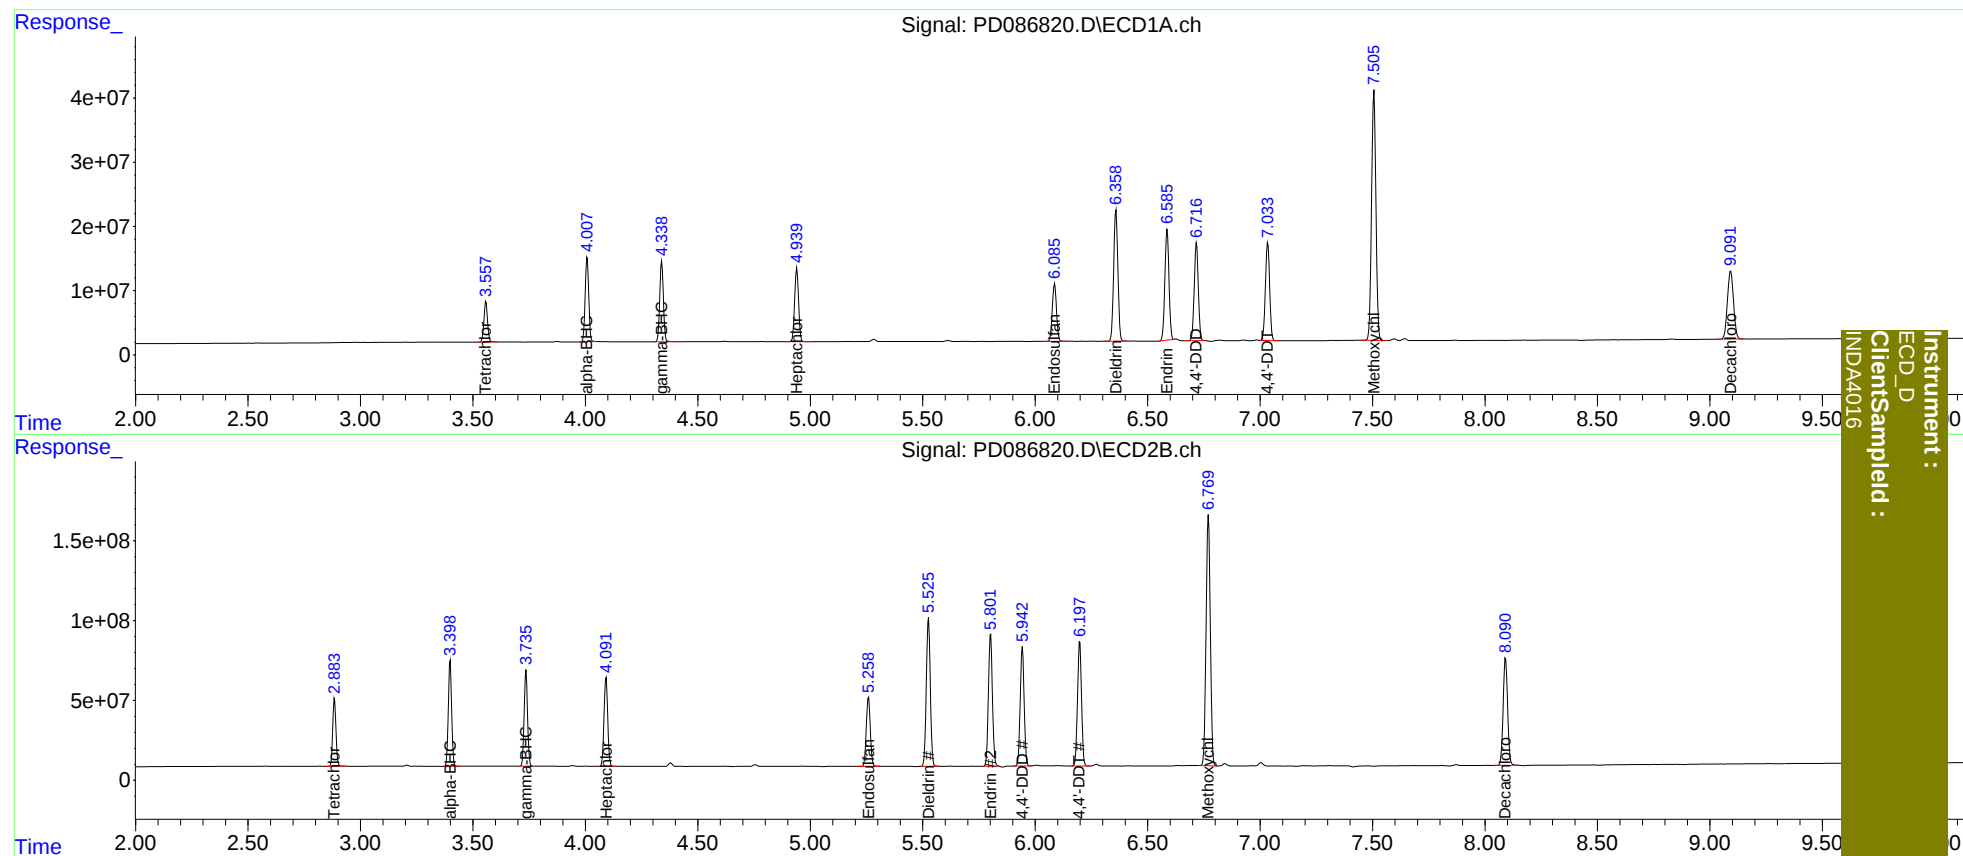


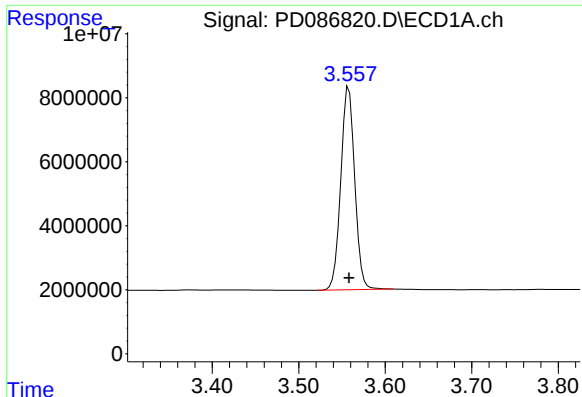

#1 Tetrachloro-m-xylene


R.T.: 3.558 min
Delta R.T.: 0.000 min
Response: 70624372
Conc: 38.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4016

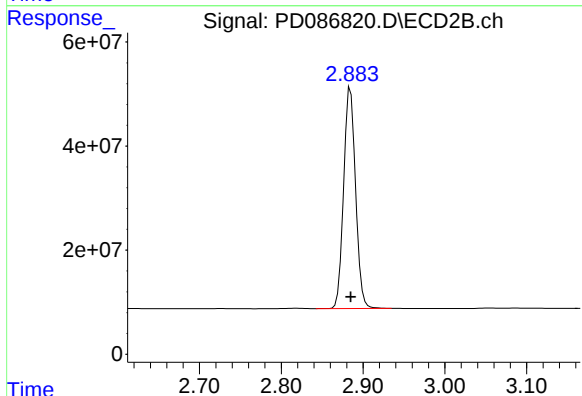


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 427163399
Conc: 37.32 ng/ml

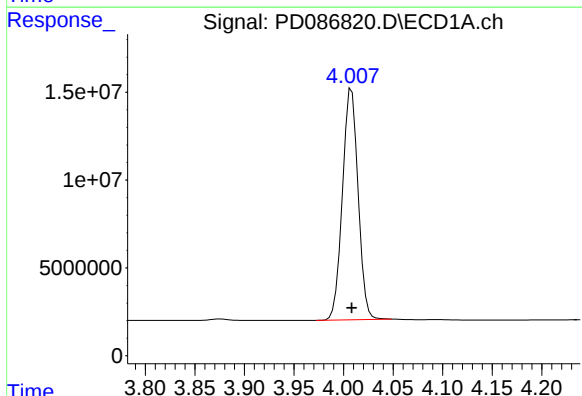


#2 alpha-BHC

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 144684638
Conc: 41.88 ng/ml

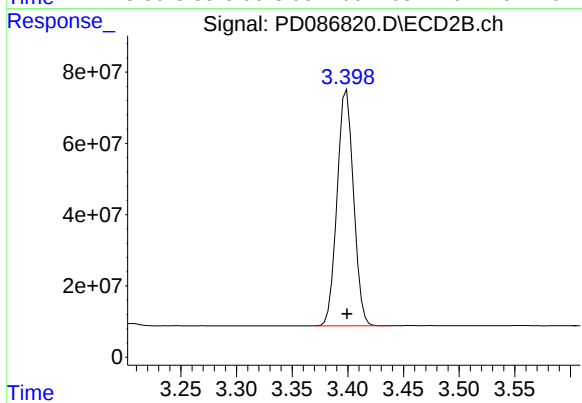

#2 alpha-BHC


R.T.: 3.399 min
Delta R.T.: 0.000 min
Response: 681784214
Conc: 38.20 ng/ml

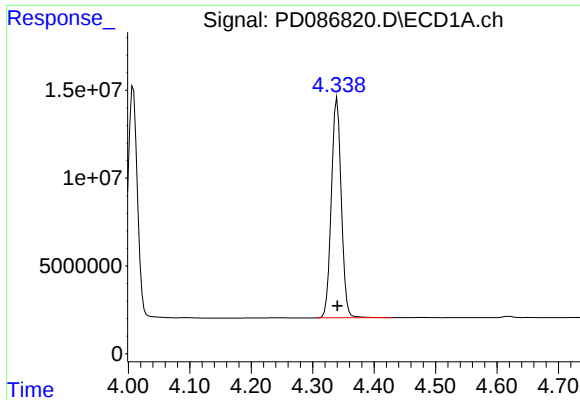

#3 gamma-BHC (Lindane)


R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 140896276
Conc: 41.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4016

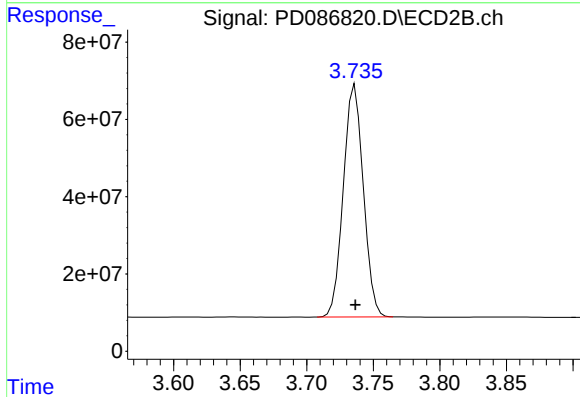


#3 gamma-BHC (Lindane)

R.T.: 3.736 min
Delta R.T.: 0.000 min
Response: 628999070
Conc: 37.79 ng/ml

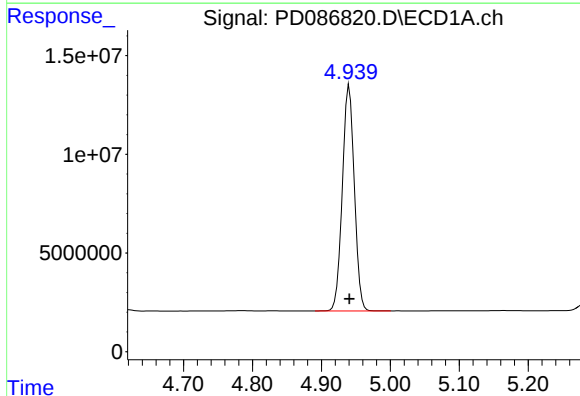


#4 Heptachlor

R.T.: 4.940 min
Delta R.T.: 0.000 min
Response: 138392228
Conc: 40.54 ng/ml

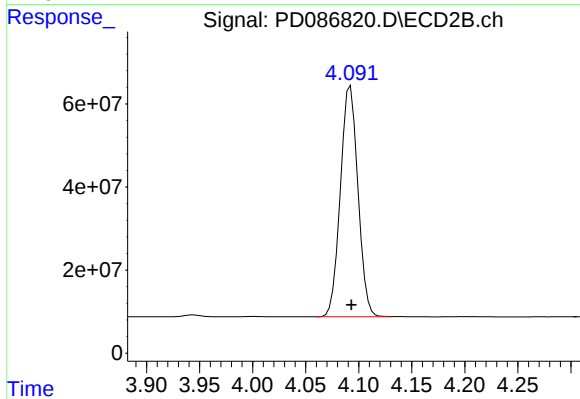

#4 Heptachlor


R.T.: 4.092 min
Delta R.T.: 0.000 min
Response: 639139632
Conc: 37.37 ng/ml

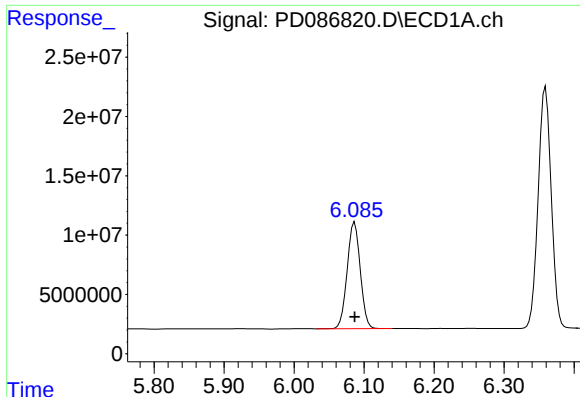

#9 Endosulfan I


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 116676080
Conc: 39.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4016

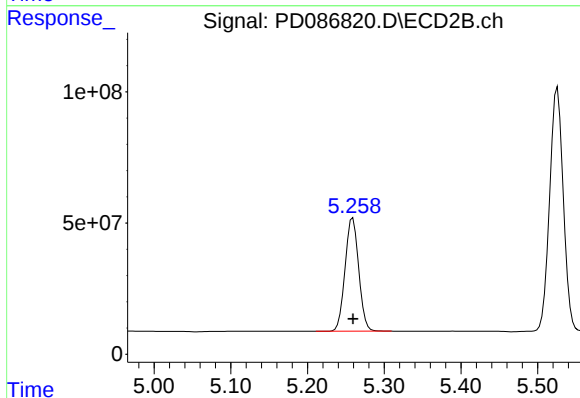


#9 Endosulfan I

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 535824196
Conc: 37.11 ng/ml

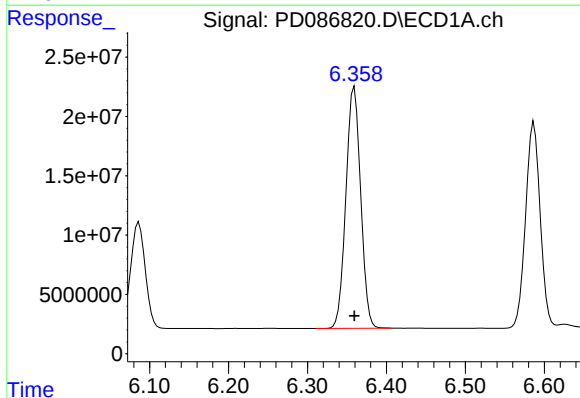


#13 Dieldrin

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 264919827
Conc: 81.64 ng/ml

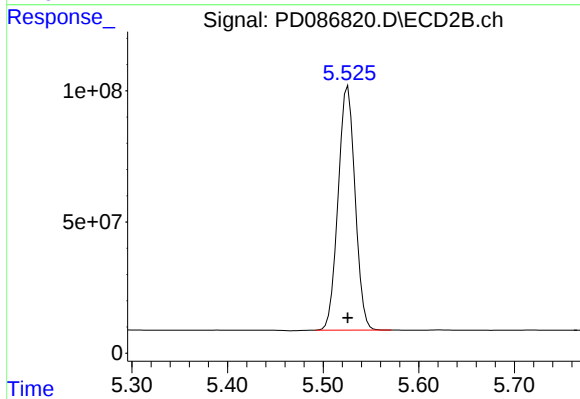

#13 Dieldrin


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 1145809275
Conc: 75.13 ng/ml

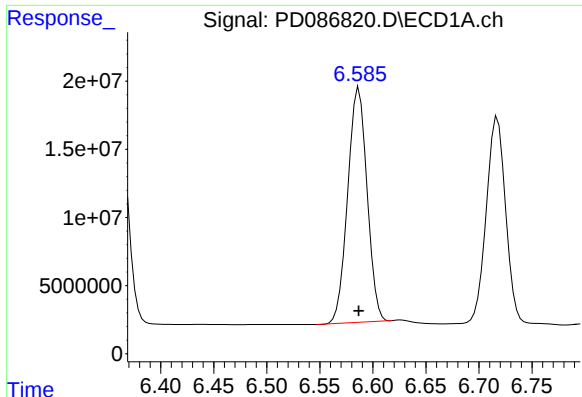

#14 Endrin


R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 218185726
Conc: 81.75 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4016

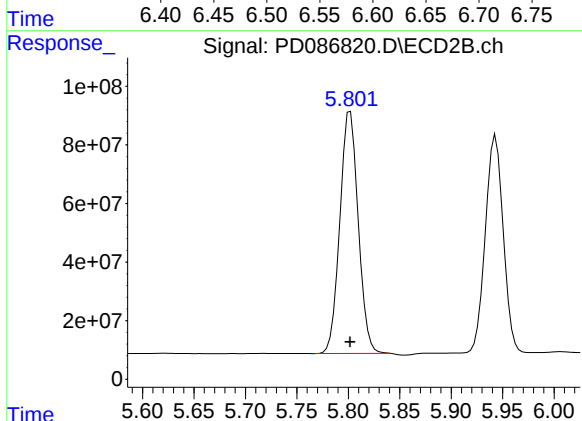


#14 Endrin

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 1027518010
Conc: 74.58 ng/ml

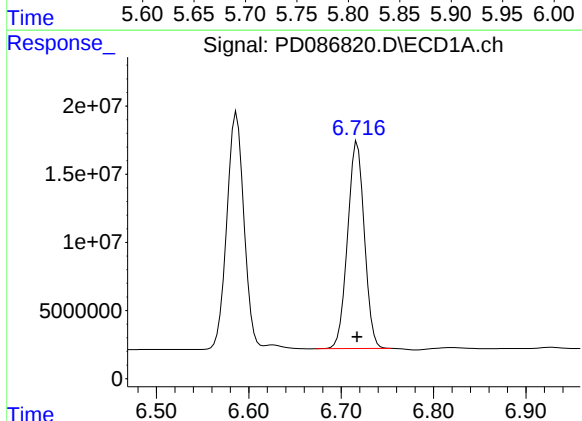


#16 4,4'-DDD

R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 191464334
Conc: 81.68 ng/ml

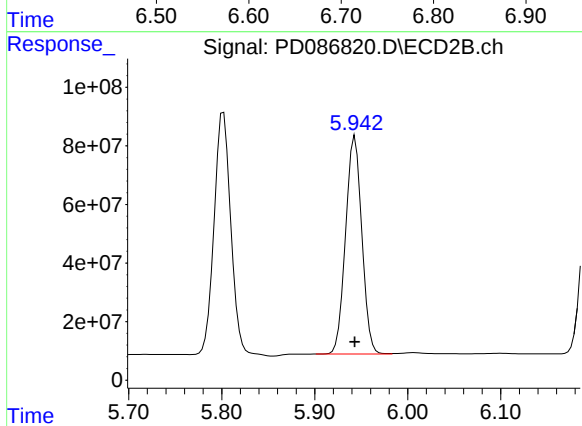

#16 4,4'-DDD


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 902533178
Conc: 74.94 ng/ml

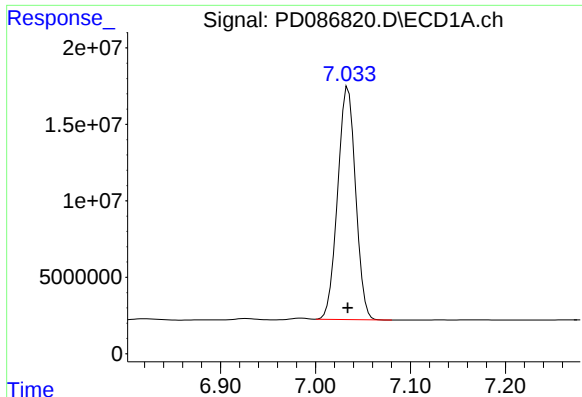

#17 4,4'-DDT


R.T.: 7.034 min
Delta R.T.: 0.000 min
Response: 199966783
Conc: 81.57 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4016

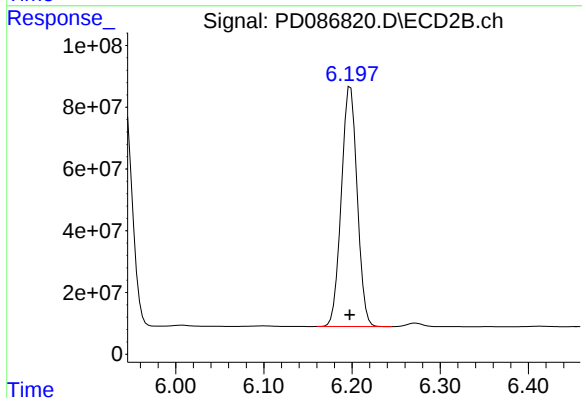


#17 4,4'-DDT

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 971234251
Conc: 75.15 ng/ml

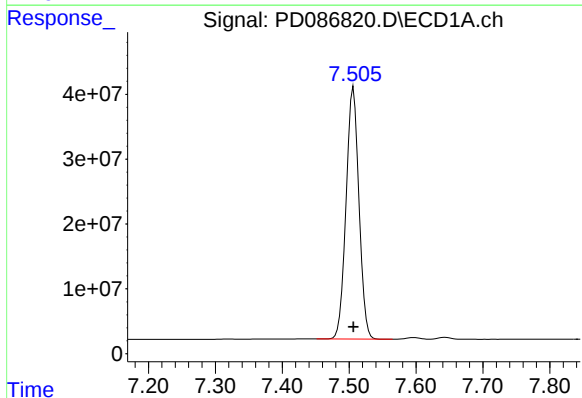


#20 Methoxychlor

R.T.: 7.506 min
Delta R.T.: 0.000 min
Response: 522618143
Conc: 387.49 ng/ml

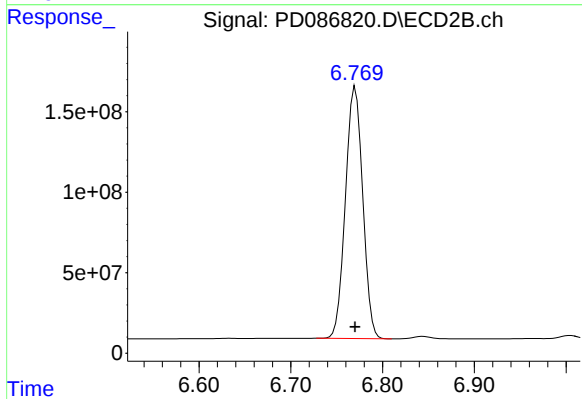

#20 Methoxychlor

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 2052299336
Conc: 353.37 ng/ml

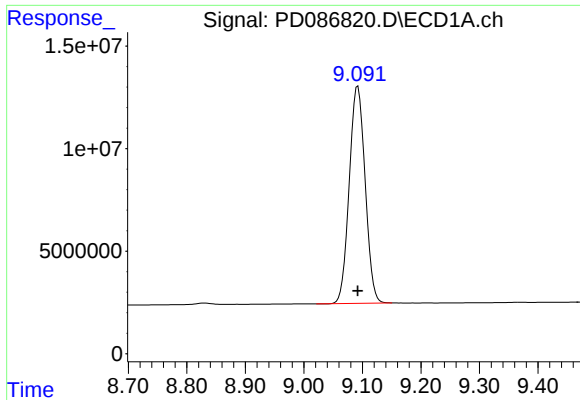

#27 Decachlorobiphenyl


R.T.: 9.092 min

Delta R.T.: 0.000 min

Response: 199511506

Conc: 75.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4016

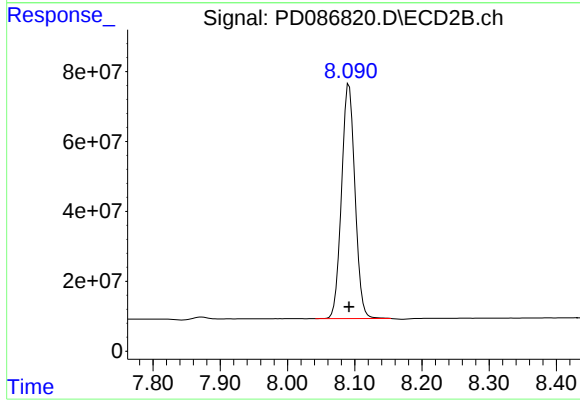

#27 Decachlorobiphenyl

R.T.: 8.091 min

Delta R.T.: 0.000 min

Response: 929890884

Conc: 73.23 ng/ml