

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
 Data File : PD086822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 23:39
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:43:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:36:31 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.885	140.1E6	805.6E6	76.957	70.387
27)	SA Decachlor...	9.093	8.091	388.7E6	1753.6E6	147.931	138.103
Target Compounds							
2)	A alpha-BHC	4.008	3.399	308.5E6	1319.9E6	89.289	73.957
3)	MA gamma-BHC...	4.340	3.736	296.1E6	1210.4E6	86.625	72.723
4)	MA Heptachlor	4.941	4.092	287.0E6	1204.9E6	84.056	70.443
9)	A Endosulfan I	6.087	5.259	236.9E6	1015.2E6	80.594	70.311
13)	MA Dieldrin	6.359	5.526	548.5E6	2165.4E6	169.028	141.985
14)	MA Endrin	6.587	5.802	451.8E6	1919.1E6	169.279	139.293
16)	A 4,4'-DDD	6.717	5.943	397.2E6	1720.5E6	169.456	142.855
17)	MA 4,4'-DDT	7.034	6.198	414.5E6	1850.3E6	169.094	143.169
20)	A Methoxychlor	7.506	6.771	1020.8E6	3593.3E6	756.872	618.694


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 23:39
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:43:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:36:31 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

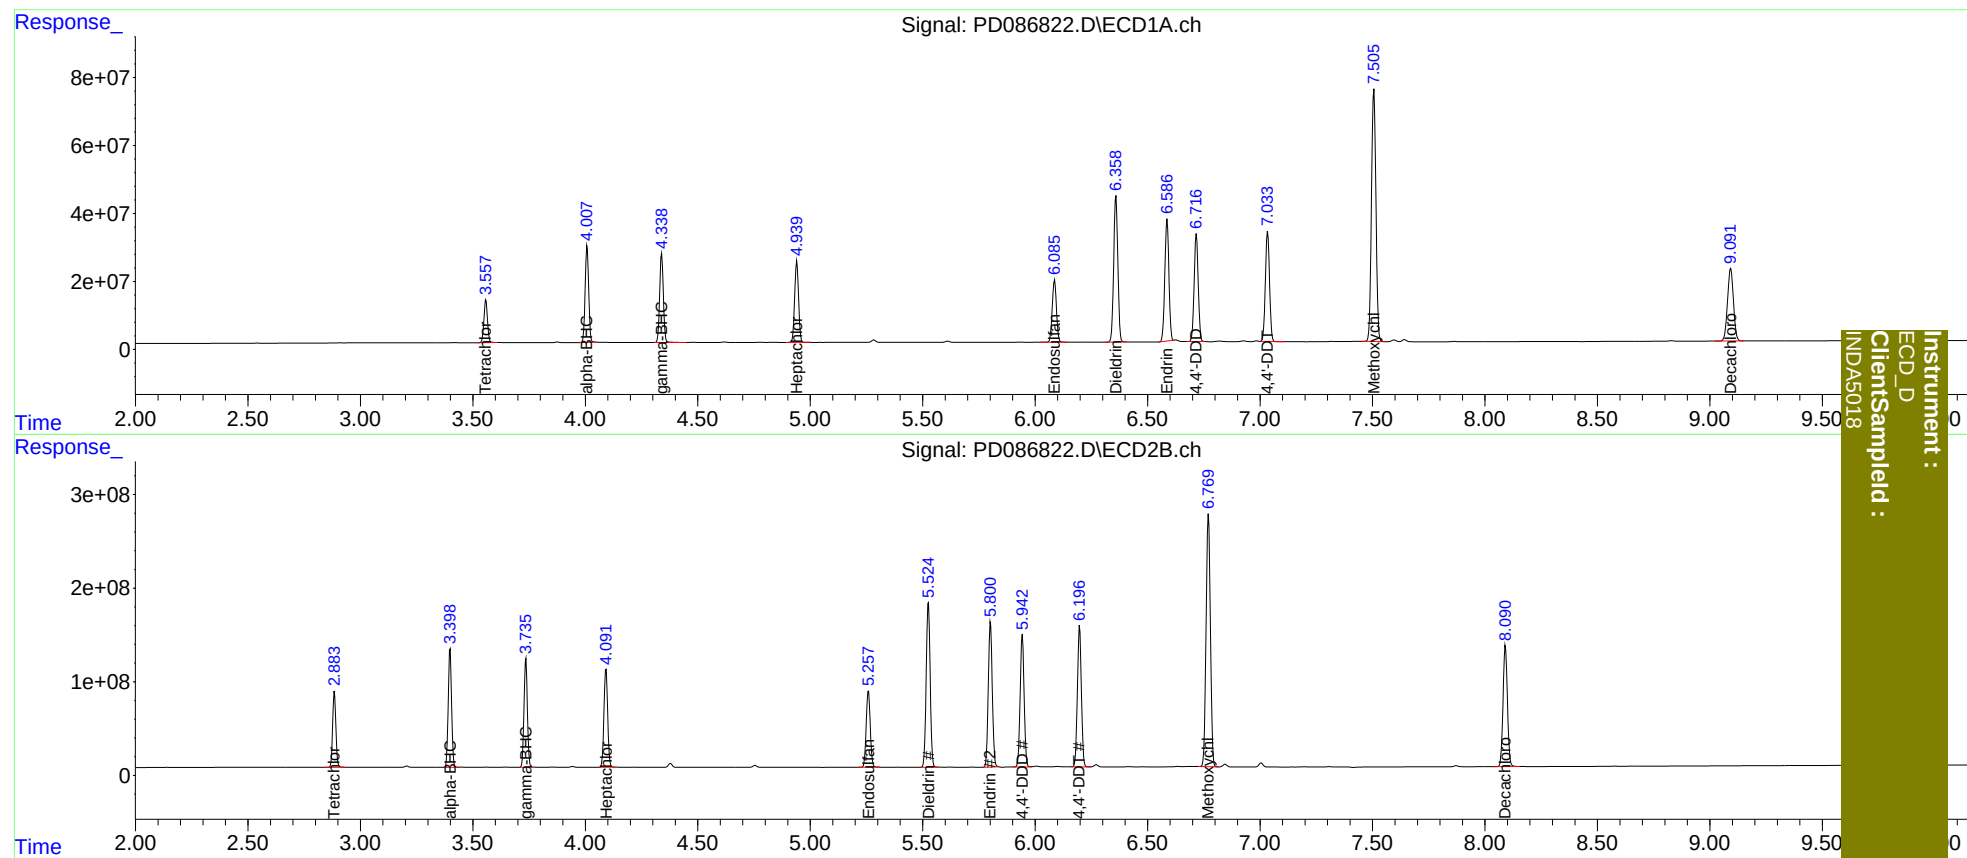


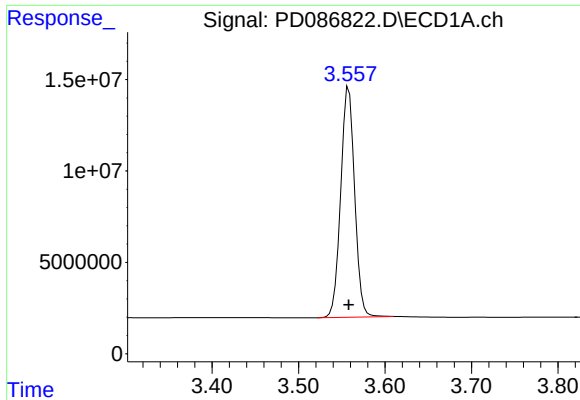

#1 Tetrachloro-m-xylene


R.T.: 3.558 min
Delta R.T.: 0.000 min
Response: 140074109
Conc: 76.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5018

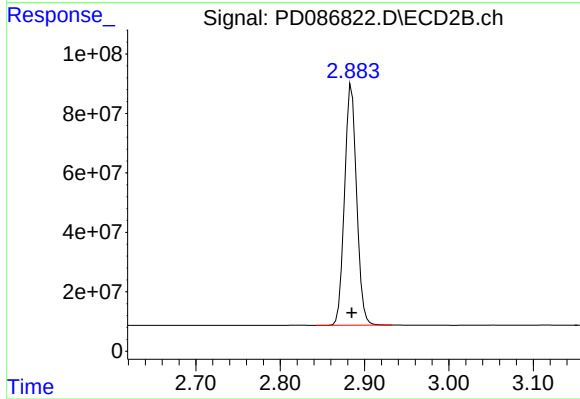


#1 Tetrachloro-m-xylene

R.T.: 2.885 min
Delta R.T.: 0.000 min
Response: 805609552
Conc: 70.39 ng/ml

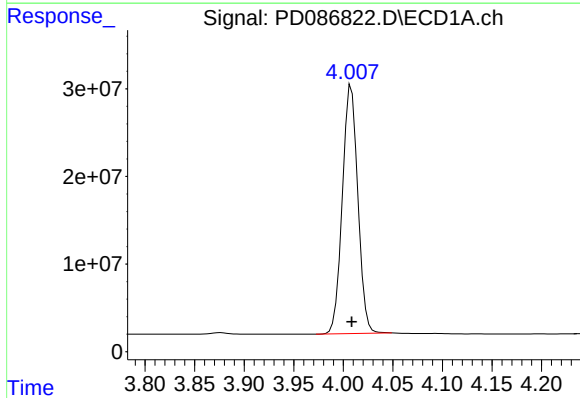


#2 alpha-BHC

R.T.: 4.008 min
Delta R.T.: 0.000 min
Response: 308502141
Conc: 89.29 ng/ml

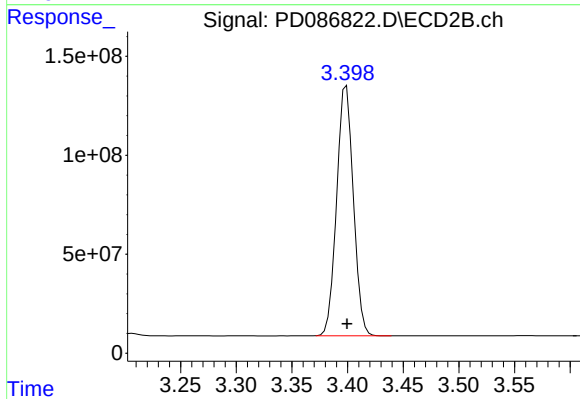

#2 alpha-BHC


R.T.: 3.399 min
Delta R.T.: 0.000 min
Response: 1319919882
Conc: 73.96 ng/ml

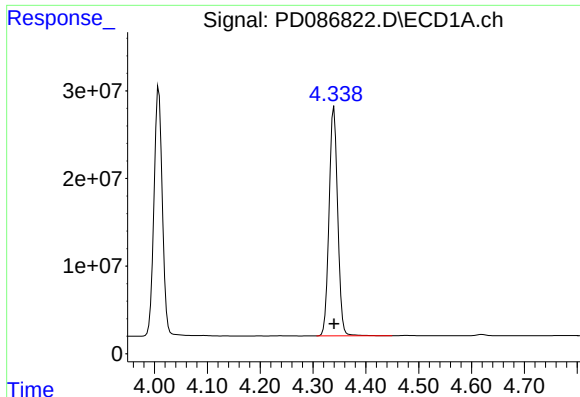

#3 gamma-BHC (Lindane)


R.T.: 4.340 min
Delta R.T.: 0.000 min
Response: 296136290
Conc: 86.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5018

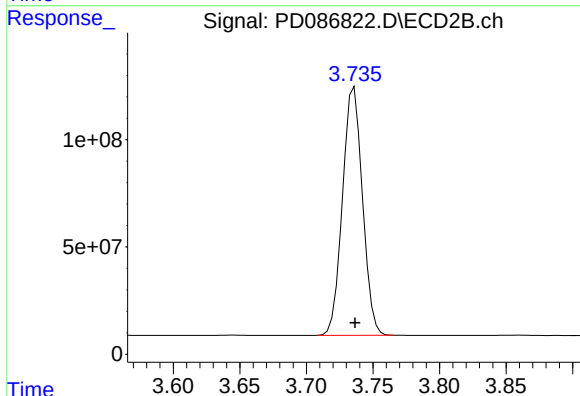


#3 gamma-BHC (Lindane)

R.T.: 3.736 min
Delta R.T.: 0.000 min
Response: 1210410358
Conc: 72.72 ng/ml

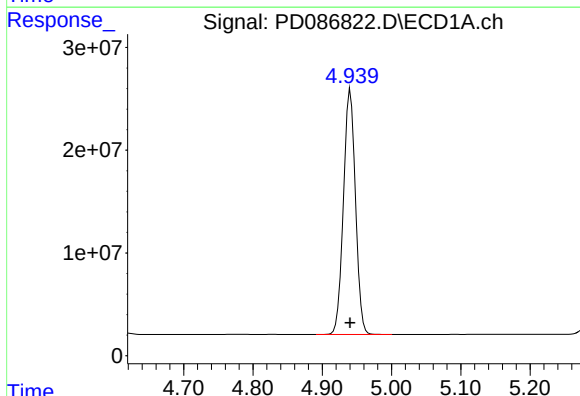


#4 Heptachlor

R.T.: 4.941 min
Delta R.T.: 0.000 min
Response: 286970817
Conc: 84.06 ng/ml

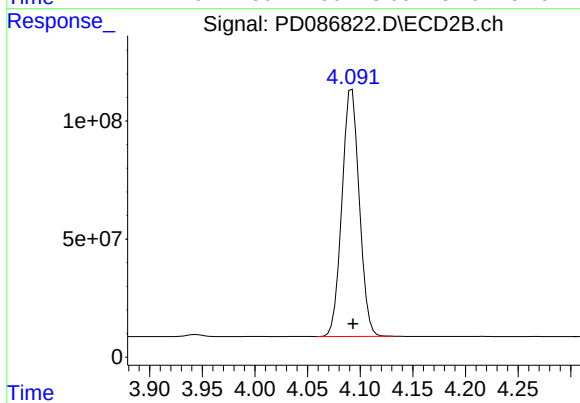

#4 Heptachlor


R.T.: 4.092 min
Delta R.T.: -0.001 min
Response: 1204885014
Conc: 70.44 ng/ml

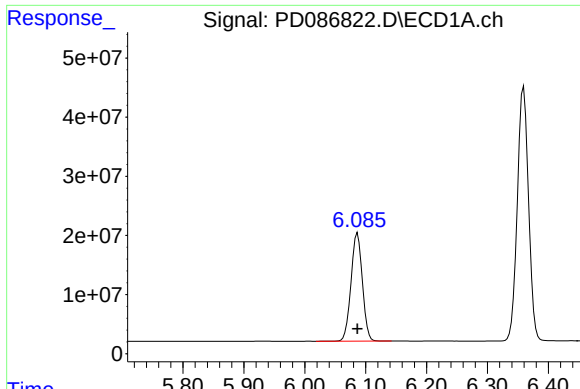

#9 Endosulfan I


R.T.: 6.087 min
Delta R.T.: 0.000 min
Response: 236850610
Conc: 80.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5018

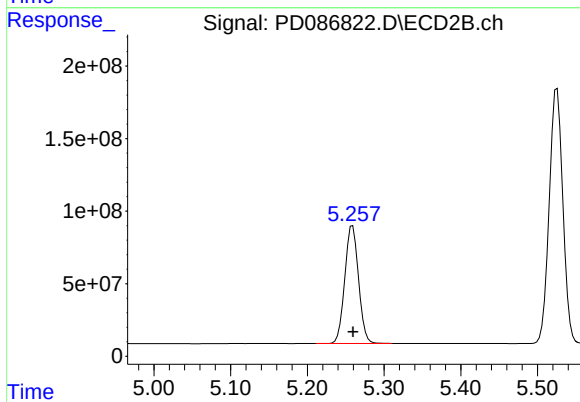


#9 Endosulfan I

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 1015153299
Conc: 70.31 ng/ml

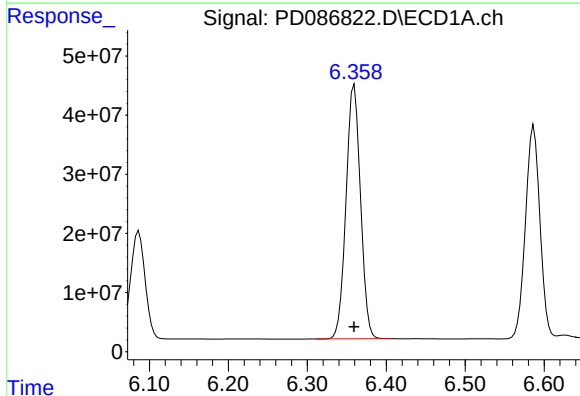


#13 Dieldrin

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 548491951
Conc: 169.03 ng/ml

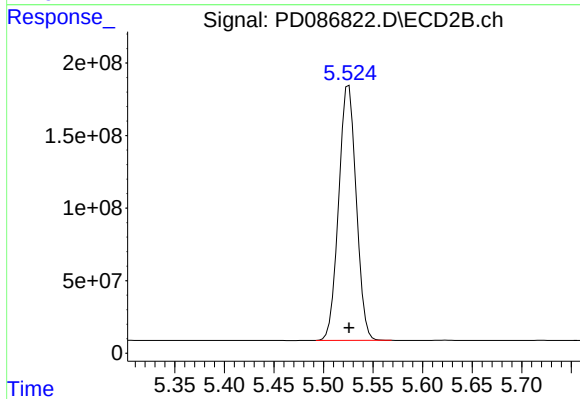

#13 Dieldrin


R.T.: 5.526 min
Delta R.T.: 0.000 min
Response: 2165364920
Conc: 141.99 ng/ml

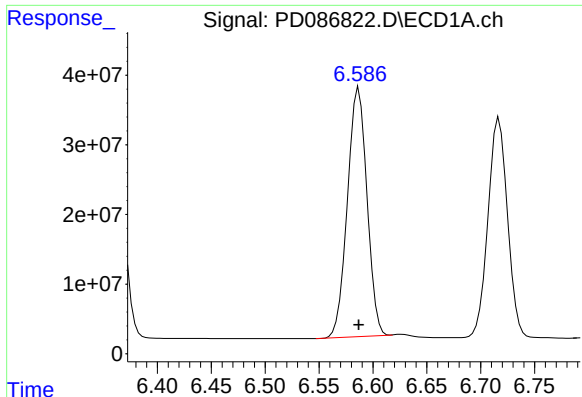

#14 Endrin


R.T.: 6.587 min
Delta R.T.: 0.000 min
Response: 451783368
Conc: 169.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5018

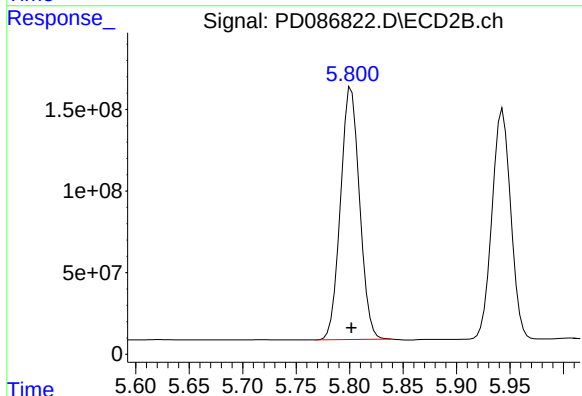


#14 Endrin

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 1919080893
Conc: 139.29 ng/ml

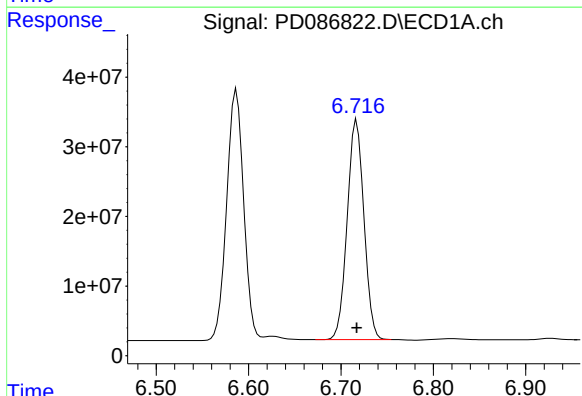


#16 4,4'-DDD

R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 397209250
Conc: 169.46 ng/ml

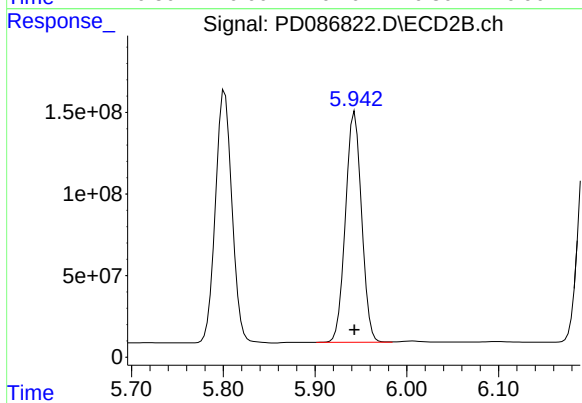

#16 4,4'-DDD


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 1720531265
Conc: 142.85 ng/ml

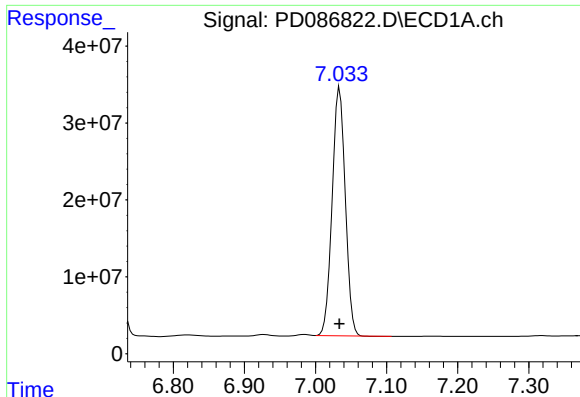

#17 4,4'-DDT


R.T.: 7.034 min
Delta R.T.: 0.000 min
Response: 414525096
Conc: 169.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5018

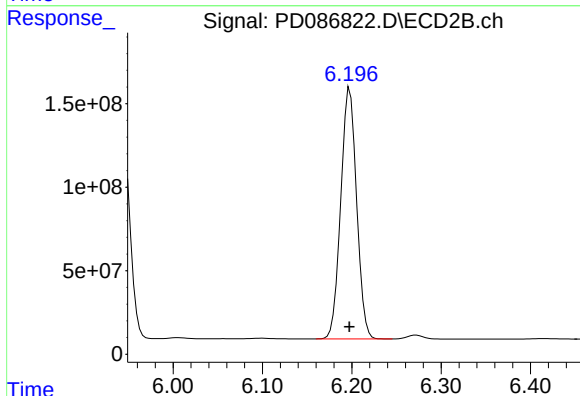


#17 4,4'-DDT

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 1850281591
Conc: 143.17 ng/ml

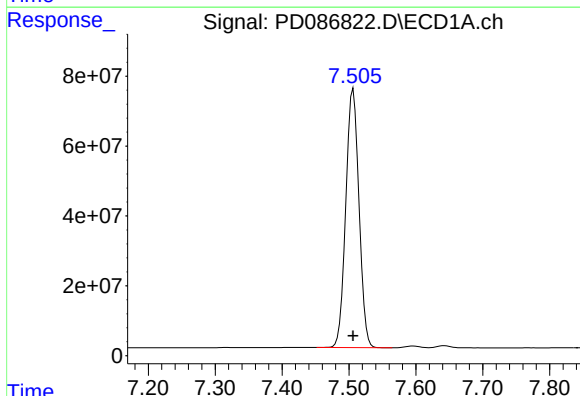


#20 Methoxychlor

R.T.: 7.506 min
Delta R.T.: 0.000 min
Response: 1020803458
Conc: 756.87 ng/ml

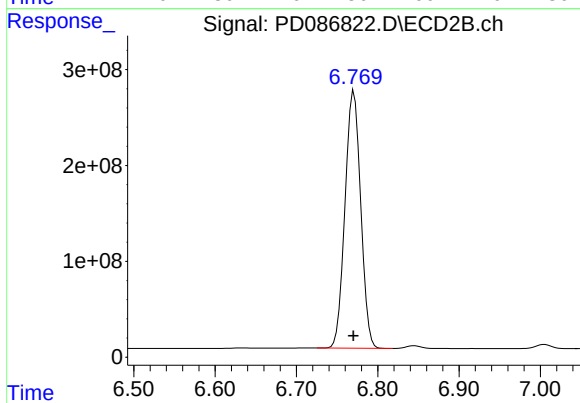

#20 Methoxychlor

R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 3593289285
Conc: 618.69 ng/ml

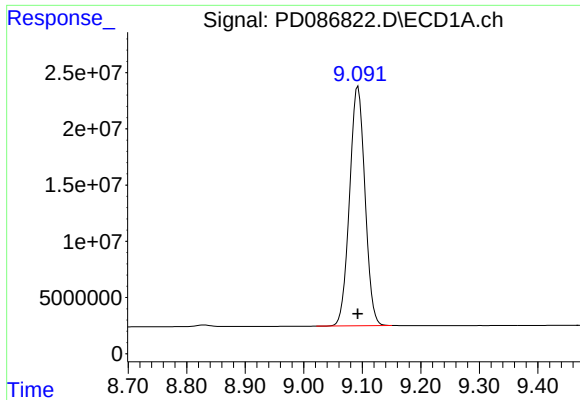

#27 Decachlorobiphenyl


R.T.: 9.093 min

Delta R.T.: 0.000 min

Response: 388696579

Conc: 147.93 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5018

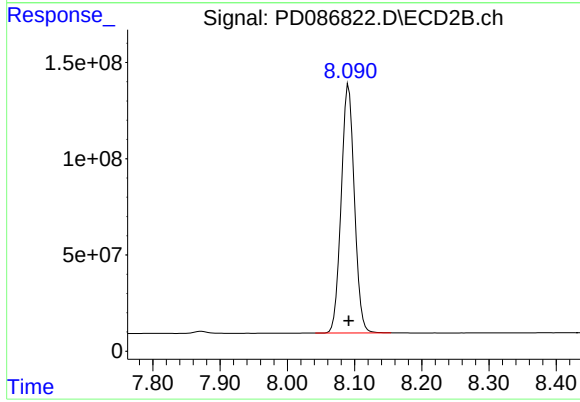

#27 Decachlorobiphenyl

R.T.: 8.091 min

Delta R.T.: 0.000 min

Response: 1753556406

Conc: 138.10 ng/ml