

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
 Data File : PD086830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 01:32
 Operator : AR\AJ
 Sample : P4847-05MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AT5MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :Ankita Jodhani 11/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:23:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.885	35897143	223.5E6	19.521	19.362
27)	SA Decachlor...	9.092	8.093	31392570	295.2E6	11.790	23.160 #
Target Compounds							
2)	A alpha-BHC	4.009	3.400	156.0E6	726.0E6	44.314	40.536
3)	MA gamma-BHC...	4.340	3.737	157.6E6	673.8E6	45.258	40.400
4)	MA Heptachlor	4.941	4.093	152.9E6	659.5E6	44.006	38.341
5)	MB Aldrin	5.283	4.379	149.2E6	616.5E6	42.247	36.091
6)	B beta-BHC	4.524	4.032	59425674	275.8E6	37.488	34.914
7)	B delta-BHC	4.773	4.270	102.6E6	454.9E6	28.196	25.906
8)	B Heptachlo...	5.703	4.884	135.3E6	606.9E6	41.404	38.271
9)	A Endosulfan I	6.085	5.258	128.6E6	548.2E6	43.242m	37.876m
10)	B trans-Chl...	5.958	5.138	133.0E6	603.0E6	41.586	36.508
11)	B cis-Chlor...	6.038	5.201	138.3E6	602.5E6	42.514m	37.597m
12)	B 4,4'-DDE	6.208	5.389	259.9E6	1145.0E6	84.275	75.097
13)	MA Dieldrin	6.360	5.526	292.5E6	1191.9E6	89.239	78.008
14)	MA Endrin	6.587	5.802	246.8E6	1103.8E6	91.305	79.902
15)	B Endosulfa...	6.799	6.094	234.6E6	1017.9E6	84.540	72.945
16)	A 4,4'-DDD	6.718	5.944	208.8E6	805.2E6	87.995	66.652
17)	MA 4,4'-DDT	7.033	6.197	219.7E6	978.2E6	88.647m	75.658m
18)	B Endrin al...	6.928	6.272	162.2E6	709.4E6	73.800	66.105
19)	B Endosulfa...	7.161	6.496	214.8E6	944.0E6	79.601	70.350
20)	A Methoxychlor	7.507	6.770	575.0E6	2142.5E6	426.025	370.582
21)	B Endrin ke...	7.644	7.005	257.6E6	1092.6E6	84.466	73.119

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 01:32
Operator : AR\AJ
Sample : P4847-05MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:23:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

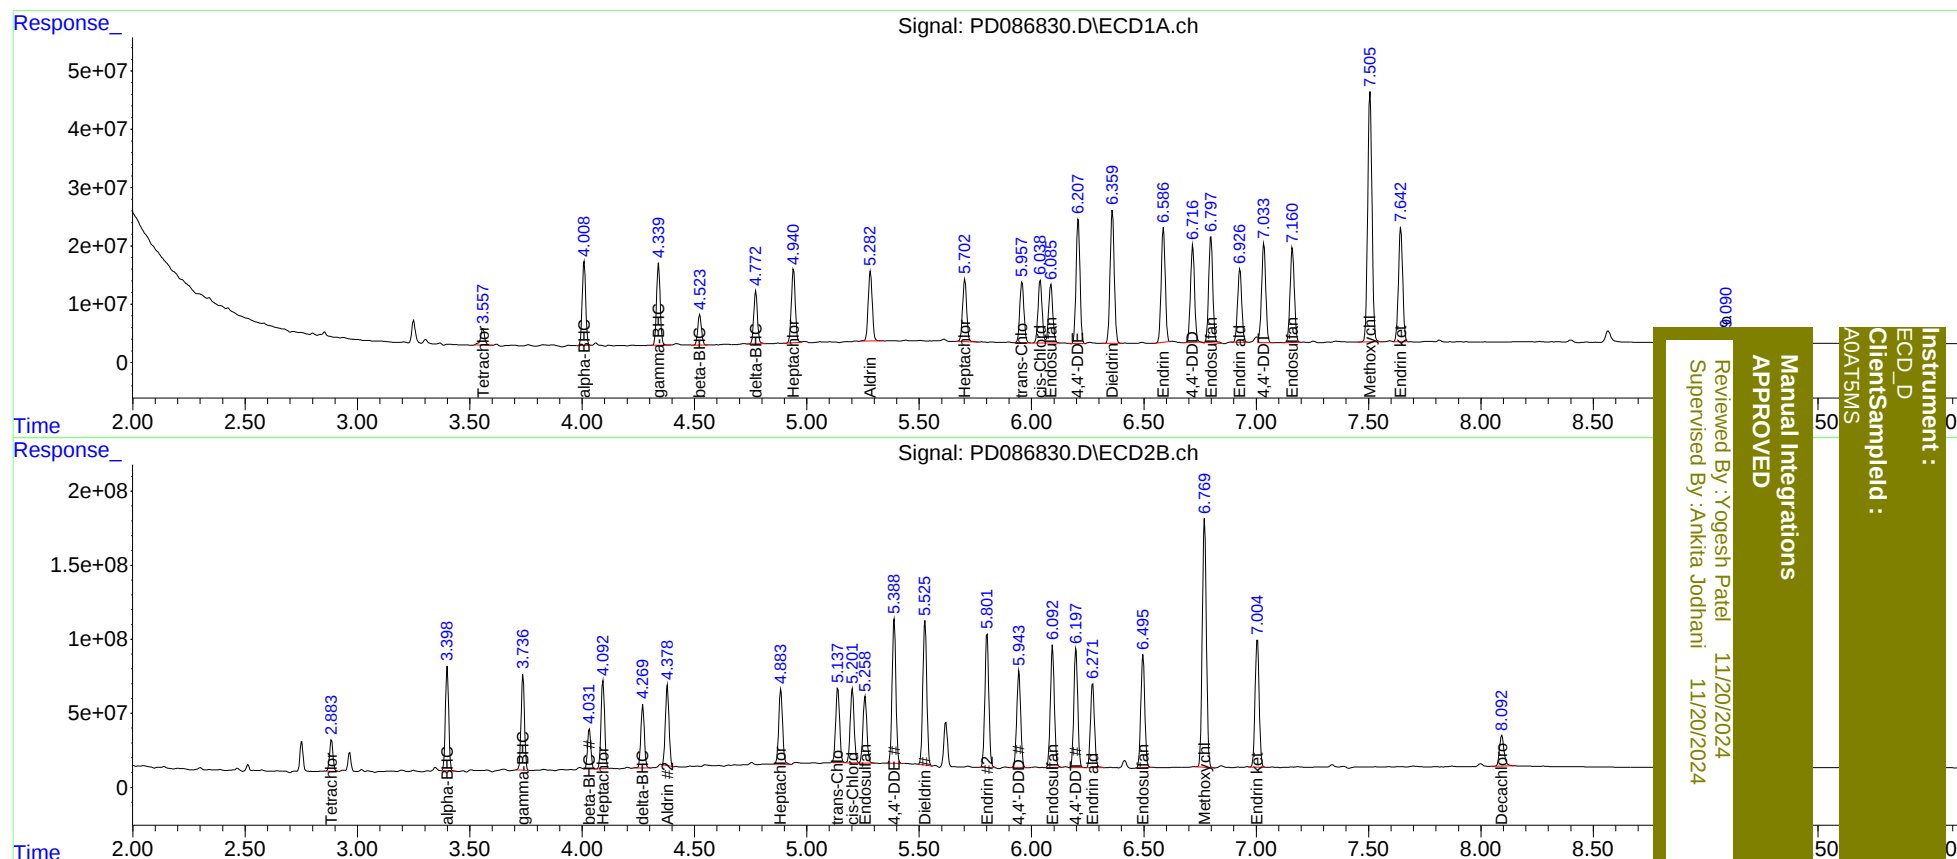

Instrument :
ECD_D
ClientSampled :
A0AT5MS

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/20/2024
Supervised By : Ankita Jodhani 11/20/2024