

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
 Data File : PD086807.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 20:09
 Operator : AR\AJ
 Sample : RESC053
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESC008

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:58:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.885	40171006	252.2E6	21.845	21.853
27)	SA Decachlor...	9.092	8.093	114.7E6	549.4E6	43.074	43.105
Target Compounds							
2)	A alpha-BHC	4.008	3.399	37460222	207.5E6	10.639	11.583
3)	MA gamma-BHC...	4.339	3.737	37593320	193.5E6	10.795	11.601
4)	MA Heptachlor	4.940	4.092	38216050	200.5E6	10.998	11.658
5)	MB Aldrin	5.283	4.379	36584477	188.8E6	10.361	11.054
6)	B beta-BHC	4.523	4.032	16603334	80838263	10.474	10.233
7)	B delta-BHC	4.772	4.270	36903995	187.9E6	10.140	10.702
8)	B Heptachlo...	5.702	4.884	33351318	171.2E6	10.204	10.794
9)	A Endosulfan I	6.086	5.259	30216673	120.8E6	10.163	8.344
10)	B trans-Chl...	5.957	5.138	32725912	176.3E6	10.232	10.676
11)	B cis-Chlor...	6.039	5.202	30589844	80611711	9.403	5.030 #
12)	B 4,4'-DDE	6.207	5.389	60865929	326.4E6	19.734	21.406
13)	MA Dieldrin	6.359	5.526	71842394	357.7E6	21.917	23.415
14)	MA Endrin	6.587	5.802	59270435	323.5E6	21.927	23.418
15)	B Endosulfa...	6.797	6.094	58755128	302.8E6	21.175	21.701
16)	A 4,4'-DDD	6.717	5.943	51914592	289.8E6	21.883	23.988
17)	MA 4,4'-DDT	7.034	6.199	56214958	303.2E6	22.679	23.453
18)	B Endrin al...	6.927	6.273	46019220	237.9E6	20.937	22.167
19)	B Endosulfa...	7.161	6.497	55626911	294.3E6	20.619	21.930
20)	A Methoxychlor	7.506	6.771	155.7E6	704.5E6	115.340	121.848
21)	B Endrin ke...	7.643	7.006	63320379	333.6E6	20.759	22.325

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 20:09
Operator : AR\AJ
Sample : RESC053
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:58:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

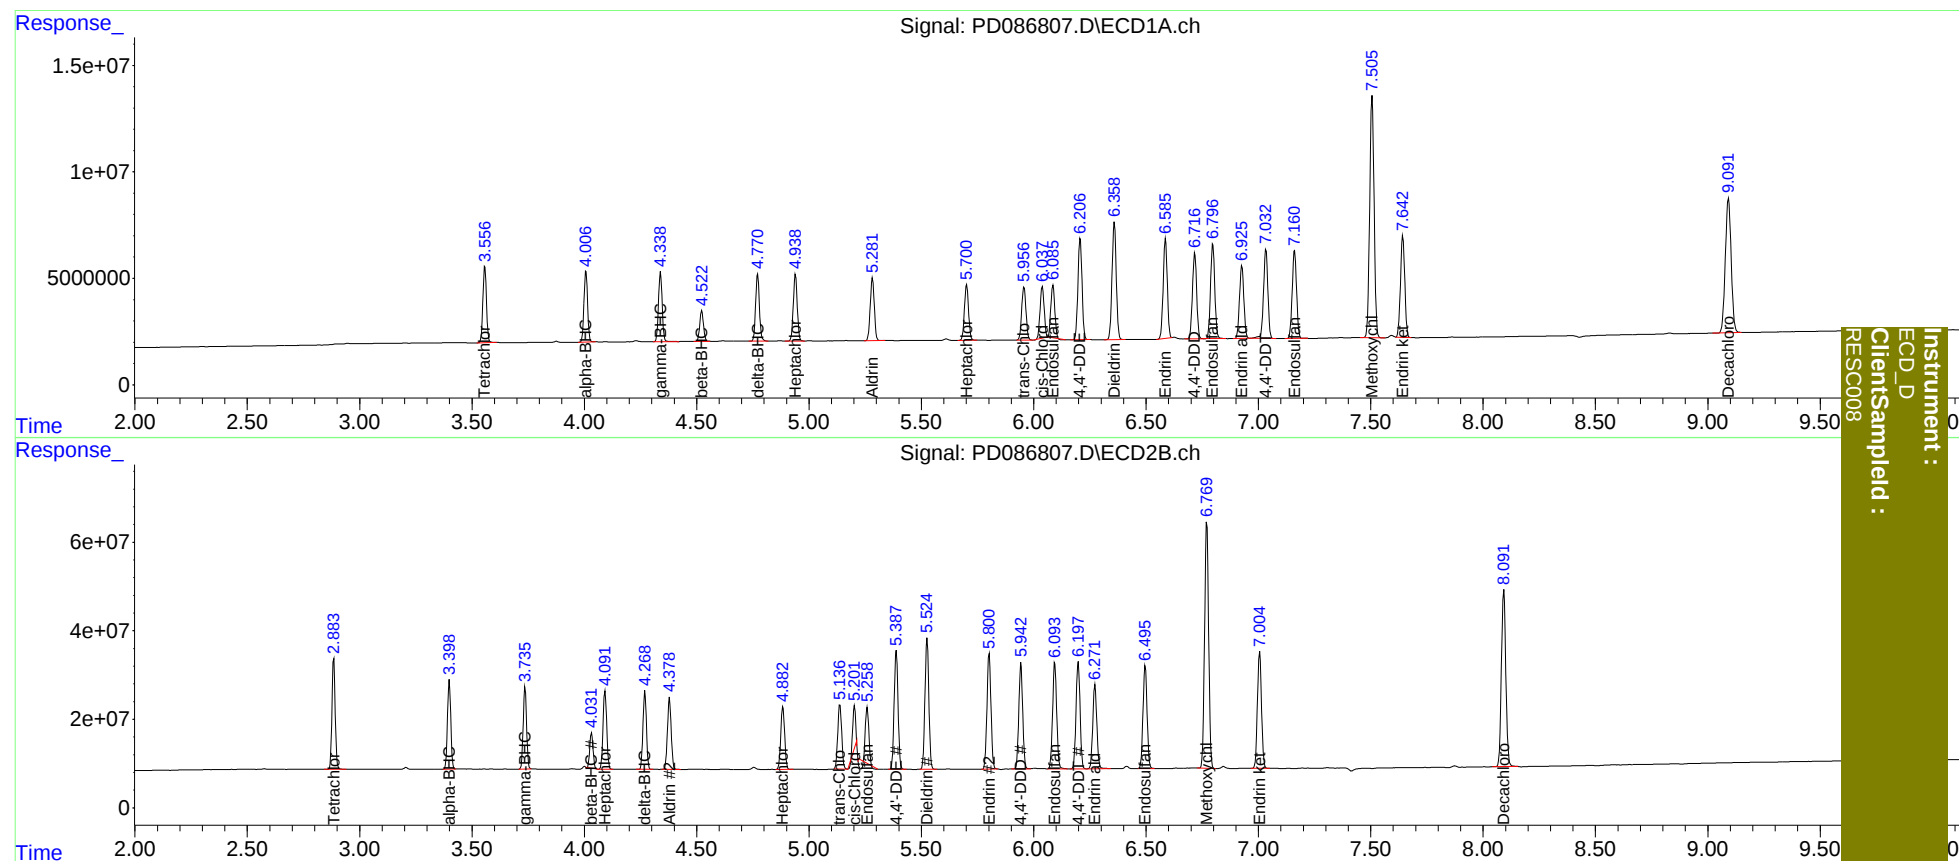

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086807.D
Acq On : 19 Nov 2024 20:09
Operator : AR\AJ
Sample : RESC053
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Title : GC Extractables
Last Update : Wed Nov 20 02:52:29 2024
Integrator: ChemStation

RT#1	RT#2	Resolution
3.558	4.008	100.00%
4.008	4.339	100.00%
4.339	4.523	100.00%
4.523	4.772	100.00%
4.772	4.940	100.00%
4.940	5.283	100.00%
5.283	5.702	100.00%
5.702	5.957	100.00%
5.957	6.039	100.00%
6.039	6.086	95.69%
6.086	6.207	100.00%
6.207	6.359	100.00%
6.359	6.587	100.00%
6.587	6.717	100.00%
6.717	6.797	100.00%
6.797	6.927	100.00%
6.927	7.034	100.00%
7.034	7.161	100.00%
7.161	7.506	100.00%
7.506	7.643	100.00%
7.643	9.092	100.00%

Signal #2


2.885	3.399	100.00%
3.399	3.737	100.00%
3.737	4.032	100.00%
4.032	4.092	100.00%
4.092	4.270	100.00%
4.270	4.379	100.00%
4.379	4.884	100.00%
4.884	5.138	100.00%
5.138	5.202	100.00%
5.202	5.259	100.00%
5.259	5.389	100.00%
5.389	5.526	100.00%
5.526	5.802	100.00%
5.802	5.943	100.00%
5.943	6.094	100.00%
6.094	6.199	100.00%
6.199	6.273	100.00%
6.273	6.497	100.00%
6.497	6.771	100.00%
6.771	7.006	100.00%
7.006	8.093	100.00%

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086807.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 20:09
Operator : AR\AJ
Sample : RESC053
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESC008

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:58:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

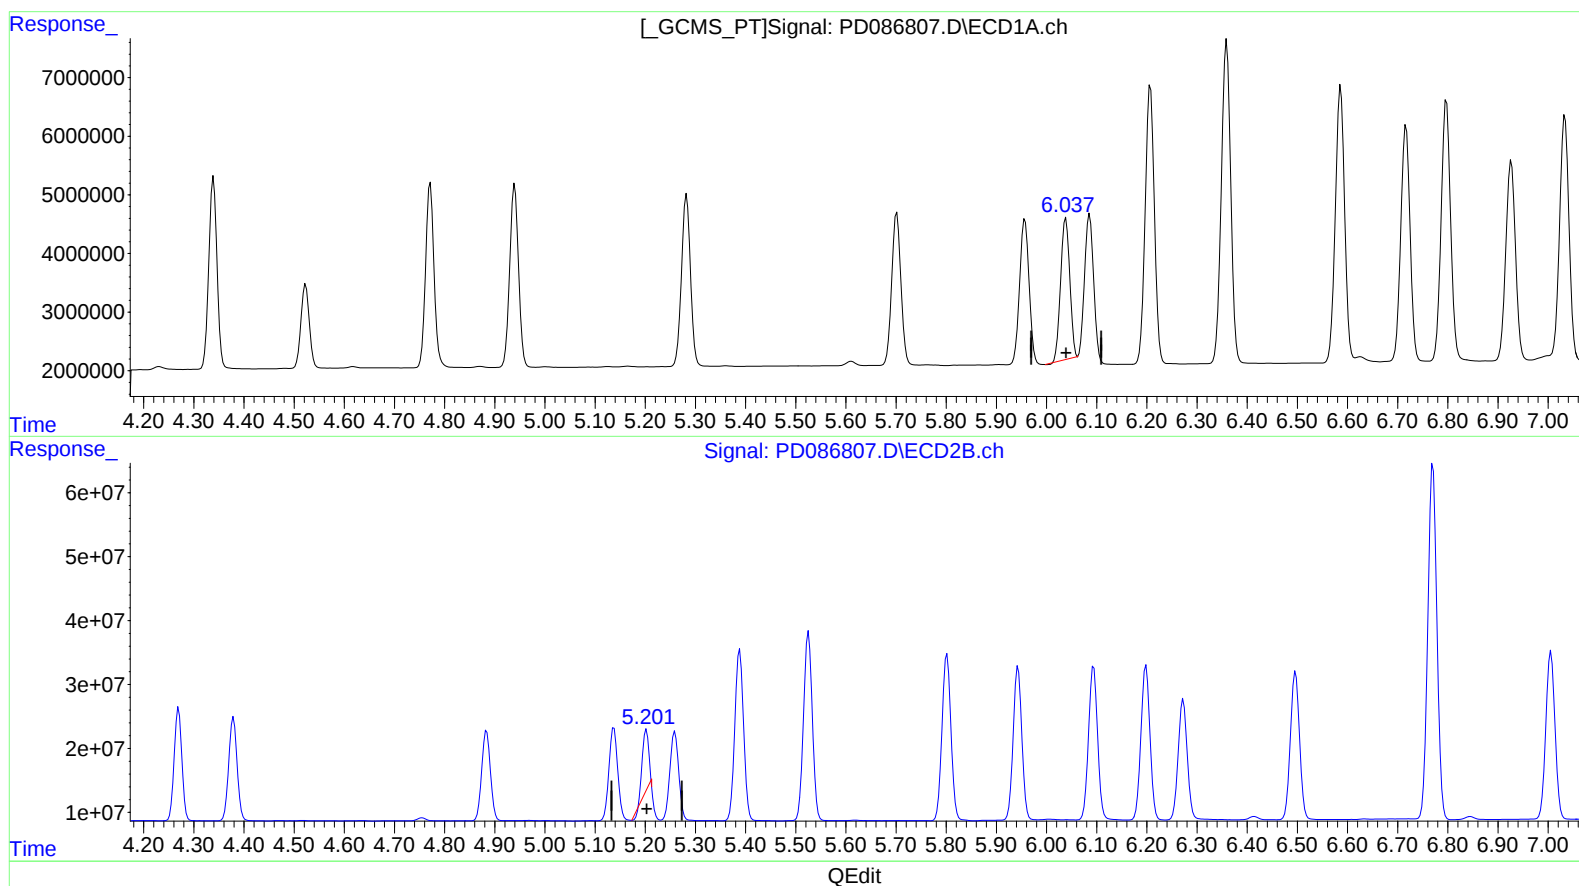

(11) cis-Chlordane (B)

6.039min 9.403 ng/ml

response 30589844

(11) cis-Chlordane #2 (B)

5.202min 5.030 ng/ml

response 80611711