

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
 Data File : PD086831.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 01:46
 Operator : AR\AJ
 Sample : P4847-06MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AT5MSD

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2024
 Supervised By :Ankita Jodhani 11/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:24:11 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.884	36246129	225.7E6	19.710	19.559
2)	SA Decachlor...	9.093	8.093	31671234	301.2E6	11.895	23.632 #
Target Compounds							
2)	A alpha-BHC	4.009	3.399	156.6E6	728.6E6	44.485	40.678
3)	MA gamma-BHC...	4.340	3.737	158.3E6	677.2E6	45.463	40.601
4)	MA Heptachlor	4.941	4.093	153.5E6	660.8E6	44.182	38.416
5)	MB Aldrin	5.283	4.379	149.6E6	617.2E6	42.370	36.130
6)	B beta-BHC	4.524	4.032	59454196	276.1E6	37.506	34.945
7)	B delta-BHC	4.772	4.269	102.8E6	456.2E6	28.243	25.980
8)	B Heptachlo...	5.703	4.884	135.3E6	606.5E6	41.380	38.243
9)	A Endosulfan I	6.085	5.258	128.7E6	542.2E6	43.271m	37.460m
10)	B trans-Chl...	5.958	5.138	132.5E6	603.0E6	41.420	36.508
11)	B cis-Chlor...	6.038	5.201	137.6E6	597.9E6	42.286m	37.311m
12)	B 4,4'-DDE	6.208	5.388	259.0E6	1141.0E6	83.972	74.831
13)	MA Dieldrin	6.360	5.525	292.7E6	1188.2E6	89.280	77.766
14)	MA Endrin	6.587	5.802	246.6E6	1105.0E6	91.213	79.987
15)	B Endosulfa...	6.799	6.093	232.2E6	1013.7E6	83.683	72.648
16)	A 4,4'-DDD	6.717	5.943	207.8E6	798.4E6	87.599	66.083
17)	MA 4,4'-DDT	7.032	6.197	220.1E6	971.8E6	88.813m	75.166
18)	B Endrin al...	6.927	6.271	161.6E6	704.2E6	73.527	65.622
19)	B Endosulfa...	7.162	6.495	214.5E6	940.1E6	79.507	70.060
20)	A Methoxychlor	7.507	6.770	575.5E6	2144.2E6	426.346	370.877
21)	B Endrin ke...	7.643	7.005	257.3E6	1086.2E6	84.347	72.696

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112024\
Data File : PD086831.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 01:46
Operator : AR\AJ
Sample : P4847-06MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:24:11 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

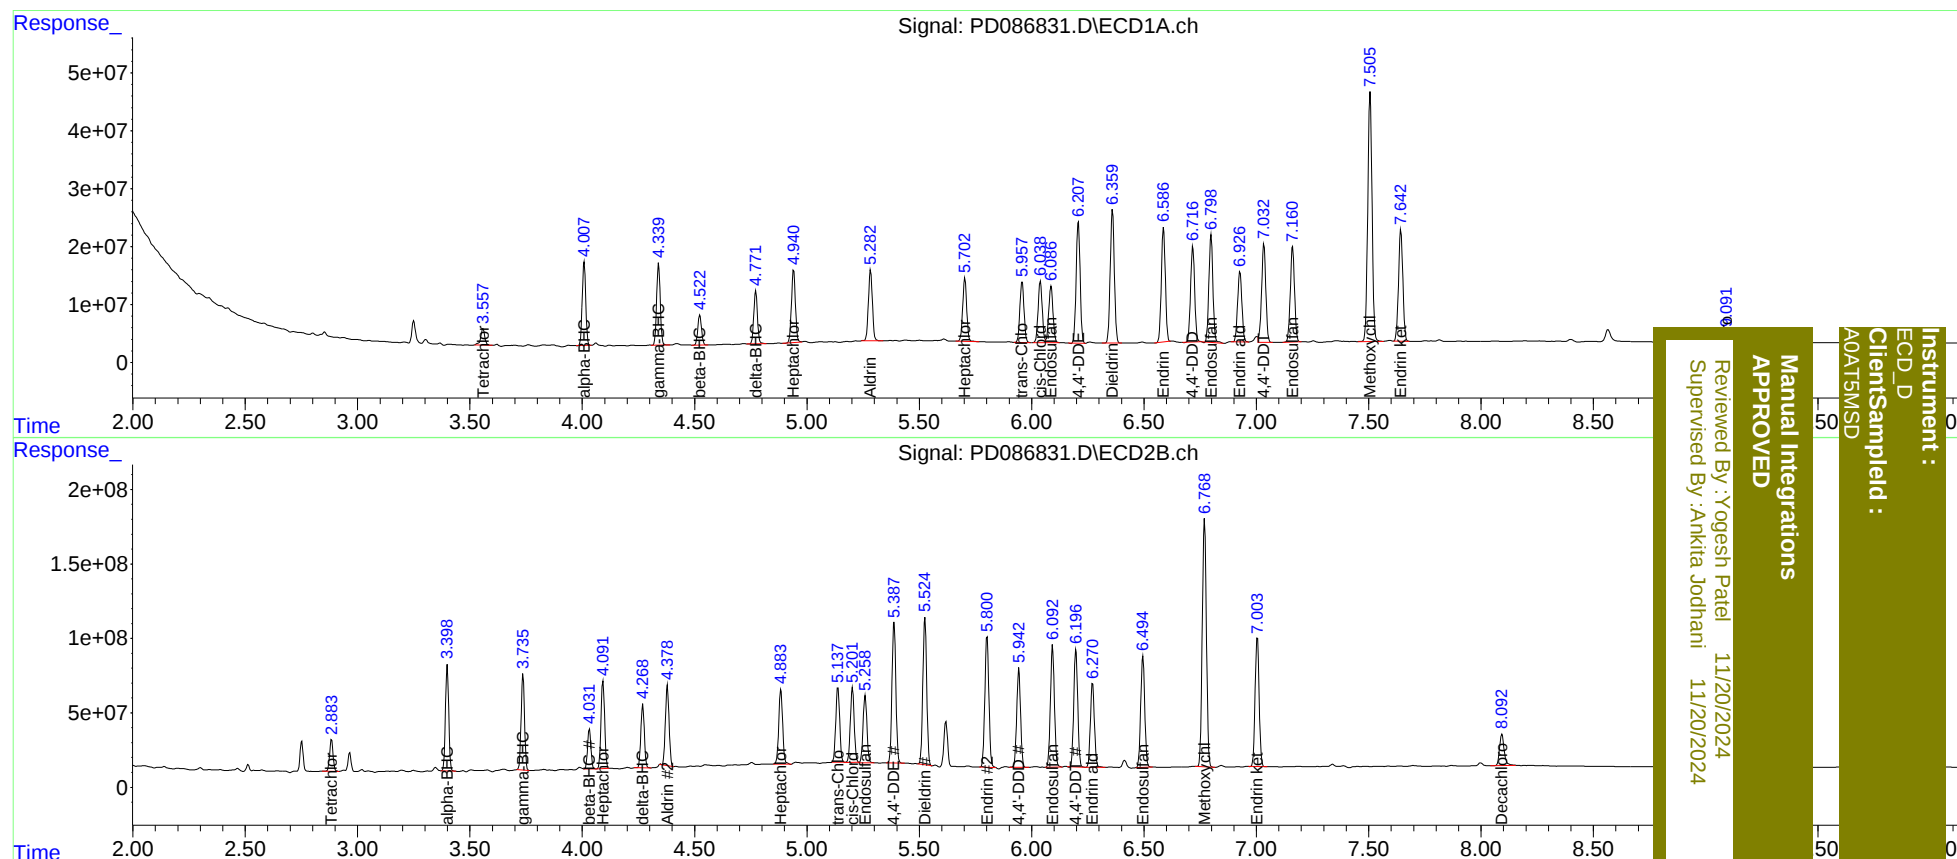

Instrument :
ECD_D
Client Sampled :
A0AT5MSD

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/20/2024
Supervised By : Ankita Jodhani 11/20/2024