

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112120\
 Data File : PD060202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2020 11:39
 Operator : DD\AJ
 Sample : L4749-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B73

Manual Integrations
 APPROVED

mohammad
 11/23/2020 1:50:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 08:06:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.023	8825985	22905495	10.299	7.684 #
27) SA Decachlor...	8.299	9.107	10353644	29307332	12.461	11.913
Target Compounds						
10) B trans-Chl...	5.467	6.138	4543075	28620617	4.277m	8.330m#
11) B cis-Chlor...	5.523	6.212	14836577	115.8E6	14.025m	33.730m#
12) B 4,4'-DDE	5.687	6.364	2356627	11635809	2.306m	3.599 #
17) MA 4,4'-DDT	6.450	7.154	2594641	4547206	2.887m	1.671m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112120\
Data File : PD060202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2020 11:39
Operator : DD\AJ
Sample : L4749-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 08:06:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

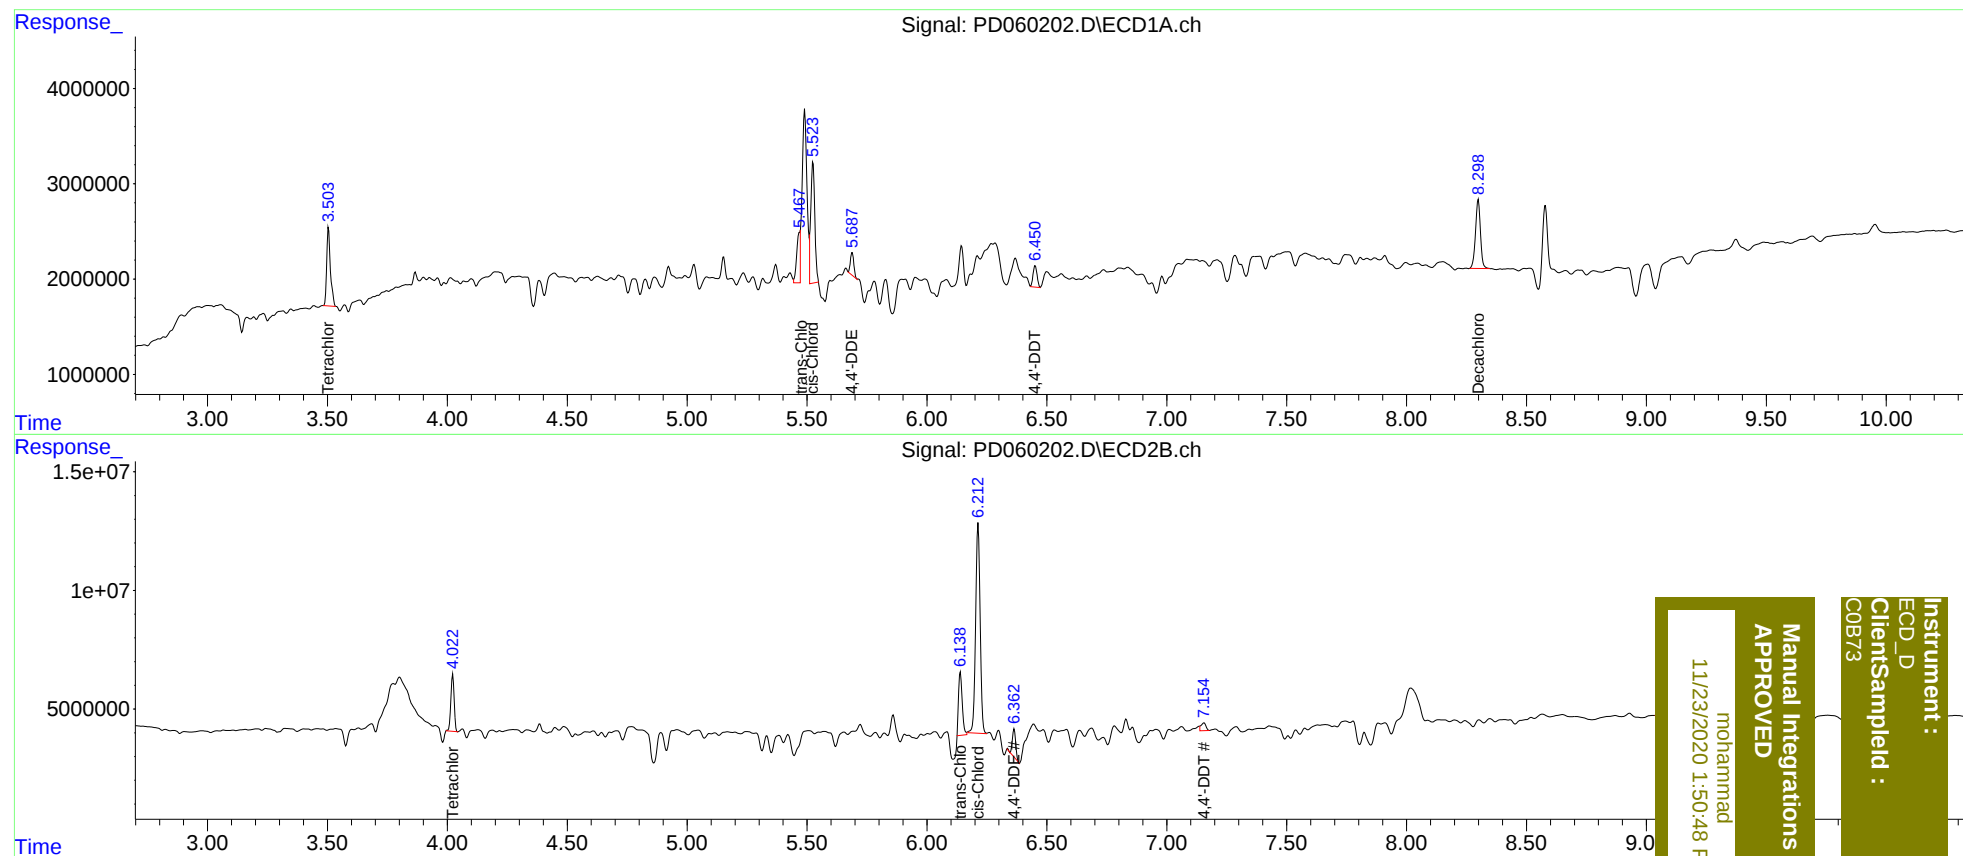

11/23/2020 1:50:48 PM
mohammad

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
C0873