

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112122\
 Data File : PD073160.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2022 12:33
 Operator : AR\AJ
 Sample : PB148453BL
 Misc : BL WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB148453BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 23:46:59 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 03:26:54 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	2.702	3.458	39222844	1103.9E6	18.483	19.925
28)	SA Decachlor...	7.828	8.908	41842501	272.3E6	20.314	21.306

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112122\
Data File : PD073160.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2022 12:33
Operator : AR\AJ
Sample : PB148453BL
Misc : BL WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB148453BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 23:46:59 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111622.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 03:26:54 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

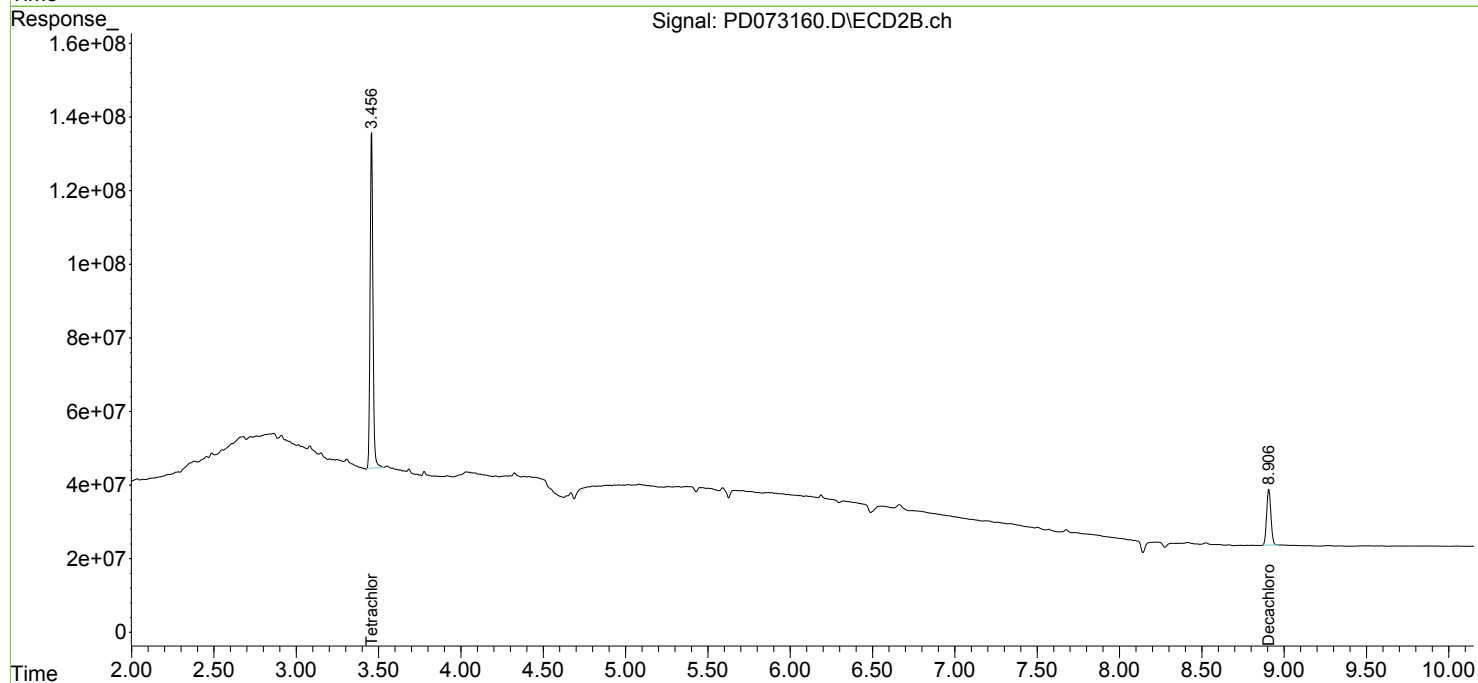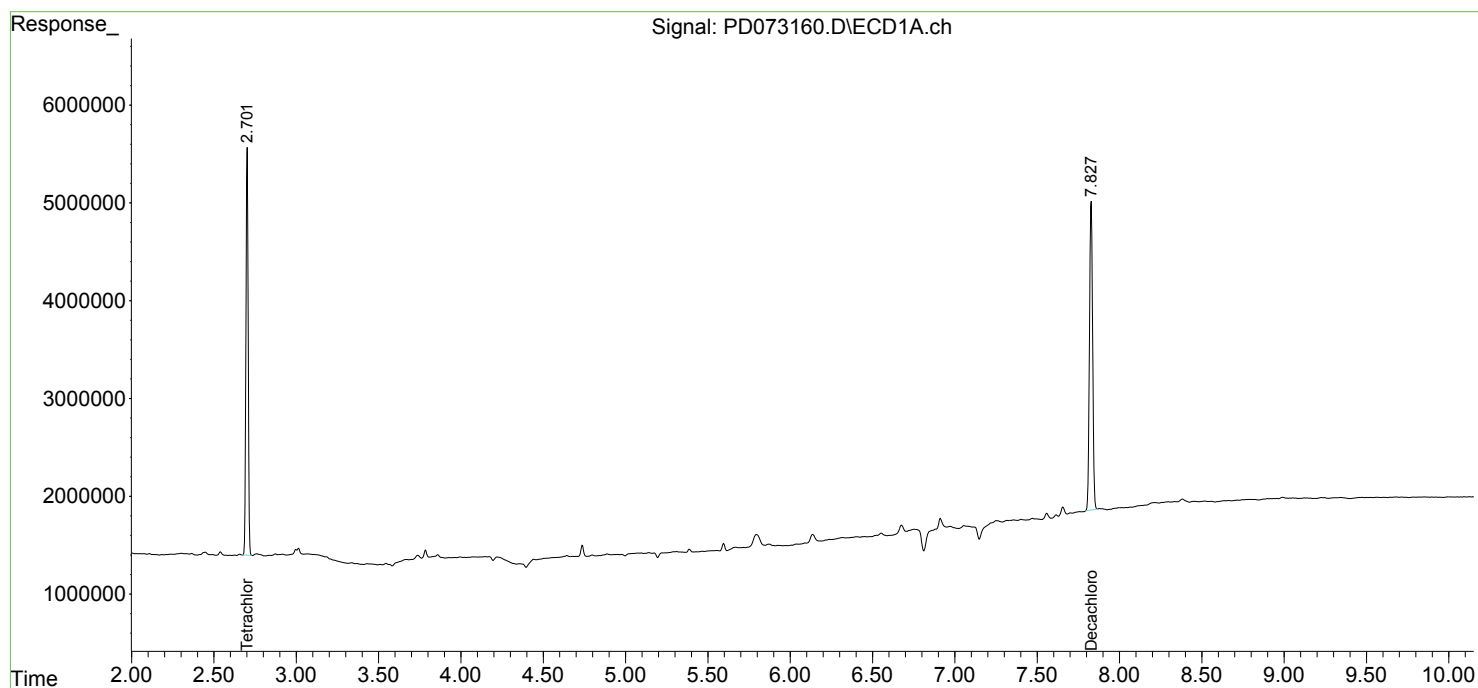


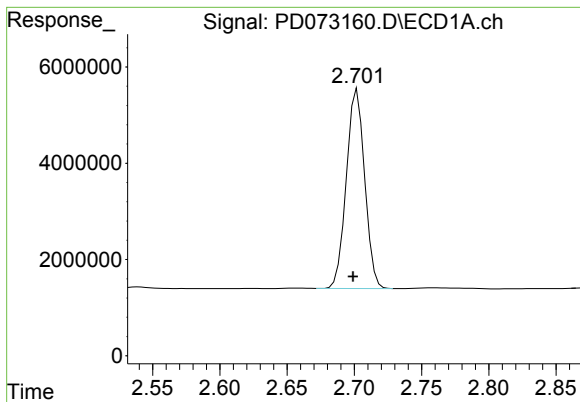

#1 Tetrachloro-m-xylene


R.T.: 2.702 min
Delta R.T.: 0.003 min
Response: 39222844
Conc: 18.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB148453BL

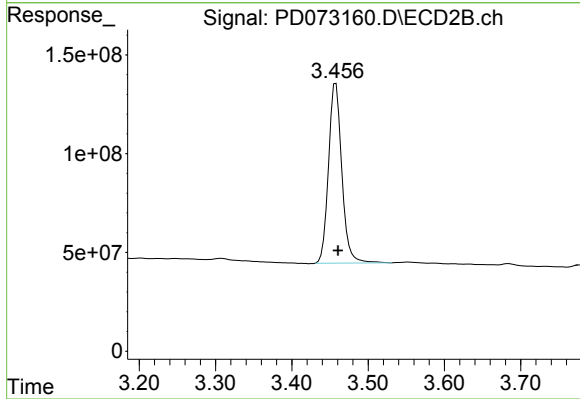


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: -0.003 min
Response: 1103869794
Conc: 19.93 ng/ml

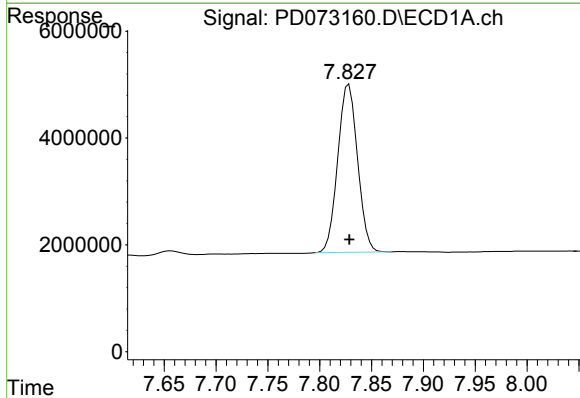

#28 Decachlorobiphenyl

R.T.: 7.828 min
Delta R.T.: 0.000 min
Response: 41842501
Conc: 20.31 ng/ml

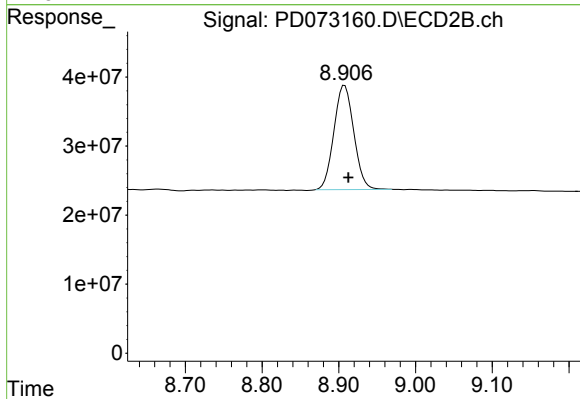

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: -0.005 min
Response: 272319543
Conc: 21.31 ng/ml