

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
 Data File : PD079769.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 18:08
 Operator : AR\AJ
 Sample : 05439-12
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 20:21:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	28696248	45308753	19.650	19.809
27)	SA Decachlor...	9.113	7.946	37938646	51249827	21.379	21.466
Target Compounds							
3)	MA gamma-BHC...	0.000	3.657	0	348541	N.D.	0.101
4)	MA Heptachlor	0.000	4.021f	0	186055	N.D.	<MDL
14)	MA Endrin	0.000	5.688	0	101783	N.D.	<MDL
15)	B Endosulfa...	0.000	5.921f	0	509717	N.D.	0.196
16)	A 4,4'-DDD	0.000	5.859f	0	68856	N.D.	<MDL
17)	MA 4,4'-DDT	0.000	6.082	0	255955	N.D.	0.107
18)	B Endrin al...	0.000	6.082f	0	255955	N.D.	0.126
19)	B Endosulfa...	0.000	6.414f	0	262807	N.D.	0.106
21)	B Endrin ke...	0.000	6.832f	0	90515	N.D.	<MDL


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
Data File : PD079769.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 18:08
Operator : AR\AJ
Sample : 05439-12
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 20:21:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

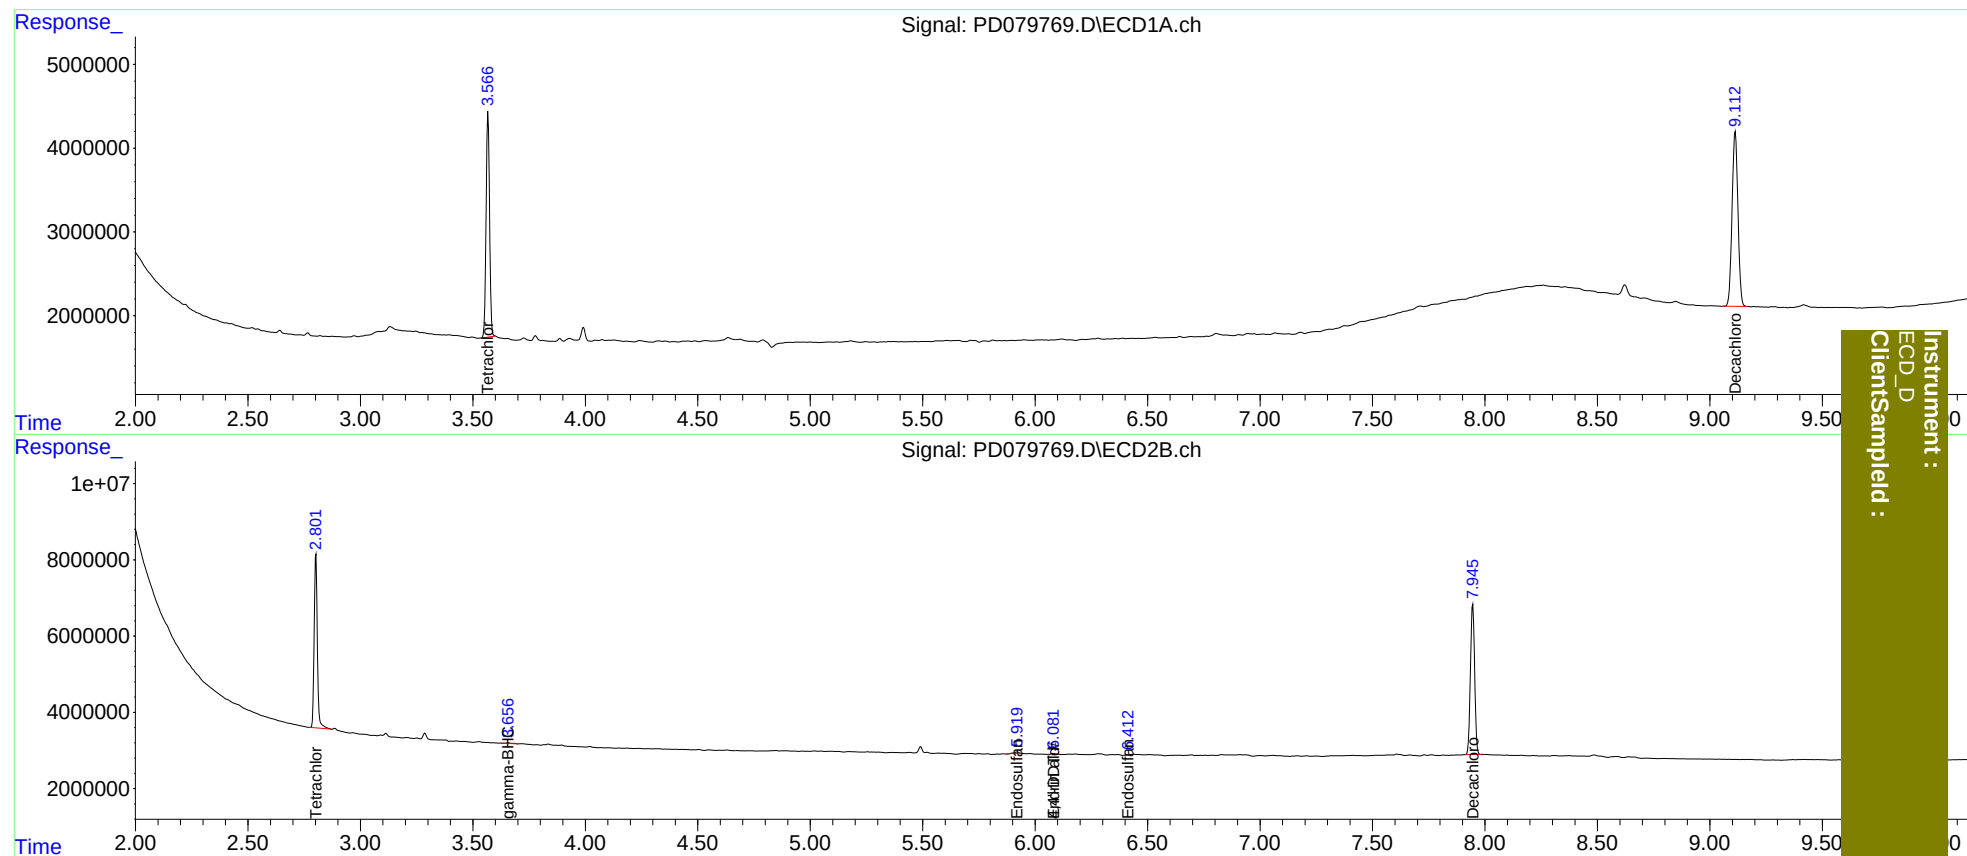


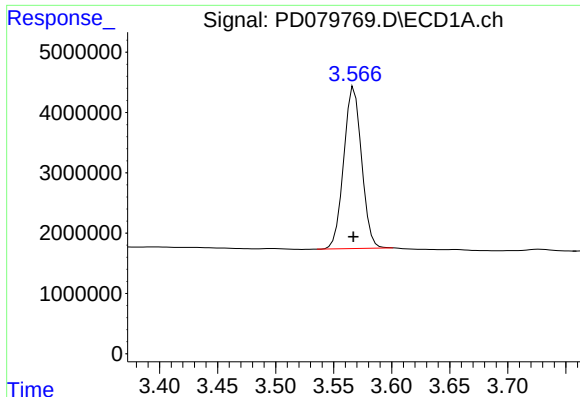

#1 Tetrachloro-m-xylene


R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 28696248
Conc: 19.65 ng/ml

Instrument :
ECD_D
ClientSampleId :

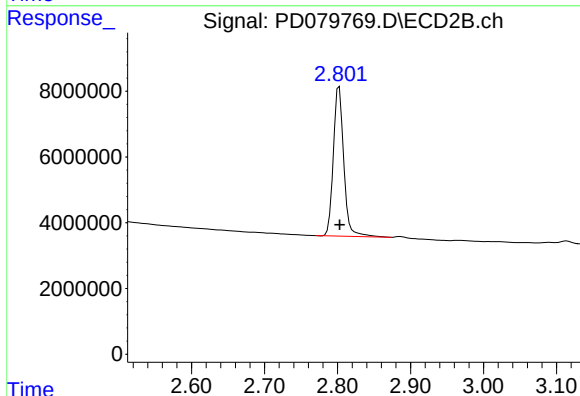


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 45308753
Conc: 19.81 ng/ml

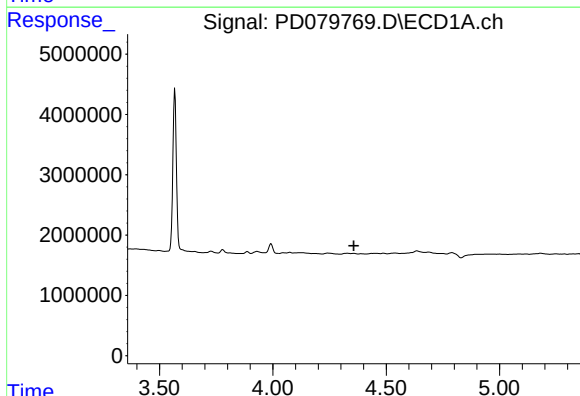


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.357 min
Response: 0
Conc: N.D.

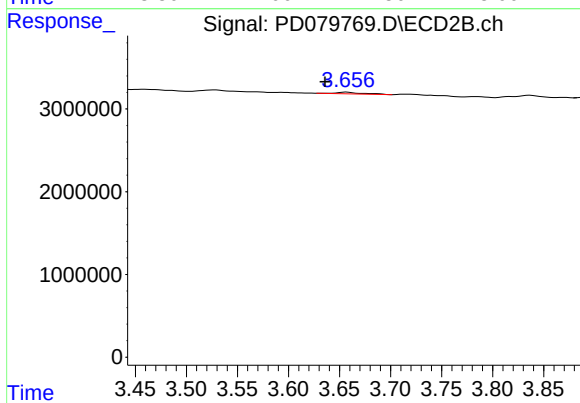

#3 gamma-BHC (Lindane)


R.T.: 3.657 min
Delta R.T.: 0.021 min
Response: 348541
Conc: 0.10 ng/ml

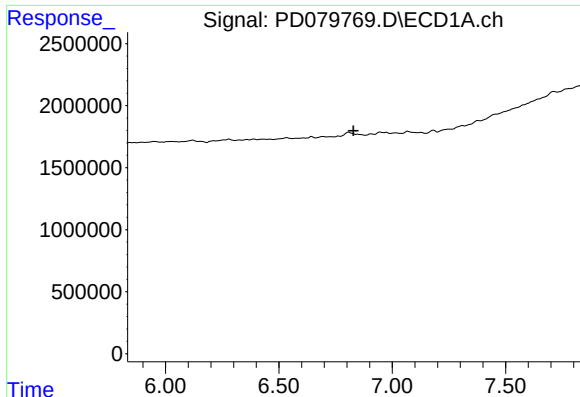

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.830 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

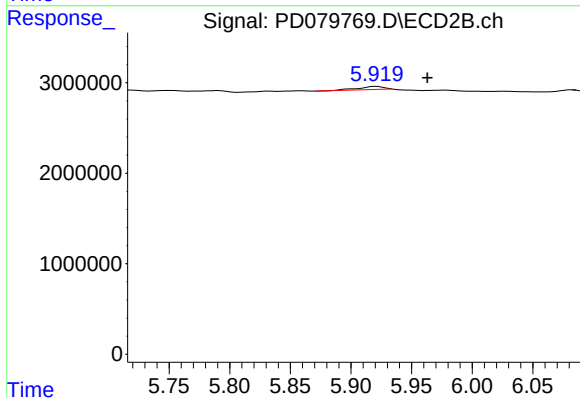


#15 Endosulfan II

R.T.: 5.921 min
Delta R.T.: -0.042 min
Response: 509717
Conc: 0.20 ng/ml

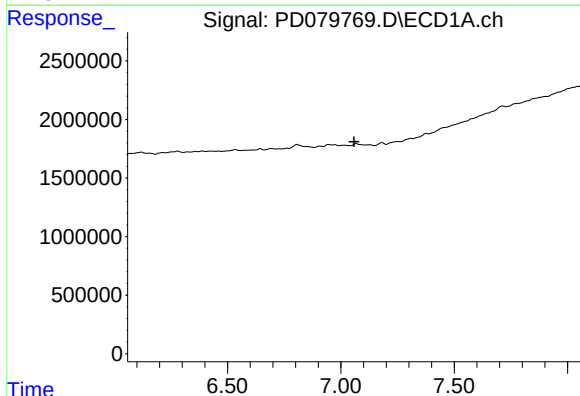


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.058 min
Response: 0
Conc: N.D.

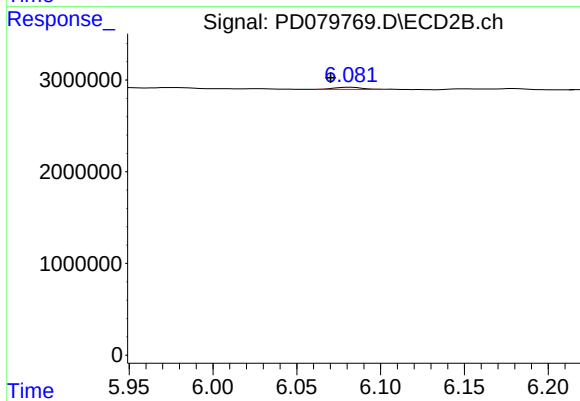

#17 4,4'-DDT


R.T.: 6.082 min
Delta R.T.: 0.012 min
Response: 255955
Conc: 0.11 ng/ml

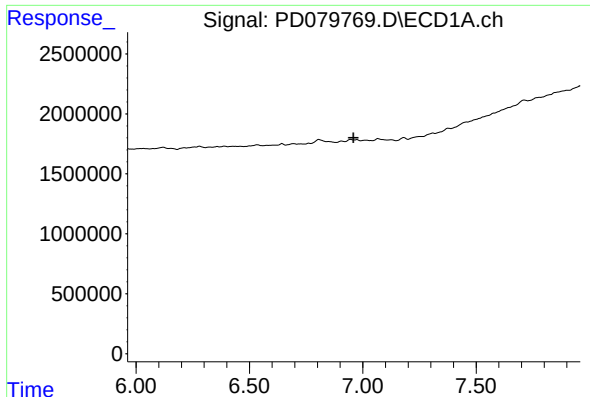

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.959 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

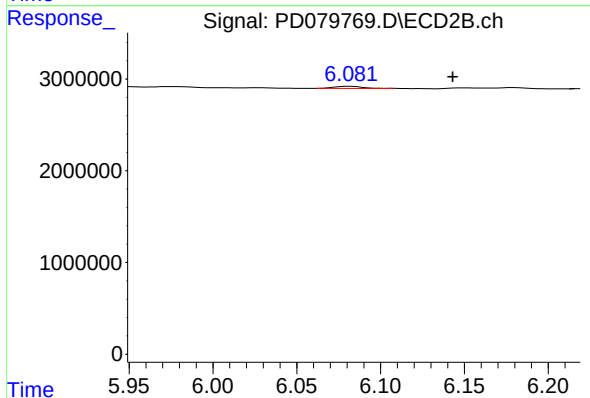


#18 Endrin aldehyde

R.T.: 6.082 min
Delta R.T.: -0.061 min
Response: 255955
Conc: 0.13 ng/ml

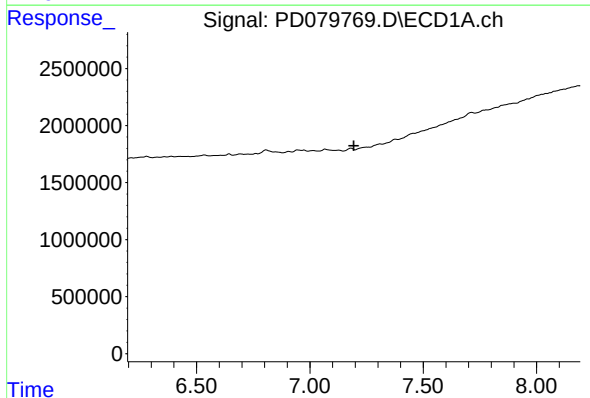


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 7.193 min
Response: 0
Conc: N.D.

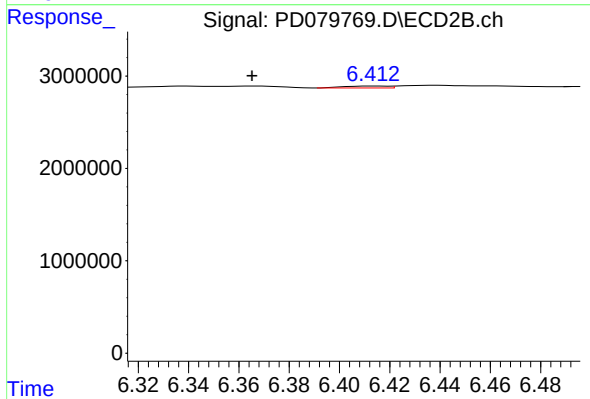

#19 Endosulfan Sulfate


R.T.: 6.414 min
Delta R.T.: 0.049 min
Response: 262807
Conc: 0.11 ng/ml

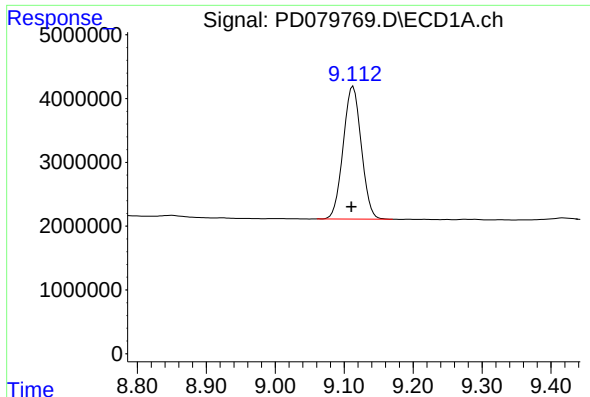

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.003 min
Response: 37938646
Conc: 21.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

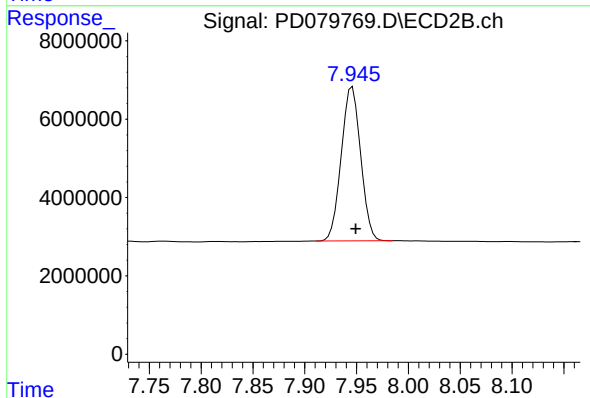

#27 Decachlorobiphenyl

R.T.: 7.946 min
Delta R.T.: -0.003 min
Response: 51249827
Conc: 21.47 ng/ml