

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
 Data File : PD079770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 18:21
 Operator : AR\AJ
 Sample : PIBLK091
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 20:21:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	27092972	44284198	18.552	19.361
2)	SA Decachlor...	9.113	7.946	65906494	91043112	37.140	38.134
Target Compounds							
2)	A alpha-BHC	0.000	3.297	0	236715	N.D.	<MDL
3)	MA gamma-BHC...	0.000	3.635	0	102489	N.D.	<MDL
4)	MA Heptachlor	0.000	3.974	0	161604	N.D.	<MDL
5)	MB Aldrin	0.000	4.237	0	1076265	N.D.	0.331
6)	B beta-BHC	0.000	3.943	0	144465	N.D.	<MDL
7)	B delta-BHC	0.000	4.162	0	160369	N.D.	<MDL
8)	B Heptachlo...	0.000	4.723f	0	125897	N.D.	<MDL
9)	A Endosulfan I	0.000	5.162	0	334893	N.D.	0.121
10)	B trans-Chl...	0.000	5.008	0	485268	N.D.	0.163
11)	B cis-Chlor...	0.000	5.008f	0	485268	N.D.	0.160
13)	MA Dieldrin	0.000	5.394	0	1649521	N.D.	0.518
14)	MA Endrin	0.000	5.685	0	729077	N.D.	0.266
15)	B Endosulfa...	0.000	5.922f	0	336337	N.D.	0.130
17)	MA 4,4'-DDT	0.000	6.068	0	184633	N.D.	<MDL
18)	B Endrin al...	0.000	6.160	0	84577	N.D.	<MDL
22)	Toxaphene-1	0.000	5.008	0	485268	N.D.	29.022
23)	Toxaphene-2	0.000	5.394	0	1649521	N.D.	98.160
25)	Toxaphene-4	0.000	6.791	0	172244	N.D.	2.188


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
Data File : PD079770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 18:21
Operator : AR\AJ
Sample : PIBLK091
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 20:21:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

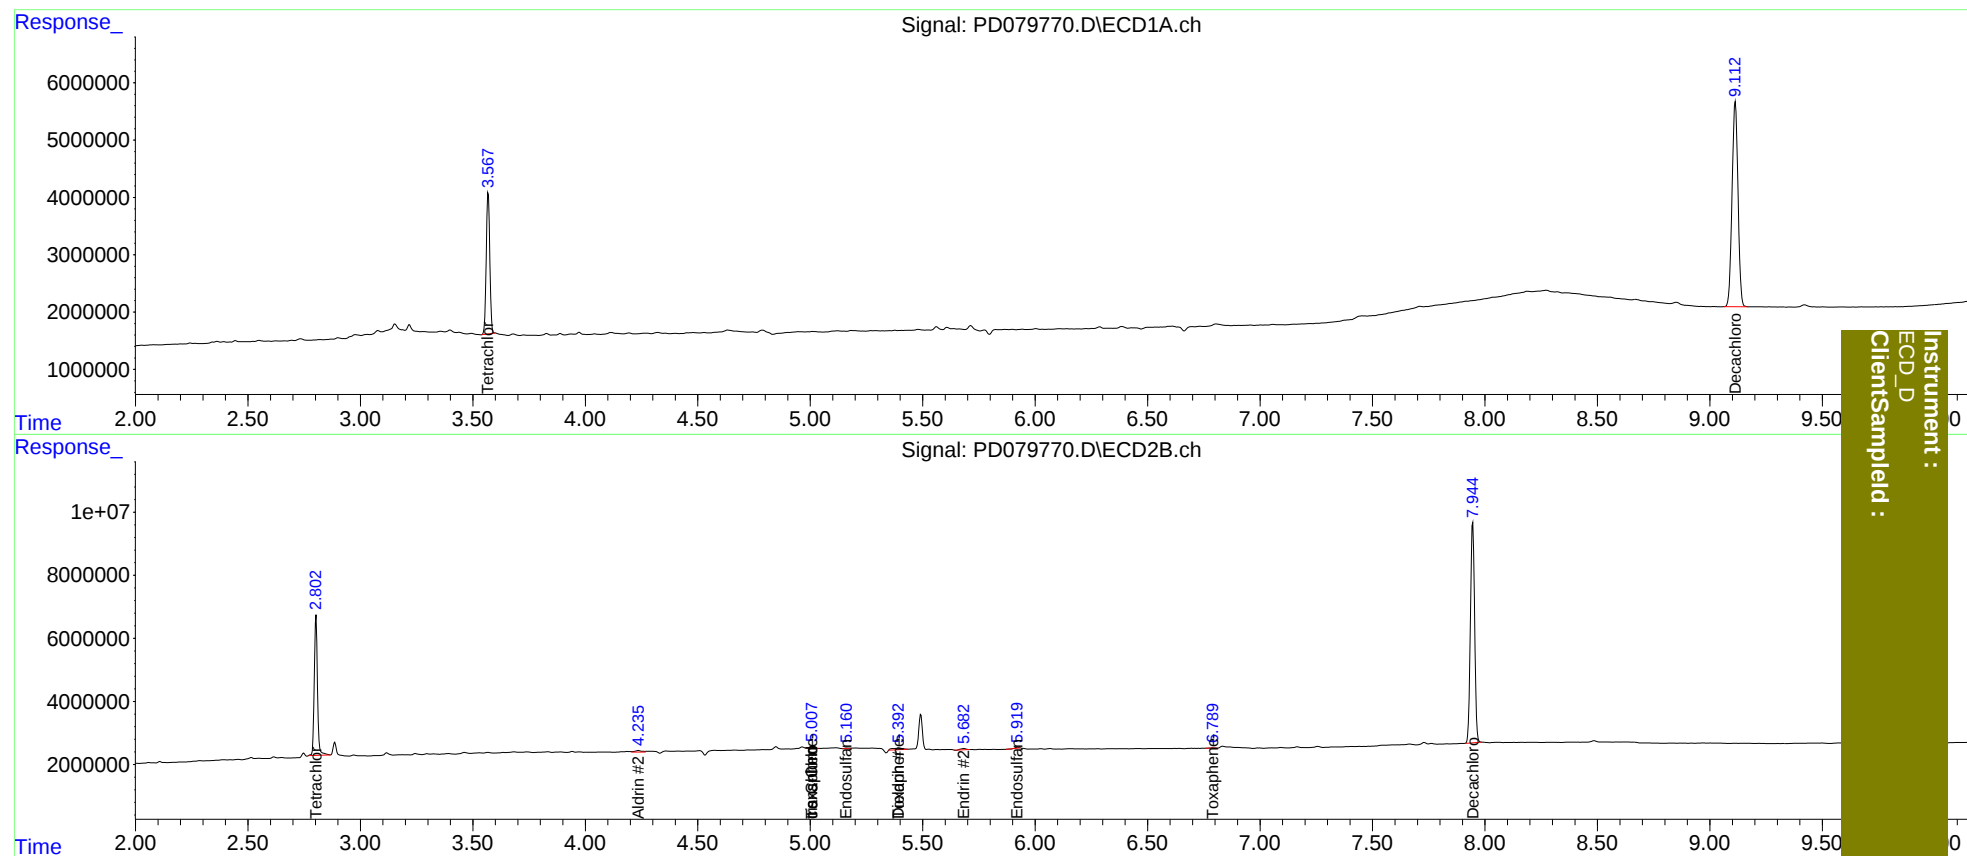


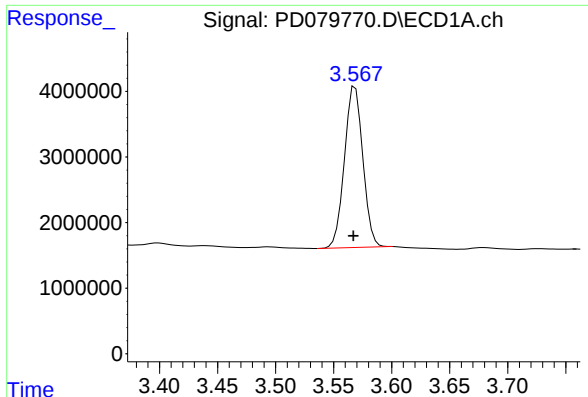

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.002 min
Response: 27092972
Conc: 18.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

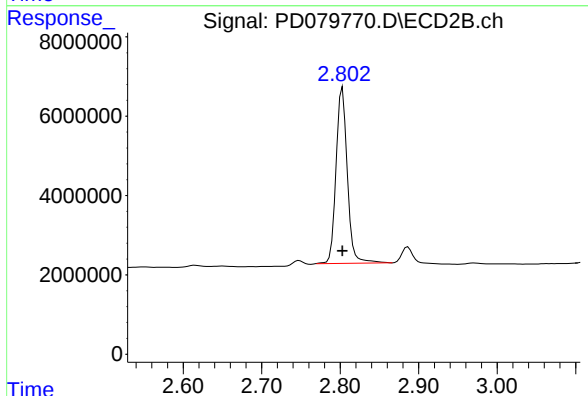


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 44284198
Conc: 19.36 ng/ml

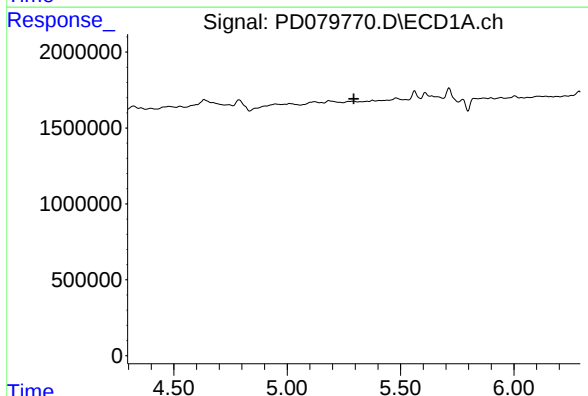


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

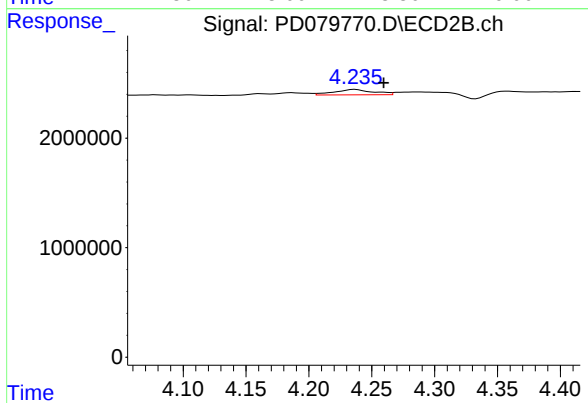

#5 Aldrin


R.T.: 4.237 min
Delta R.T.: -0.023 min
Response: 1076265
Conc: 0.33 ng/ml

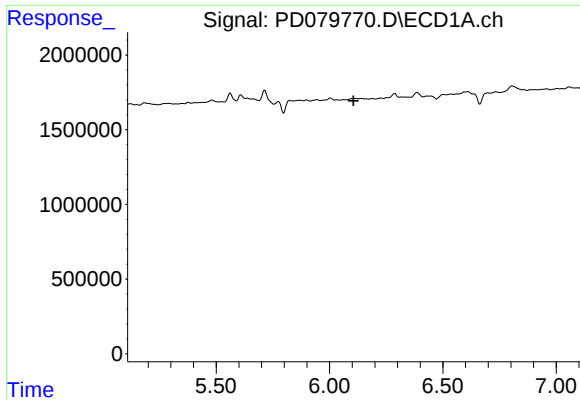

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.106 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

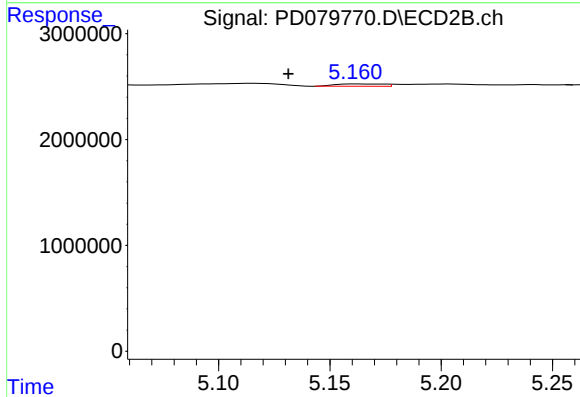


#9 Endosulfan I

R.T.: 5.162 min
Delta R.T.: 0.030 min
Response: 334893
Conc: 0.12 ng/ml

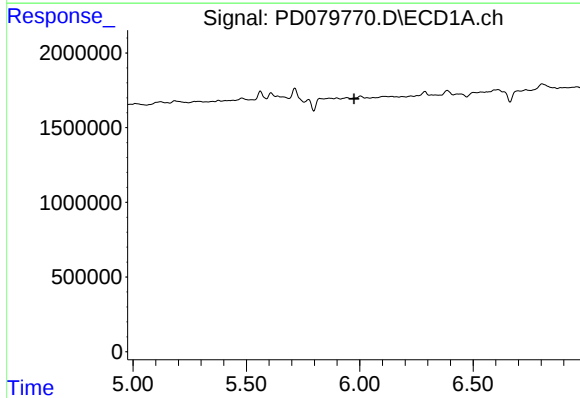


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

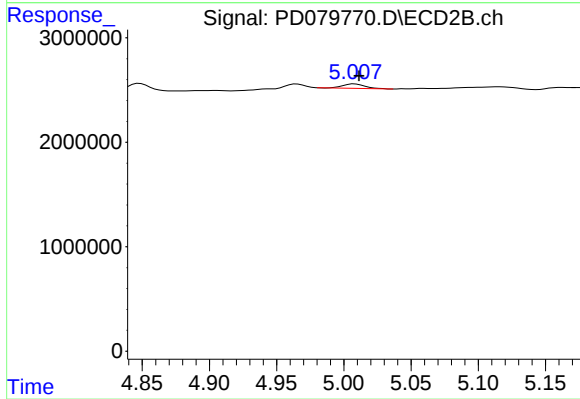

#10 trans-Chlordane


R.T.: 5.008 min
Delta R.T.: -0.003 min
Response: 485268
Conc: 0.16 ng/ml

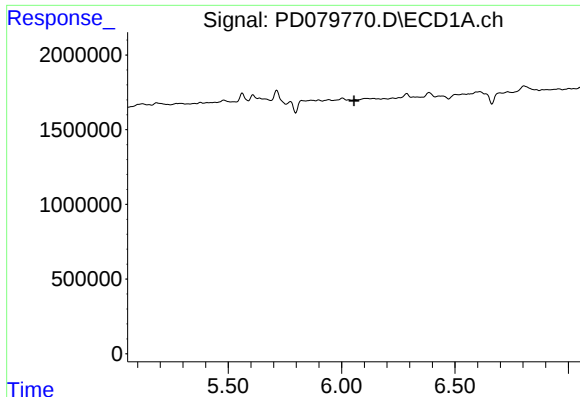

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.056 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

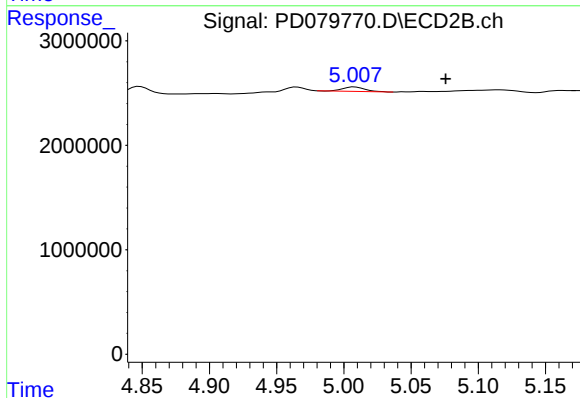


#11 cis-Chlordane

R.T.: 5.008 min
Delta R.T.: -0.068 min
Response: 485268
Conc: 0.16 ng/ml

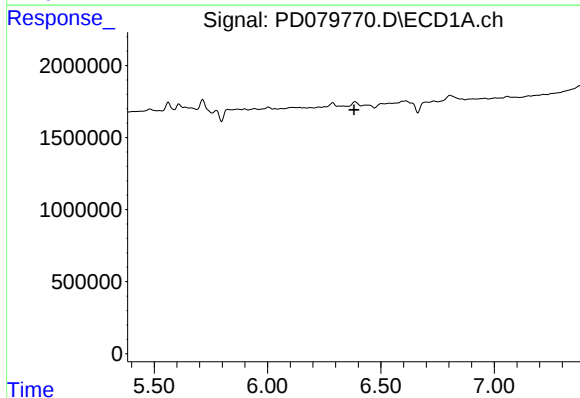


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.382 min
Response: 0
Conc: N.D.

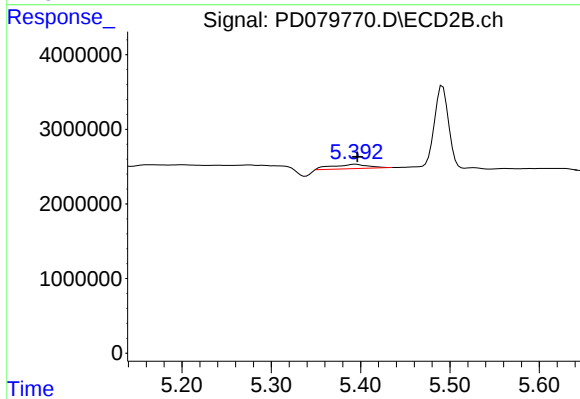

#13 Dieldrin


R.T.: 5.394 min
Delta R.T.: -0.002 min
Response: 1649521
Conc: 0.52 ng/ml

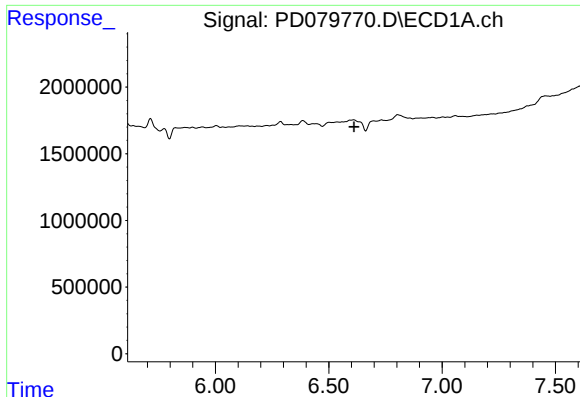

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

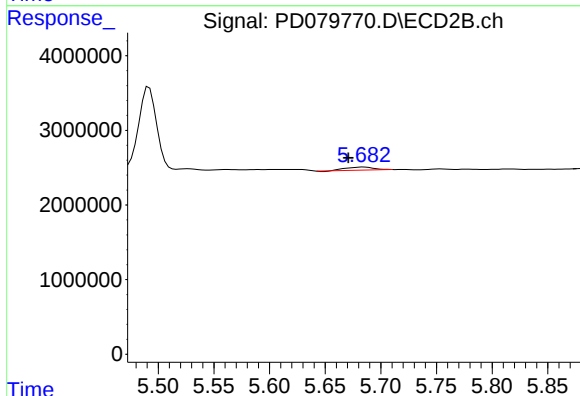


#14 Endrin

R.T.: 5.685 min
Delta R.T.: 0.014 min
Response: 729077
Conc: 0.27 ng/ml

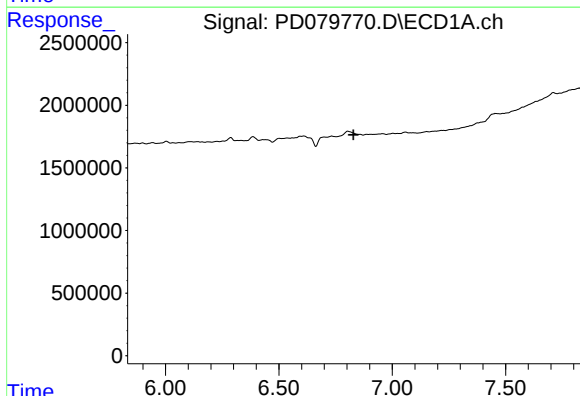


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.830 min
Response: 0
Conc: N.D.

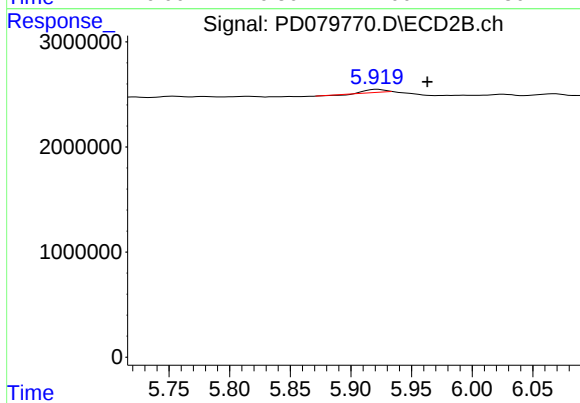

#15 Endosulfan II


R.T.: 5.922 min
Delta R.T.: -0.041 min
Response: 336337
Conc: 0.13 ng/ml

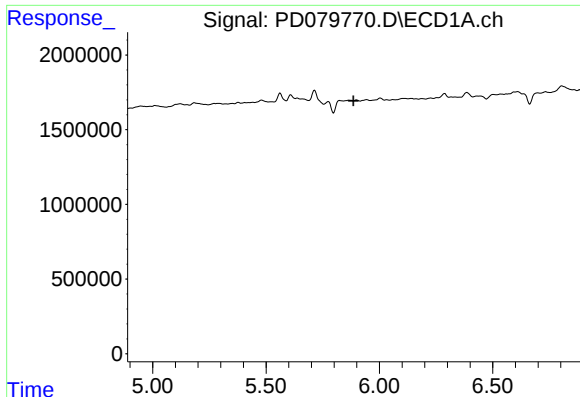

#22 Toxaphene-1


R.T.: 0.000 min
Exp R.T.: 5.886 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

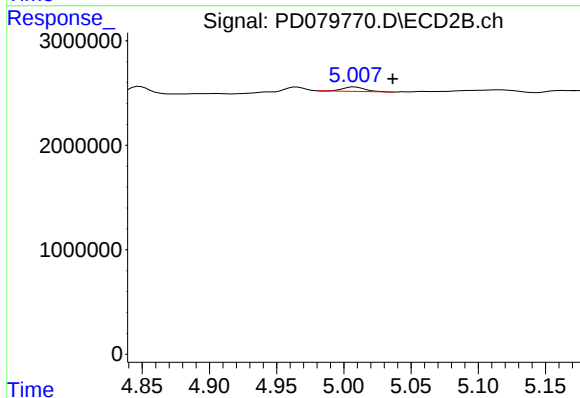


#22 Toxaphene-1

R.T.: 5.008 min
Delta R.T.: -0.028 min
Response: 485268
Conc: 29.02 ng/ml

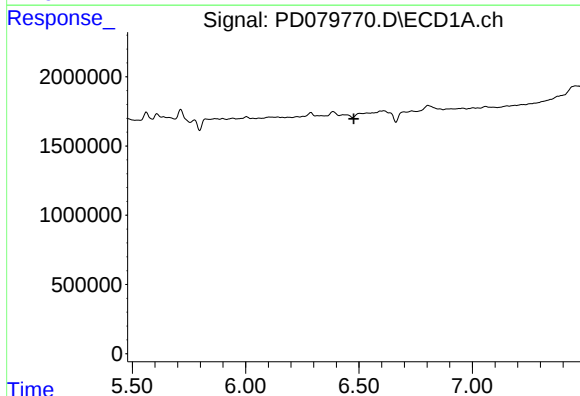


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 6.477 min
Response: 0
Conc: N.D.

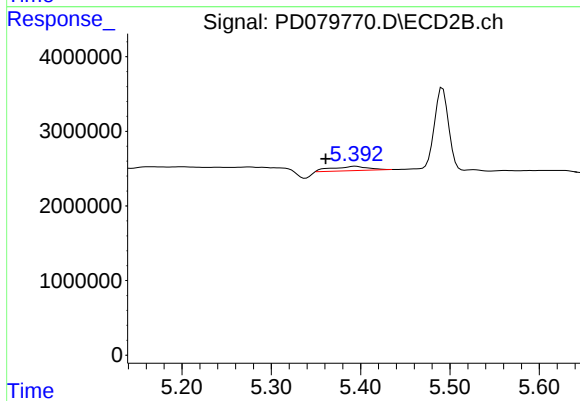

#23 Toxaphene-2


R.T.: 5.394 min
Delta R.T.: 0.033 min
Response: 1649521
Conc: 98.16 ng/ml

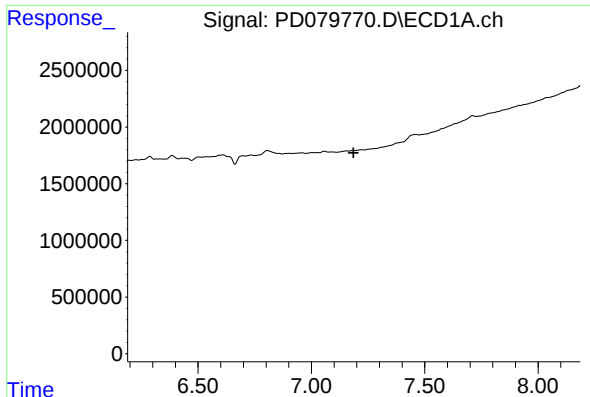

#25 Toxaphene-4


R.T.: 0.000 min
Exp R.T.: 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

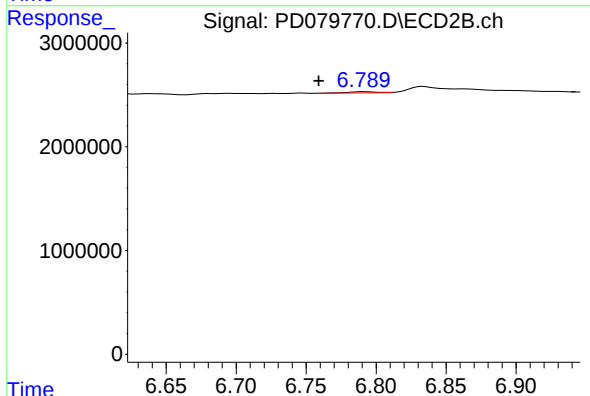


#25 Toxaphene-4

R.T.: 6.791 min
Delta R.T.: 0.032 min
Response: 172244
Conc: 2.19 ng/ml

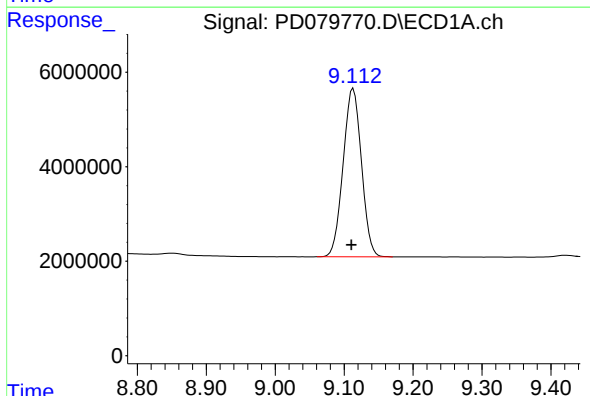

#27 Decachlorobiphenyl

R.T.: 9.113 min
Delta R.T.: 0.003 min
Response: 65906494
Conc: 37.14 ng/ml

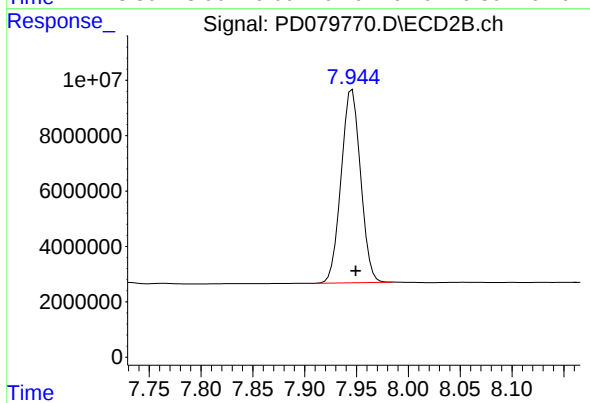

#27 Decachlorobiphenyl

R.T.: 7.946 min
Delta R.T.: -0.003 min
Response: 91043112
Conc: 38.13 ng/ml