

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
 Data File : PD079772.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 18:48
 Operator : AR\AJ
 Sample : 05439-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:12:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	31542998	50205466	21.599	21.950
27)	SA Decachlor...	9.112	7.947	39713417	53916225	22.380	22.583
Target Compounds							
7)	B delta-BHC	0.000	4.185	0	134578	N.D.	<MDL
13)	MA Dieldrin	0.000	5.445f	0	291140	N.D.	<MDL
14)	MA Endrin	0.000	5.688	0	178969	N.D.	<MDL
15)	B Endosulfa...	0.000	5.921f	0	592808	N.D.	0.228
16)	A 4,4'-DDD	0.000	5.854f	0	147760	N.D.	<MDL
17)	MA 4,4'-DDT	0.000	6.082	0	265099	N.D.	0.110
18)	B Endrin al...	0.000	6.082f	0	265099	N.D.	0.131
19)	B Endosulfa...	0.000	6.412f	0	311377	N.D.	0.125


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
Data File : PD079772.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 18:48
Operator : AR\AJ
Sample : 05439-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:12:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

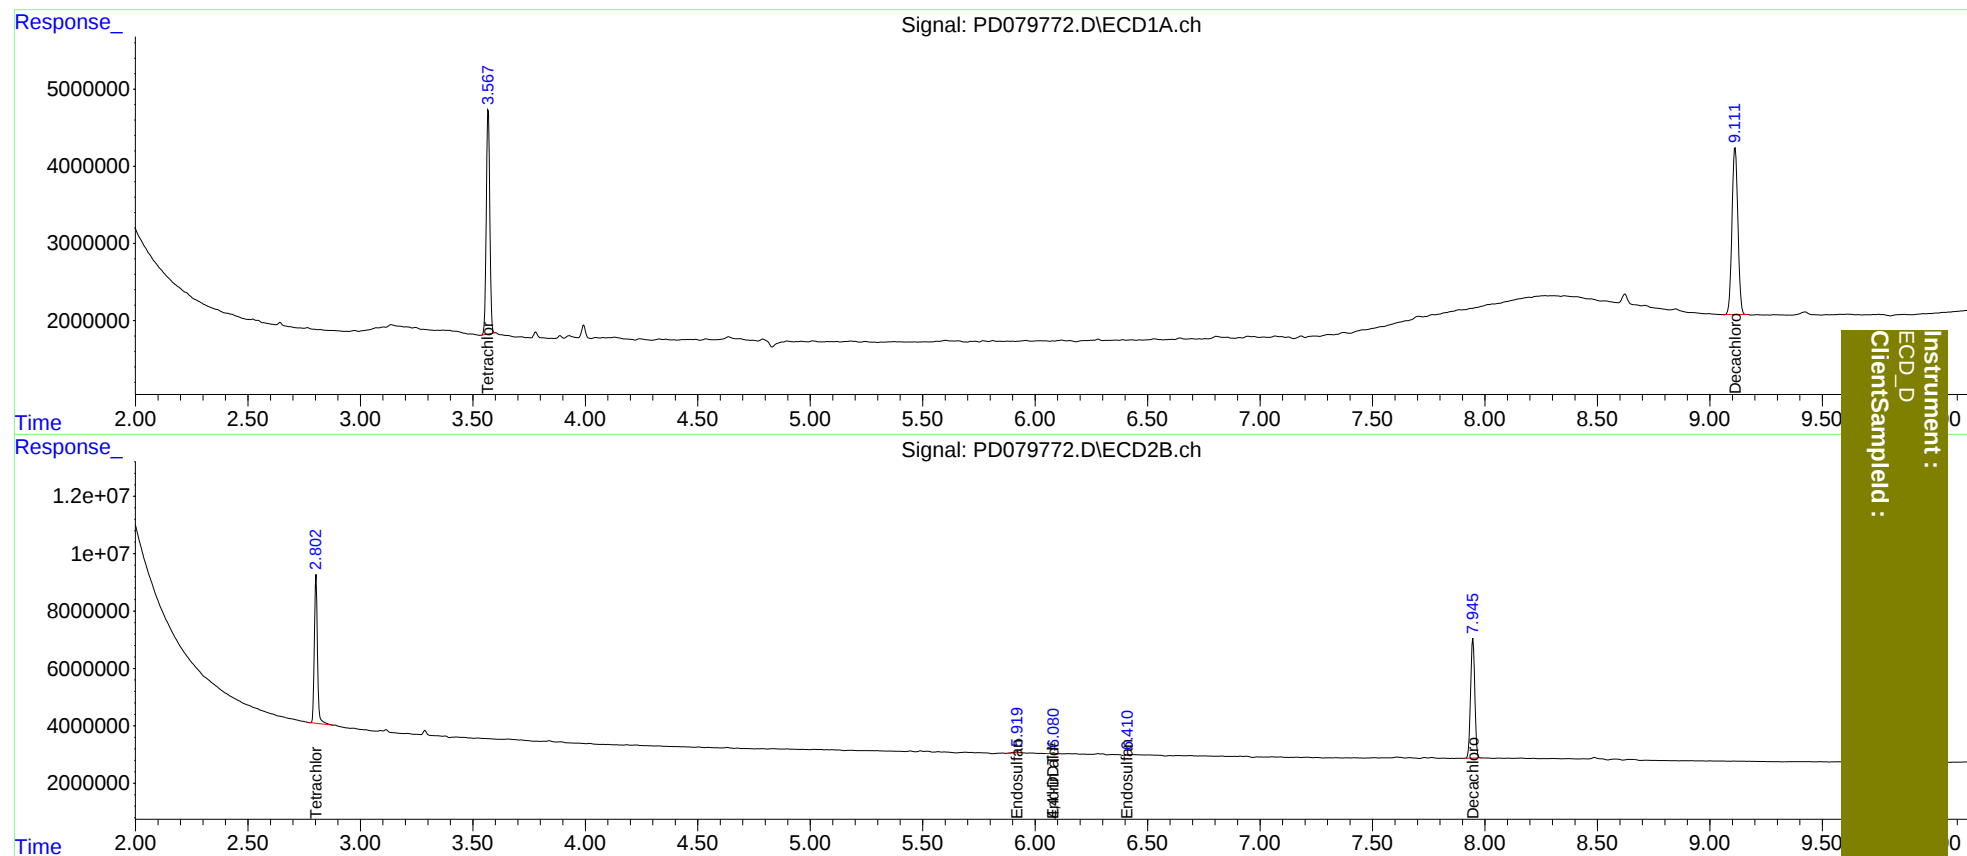


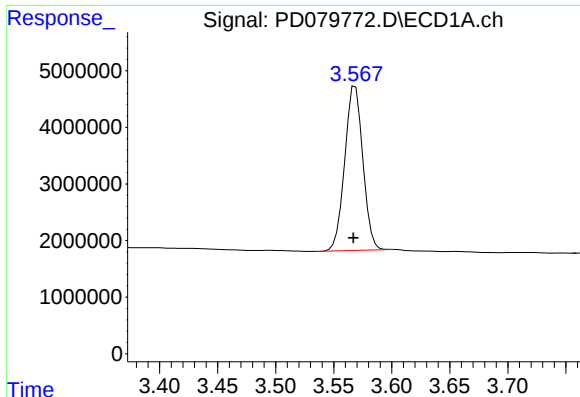

#1 Tetrachloro-m-xylene


R.T.: 3.569 min
Delta R.T.: 0.002 min
Response: 31542998
Conc: 21.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

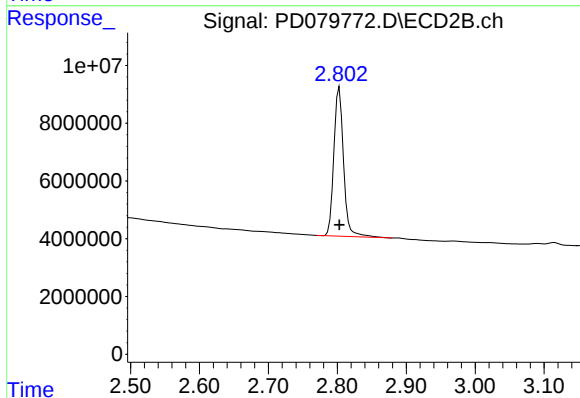


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 50205466
Conc: 21.95 ng/ml

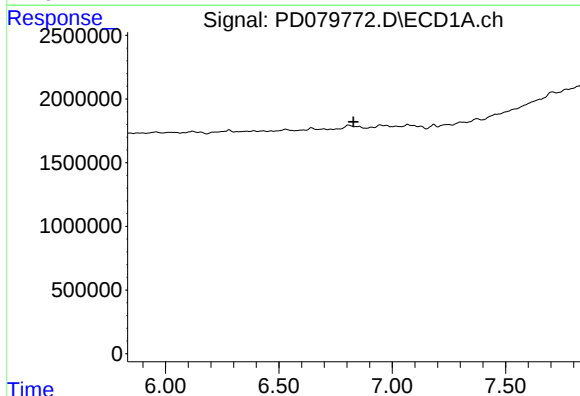


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.830 min
Response: 0
Conc: N.D.

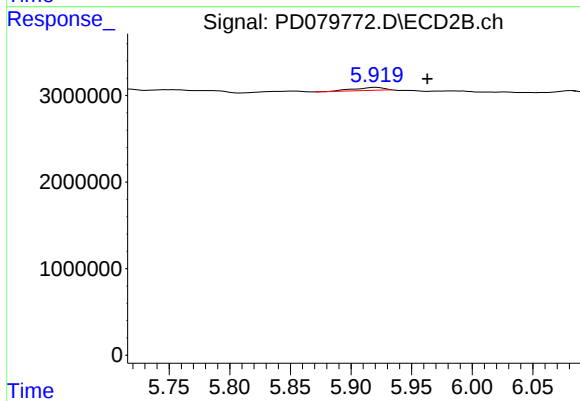

#15 Endosulfan II


R.T.: 5.921 min
Delta R.T.: -0.042 min
Response: 592808
Conc: 0.23 ng/ml

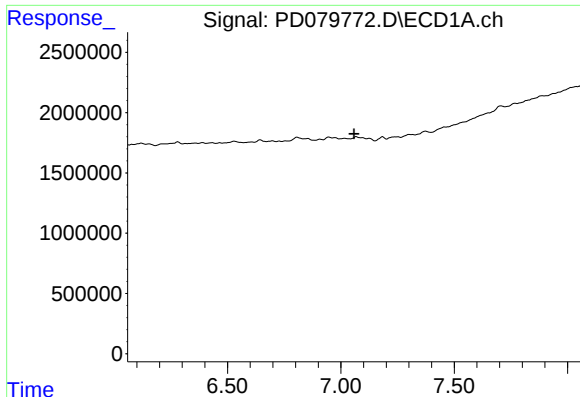

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.058 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

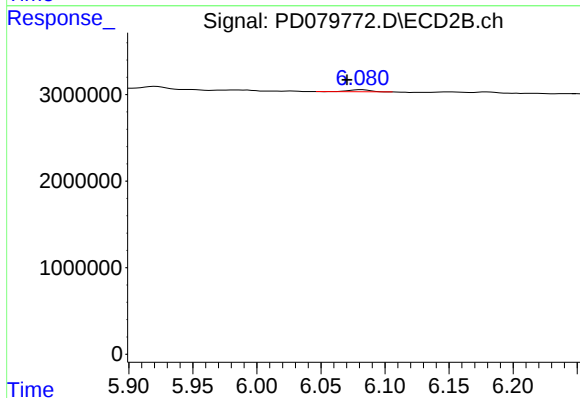


#17 4,4'-DDT

R.T.: 6.082 min
Delta R.T.: 0.011 min
Response: 265099
Conc: 0.11 ng/ml

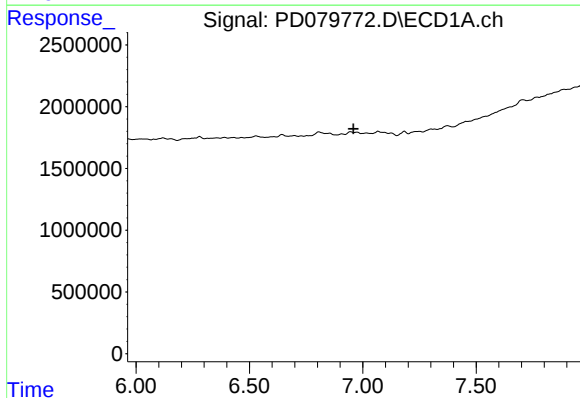


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.959 min
Response: 0
Conc: N.D.

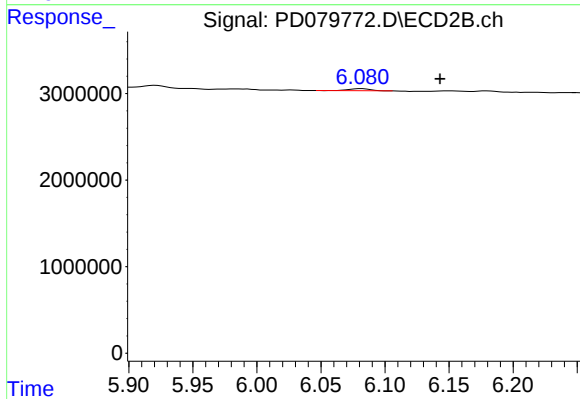

#18 Endrin aldehyde


R.T.: 6.082 min
Delta R.T.: -0.061 min
Response: 265099
Conc: 0.13 ng/ml

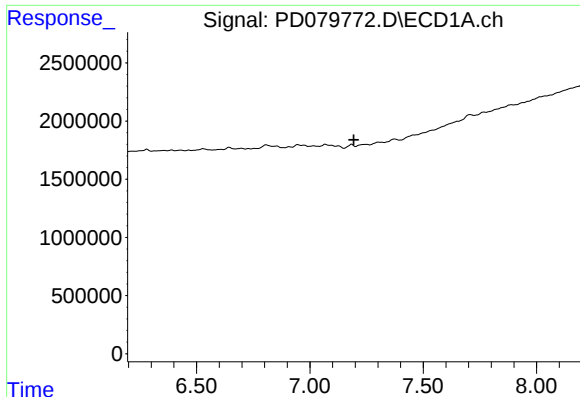

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.193 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

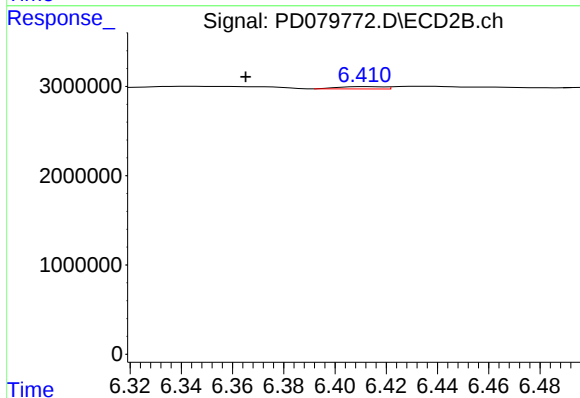


#19 Endosulfan Sulfate

R.T.: 6.412 min
Delta R.T.: 0.047 min
Response: 311377
Conc: 0.13 ng/ml

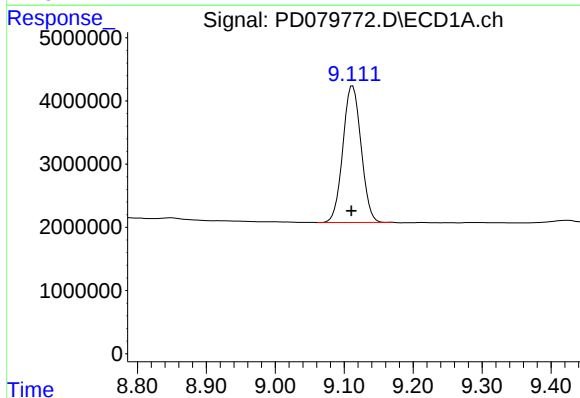

#27 Decachlorobiphenyl

R.T.: 9.112 min
Delta R.T.: 0.002 min
Response: 39713417
Conc: 22.38 ng/ml

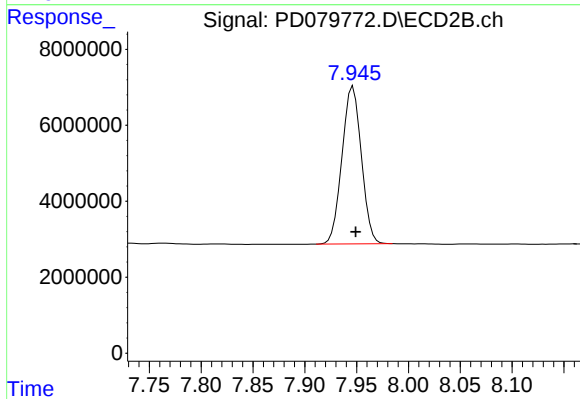

#27 Decachlorobiphenyl

R.T.: 7.947 min
Delta R.T.: -0.003 min
Response: 53916225
Conc: 22.58 ng/ml