

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
 Data File : PD079793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 23:28
 Operator : AR\AJ
 Sample : 05416-14
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AG7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2023
 Supervised By :Ankita Jodhani 11/22/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 01:17:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	24216216	41749941	16.582	18.253
27)	SA Decachlor...	9.114	7.947	27144363	39305643	15.297	16.463
Target Compounds							
9)	A Endosulfan I	6.137	5.142	2344558	3032148	1.134m	1.094m
13)	MA Dieldrin	6.401	5.400	1398801	3257913	0.636	1.023 #
16)	A 4,4'-DDD	6.732	5.814	2769831	3440729	1.710	1.462m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
Data File : PD079793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 23:28
Operator : AR\AJ
Sample : 05416-14
Misc :
ALS Vial : 45 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 01:17:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

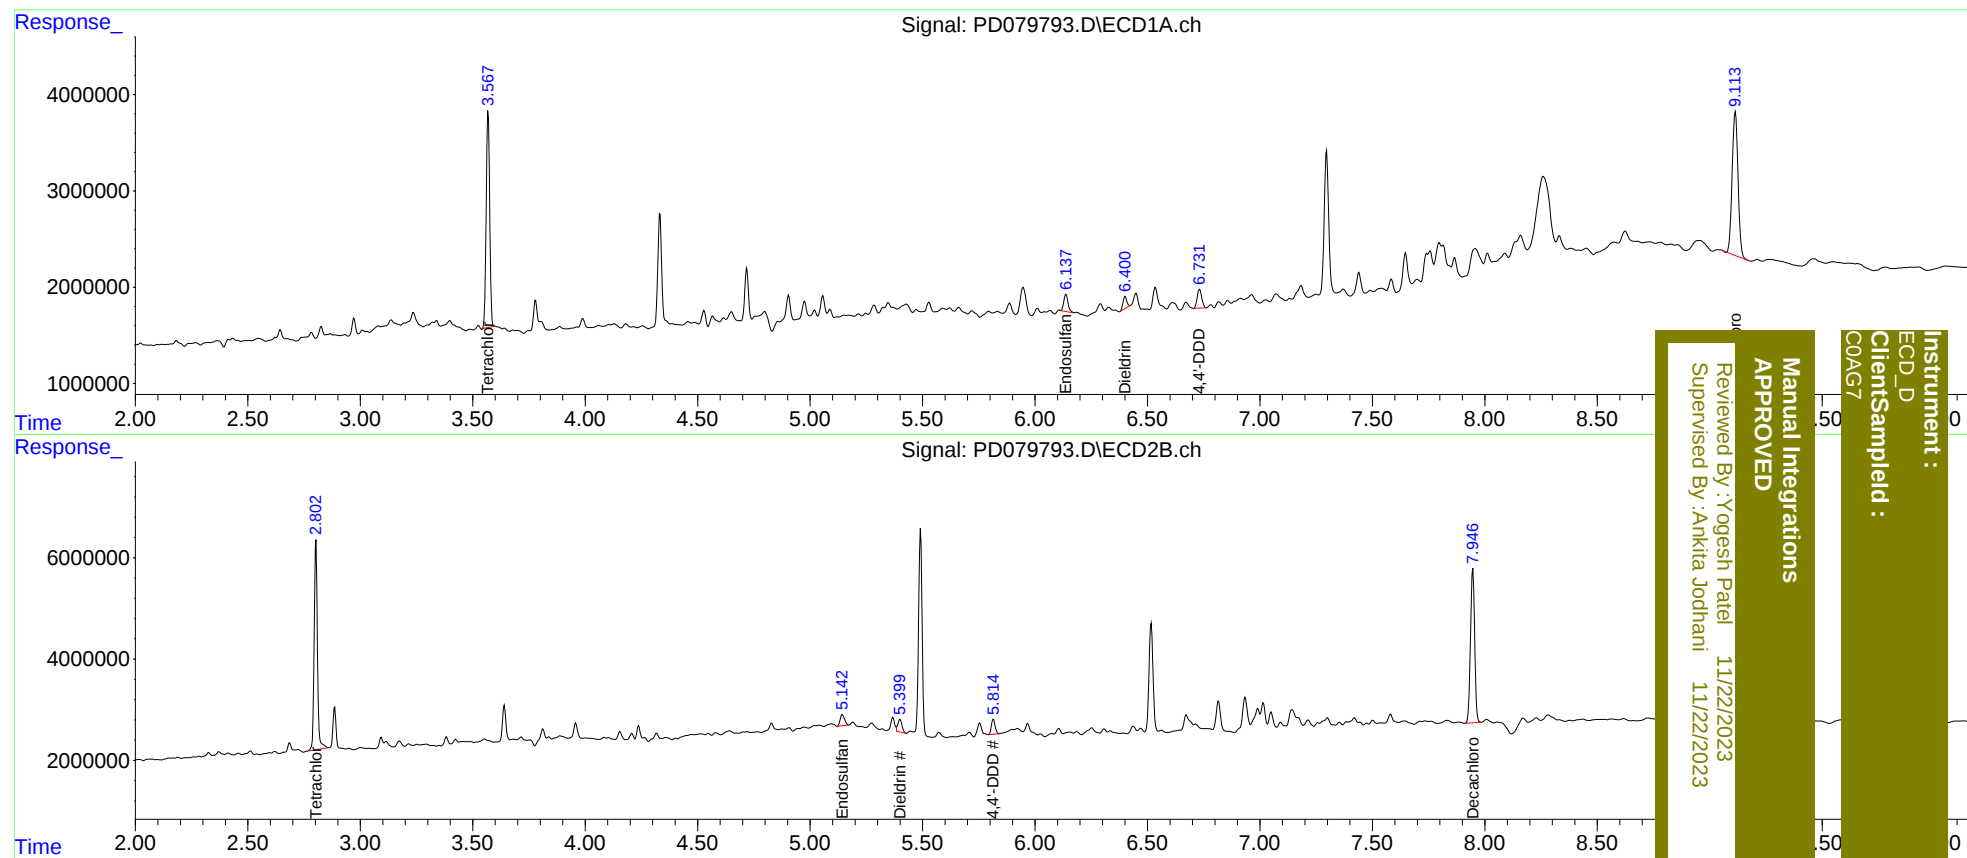

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/22/2023
Supervised By : Ankita Jodhani 11/22/2023

Instrument :
ECD_D
ClientSampled :
COAG7