

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
 Data File : PD079792.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2023 23:15
 Operator : AR\AJ
 Sample : 05416-13
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AG6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/24/2023
 Supervised By :Ankita Jodhani 11/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 04:05:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.803	17304796	26746699	11.850	11.694
27)	SA Decachlor...	9.112	7.947	18851601	25342168	10.623m	10.615
Target Compounds							
13)	MA Dieldrin	6.397	5.399	1862434	2110553	0.847m	0.663m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112123\
Data File : PD079792.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2023 23:15
Operator : AR\AJ
Sample : 05416-13
Misc :
ALS Vial : 44 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 04:05:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

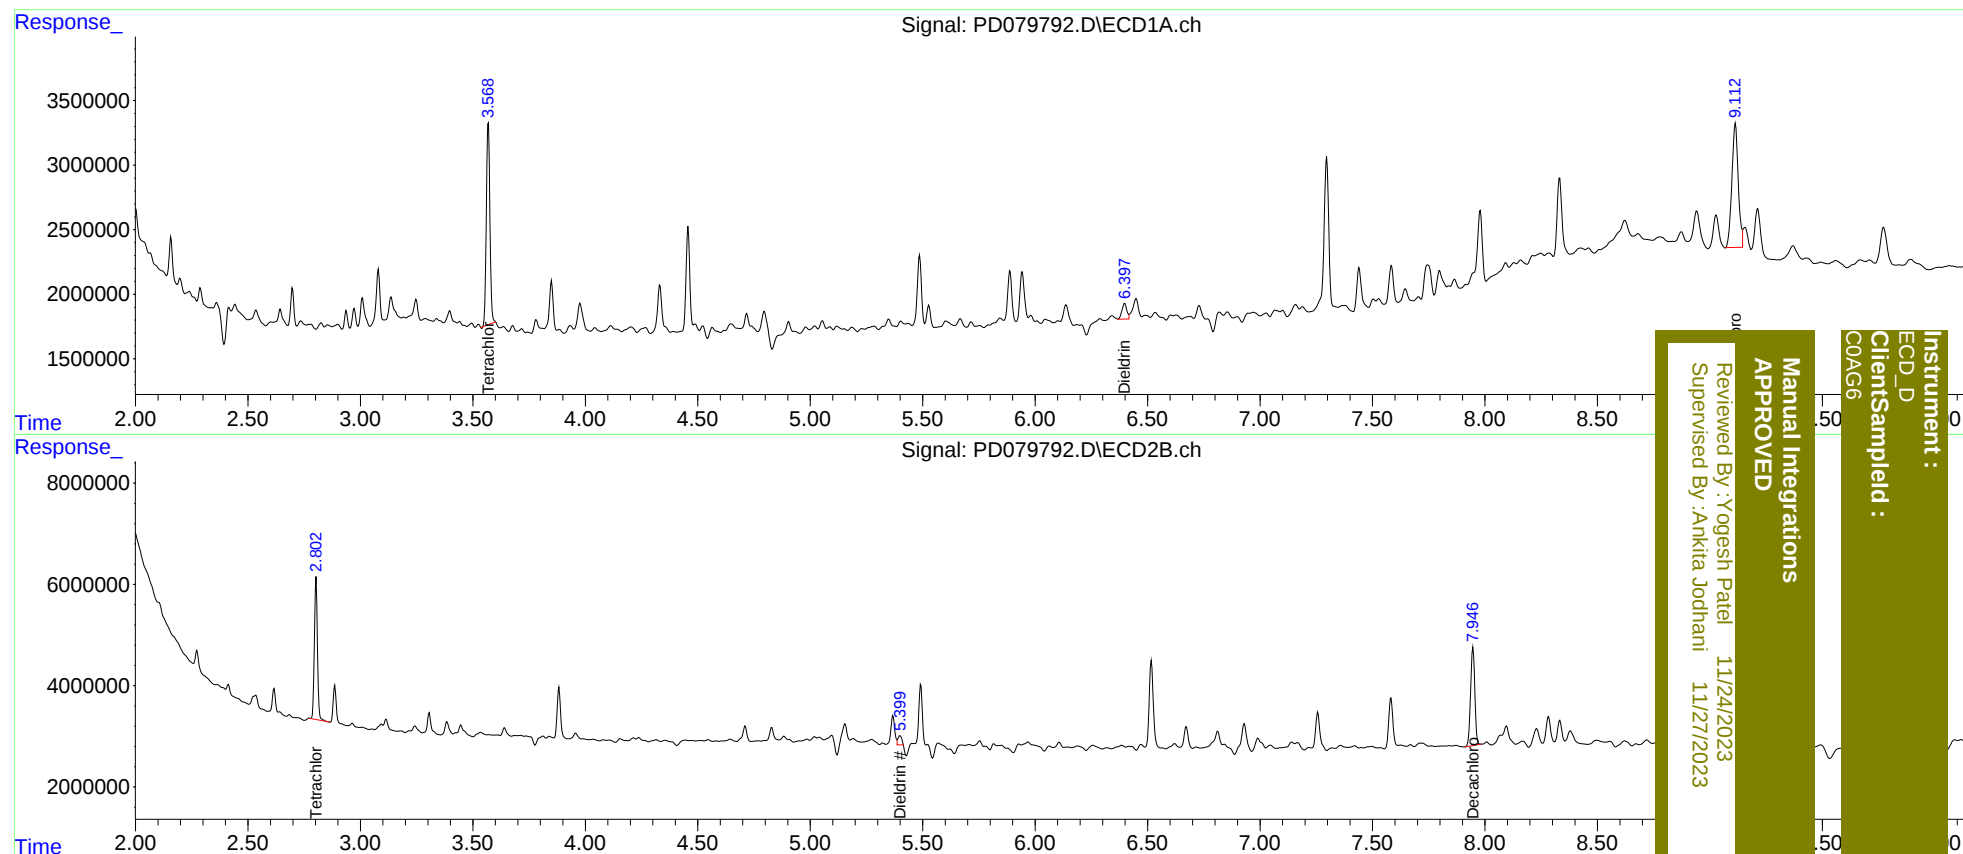

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/24/2023
Supervised By : Ankita Jodhani 11/27/2023

Instrument :
ECD_D
ClientSampled :
COAG6