

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
 Data File : PD086840.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 09:54
 Operator : AR\AJ
 Sample : P4847-02DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AT1DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2024
 Supervised By :Ankita Jodhani 11/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:13:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	20832681	128.8E6	11.329m	11.164
27)	SA Decachlor...	9.093	8.091	41135499	191.4E6	15.450	15.021
Target Compounds							
2)	A alpha-BHC	4.009	3.400	2645.7E6	8168.9E6	751.406	456.091 #
3)	MA gamma-BHC...	4.340	3.737	820.4E6	2820.4E6	235.564	169.102 #
4)	MA Heptachlor	4.941	4.093	984.5E6	3152.4E6	283.324	183.260 #
5)	MB Aldrin	5.284	4.380	2758.6E6	7949.4E6	781.243	465.355 #
6)	B beta-BHC	4.524	4.032	712.8E6	2687.3E6	449.646	340.180
7)	B delta-BHC	4.773	4.270	1023.9E6	3410.9E6	281.346	194.258 #
8)	B Heptachlo...	5.703	4.884	1161.3E6	3800.2E6	355.279	239.625 #
9)	A Endosulfan I	6.087	5.259	2756.9E6	8023.4E6	927.265	554.346 #
10)	B trans-Chl...	5.958	5.138	788.1E6	2877.6E6	246.418	174.212 #
11)	B cis-Chlor...	6.040	5.203	1264.8E6	4349.5E6	388.787	271.418 #
12)	B 4,4'-DDE	6.208	5.388	1450.8E6	5017.3E6	470.381	329.064 #
13)	MA Dieldrin	6.360	5.525	2476.3E6	7493.7E6	755.454	490.469 #
14)	MA Endrin	6.587	5.802	2127.7E6	6458.5E6	787.129	467.517 #
15)	B Endosulfa...	6.799	6.093	1148.6E6	4078.3E6	413.956	292.261 #
16)	A 4,4'-DDD	6.717	5.943	763.7E6	2864.9E6	321.928	237.134 #
17)	MA 4,4'-DDT	7.033	6.198	515.3E6	2040.1E6	207.905m	157.794
18)	B Endrin al...	6.927	6.272	1585.4E6	5159.3E6	721.327	480.753 #
19)	B Endosulfa...	7.162	6.496	796.9E6	2979.1E6	295.394	222.007
20)	A Methoxychlor	7.506	6.770	232.8E6	905.7E6	172.516	156.651
21)	B Endrin ke...	7.643	7.005	2582.4E6	7896.7E6	846.621	528.478 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
Data File : PD086840.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 09:54
Operator : AR\AJ
Sample : P4847-02DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:13:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

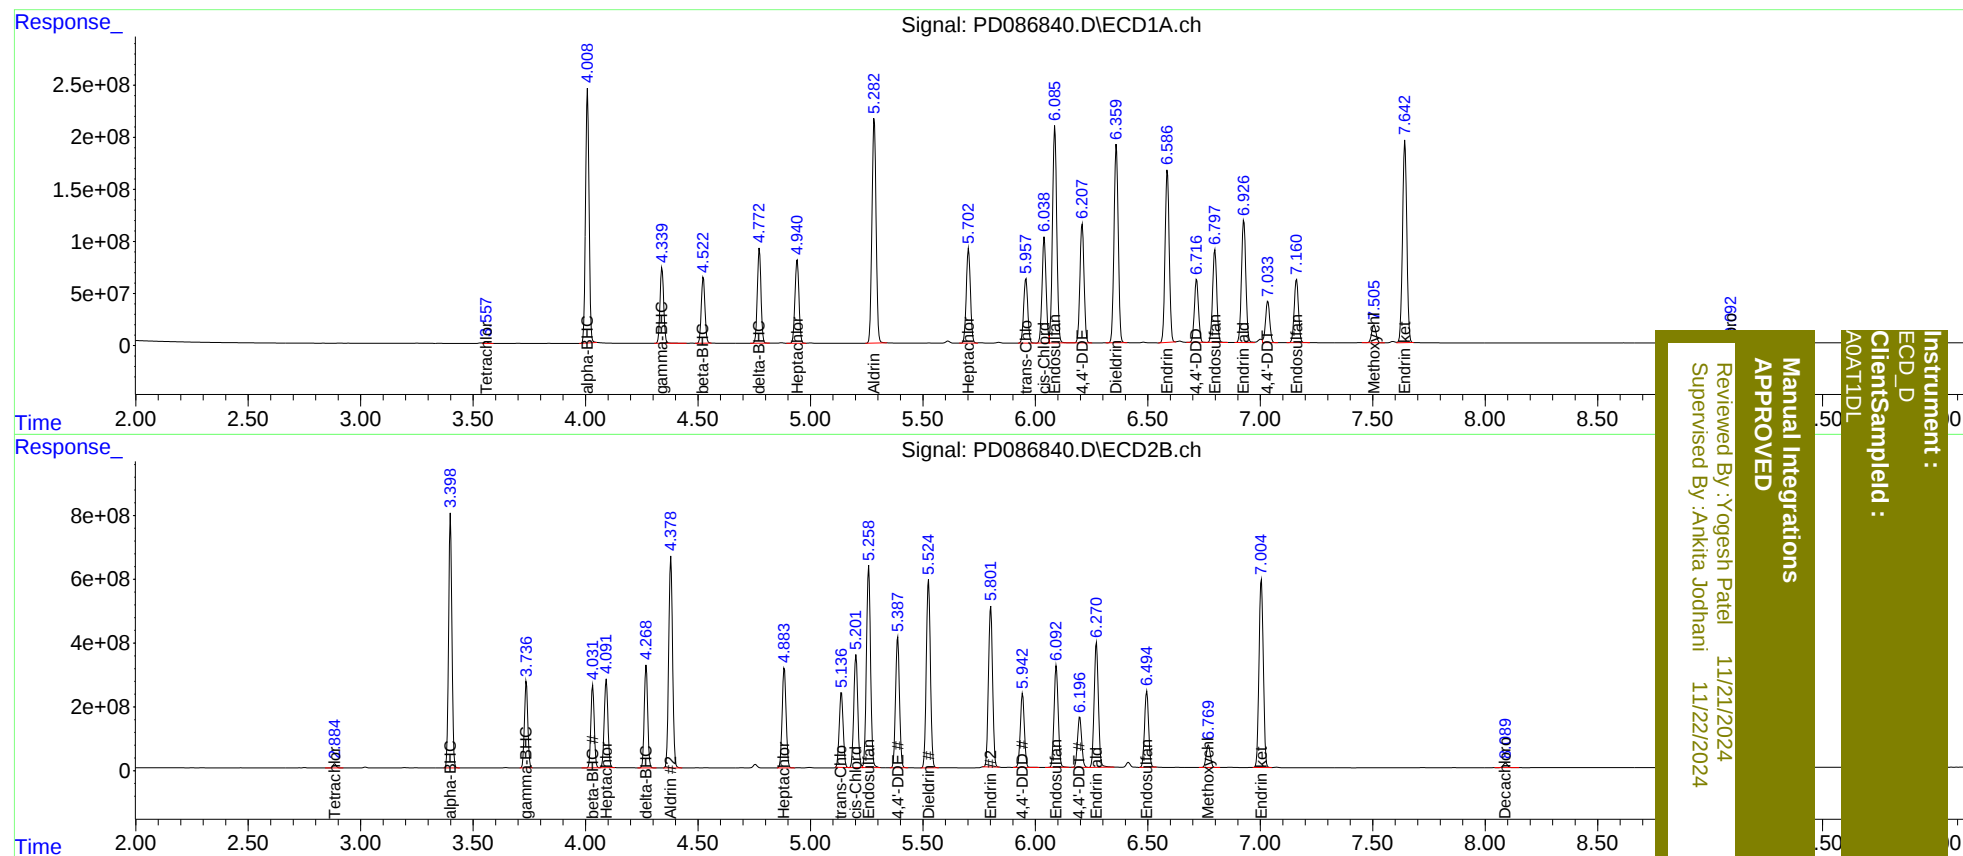

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/21/2024
Supervised By : Ankita Jodhani 11/22/2024

Instrument :
ECD_D
Client Sampled :
A0AT1DL