

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
 Data File : PD086841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 10:08
 Operator : AR\AJ
 Sample : P4847-02DL2 20X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 A0AT1DL2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :Ankita Jodhani 11/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:14:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.884	2410620	15781316	1.311m	1.367
27)	SA Decachlor...	9.092	8.089	5195158	25742687	1.951	2.020m
Target Compounds							
2)	A alpha-BHC	4.008	3.399	221.5E6	931.9E6	62.916	52.033
3)	MA gamma-BHC...	4.339	3.736	71244877	326.7E6	20.457	19.585
4)	MA Heptachlor	4.940	4.092	89203835	392.8E6	25.671	22.834
5)	MB Aldrin	5.283	4.379	256.4E6	1020.5E6	72.602	59.739
6)	B beta-BHC	4.523	4.032	72108755	329.0E6	45.489	41.647
7)	B delta-BHC	4.772	4.269	86728610	392.3E6	23.831	22.341
8)	B Heptachlo...	5.703	4.883	110.1E6	482.1E6	33.673	30.396
9)	A Endosulfan I	6.087	5.259	274.6E6	1099.3E6	92.370	75.953
10)	B trans-Chl...	5.957	5.136	71684866	349.1E6	22.413	21.133m
11)	B cis-Chlor...	6.039	5.202	117.5E6	524.8E6	36.104	32.751
12)	B 4,4'-DDE	6.208	5.388	127.9E6	607.4E6	41.456	39.834
13)	MA Dieldrin	6.359	5.525	234.3E6	972.1E6	71.491	63.625
14)	MA Endrin	6.586	5.801	199.5E6	862.1E6	73.817	62.407
15)	B Endosulfa...	6.798	6.093	110.4E6	525.8E6	39.799	37.680
16)	A 4,4'-DDD	6.717	5.943	69615467	359.6E6	29.344	29.763
17)	MA 4,4'-DDT	7.032	6.197	46925629	244.5E6	18.931m	18.910
18)	B Endrin al...	6.927	6.272	164.2E6	711.7E6	74.725	66.322
19)	B Endosulfa...	7.161	6.495	79235330	384.4E6	29.370	28.649
20)	A Methoxychlor	7.506	6.769	25938571	122.6E6	19.218	21.212
21)	B Endrin ke...	7.643	7.005	261.5E6	1122.6E6	85.716	75.130

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
Data File : PD086841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 10:08
Operator : AR\AJ
Sample : P4847-02DL2 20X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:14:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

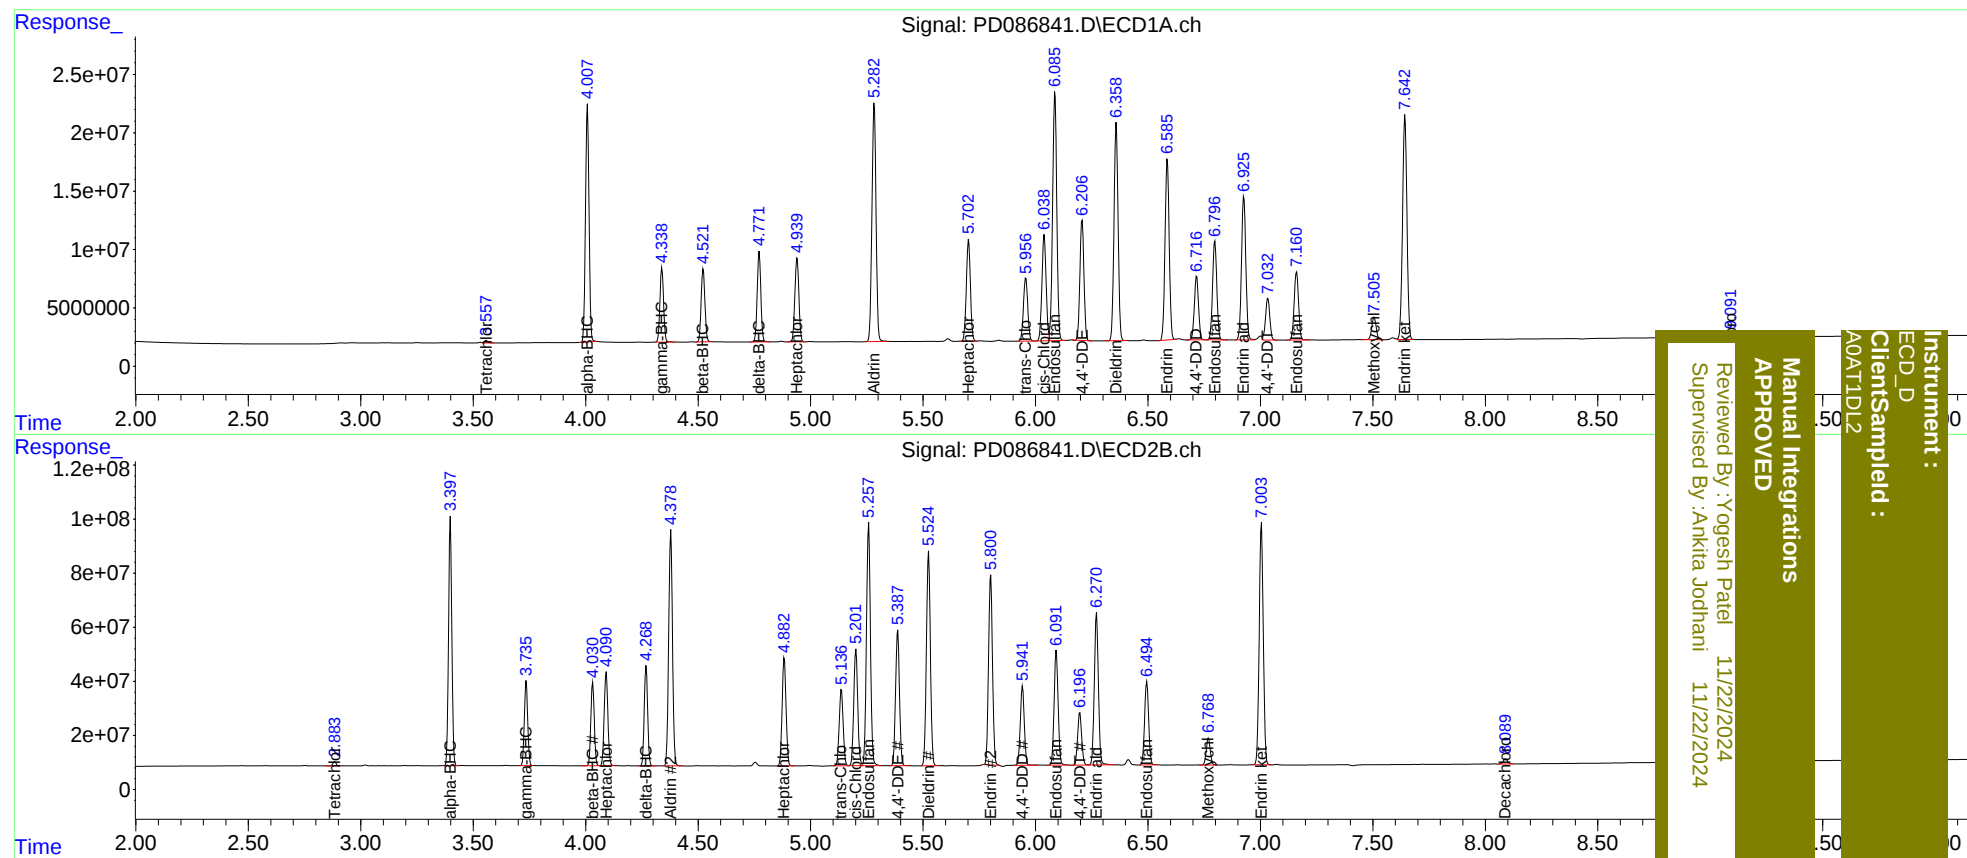

Instrument :
ECD_D
Client Sampled :
A0AT1DL2

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/22/2024
Supervised By : Ankita Jodhani 11/22/2024