

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
 Data File : PD086849.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 13:10
 Operator : AR\AJ
 Sample : P4872-06MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29X5MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:16:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.884	20453886	129.5E6	11.123m	11.219
27)	SA Decachlor...	9.095	8.091	28501347	133.8E6	10.705	10.496
Target Compounds							
2)	A alpha-BHC	4.009	3.399	192.3E6	908.6E6	54.610	50.732
3)	MA gamma-BHC...	4.340	3.736	187.8E6	777.9E6	53.931	46.641
4)	MA Heptachlor	4.941	4.092	193.8E6	765.0E6	55.758	44.470
5)	MB Aldrin	5.283	4.377	190.7E6	730.6E6	54.012	42.770m
6)	B beta-BHC	4.524	4.030	70346381	326.1E6	44.378	41.280m
7)	B delta-BHC	4.772	4.269	128.8E6	520.6E6	35.392	29.649
8)	B Heptachlo...	5.703	4.883	166.8E6	664.4E6	51.039	41.897
9)	A Endosulfan I	6.087	5.259	159.8E6	619.0E6	53.735	42.770
10)	B trans-Chl...	5.957	5.138	151.7E6	694.2E6	47.445	42.030
11)	B cis-Chlor...	6.039	5.202	168.2E6	701.4E6	51.689	43.769
12)	B 4,4'-DDE	6.208	5.388	315.2E6	1317.8E6	102.189	86.425
13)	MA Dieldrin	6.360	5.525	357.1E6	1371.4E6	108.942	89.757
14)	MA Endrin	6.587	5.801	299.7E6	1257.1E6	110.887	91.000
15)	B Endosulfa...	6.798	6.093	262.8E6	1182.9E6	94.718	84.768
16)	A 4,4'-DDD	6.717	5.943	255.2E6	1076.8E6	107.562	89.131
17)	MA 4,4'-DDT	7.033	6.197	275.3E6	1153.1E6	111.074m	89.192
18)	B Endrin al...	6.927	6.271	203.1E6	835.1E6	92.400	77.815
19)	B Endosulfa...	7.161	6.495	254.3E6	1206.1E6	94.255	89.880
20)	A Methoxychlor	7.506	6.770	686.4E6	2379.1E6	508.521	411.513
21)	B Endrin ke...	7.643	7.005	301.4E6	1232.5E6	98.800	82.485

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
Data File : PD086849.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 13:10
Operator : AR\AJ
Sample : P4872-06MS
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:16:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

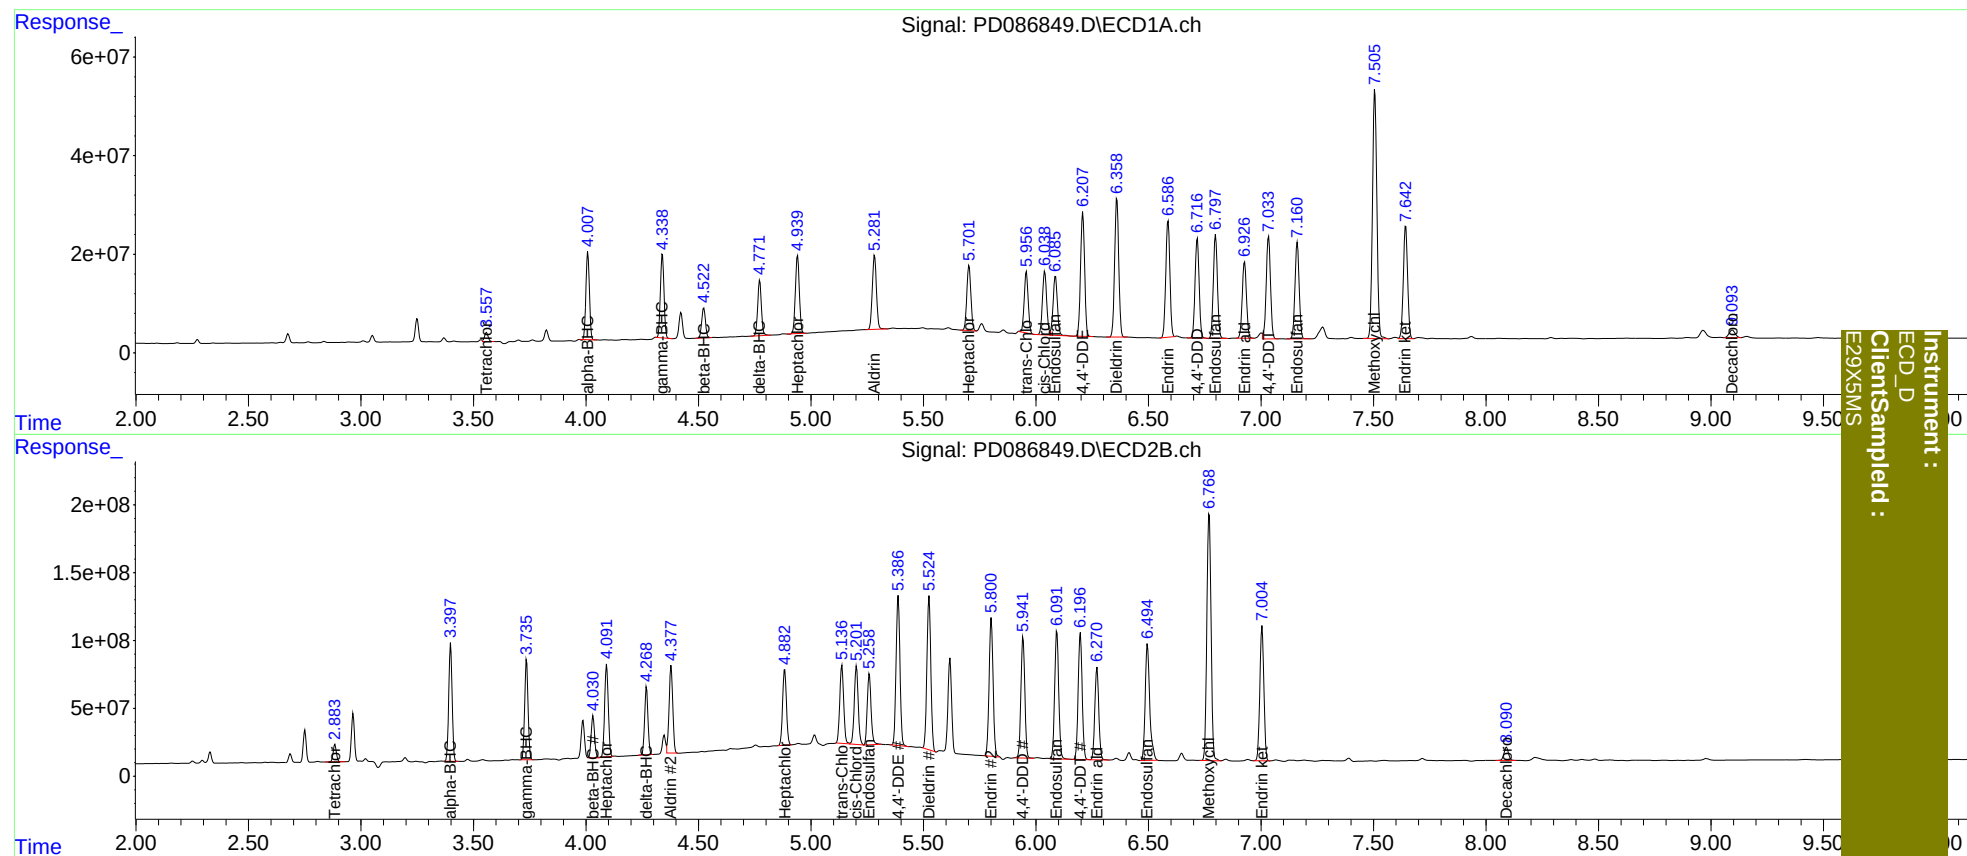

Instrument :
ECD_D
ClientSampled :
E29X5MS