

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
 Data File : PD086850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Nov 2024 13:38
 Operator : AR\AJ
 Sample : P4872-07MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29X5MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 00:16:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.557	2.885	21112519	127.3E6	11.481m	11.033
2)	SA Decachlor...	9.094	8.091	28010098	131.7E6	10.520	10.333
Target Compounds							
2)	A alpha-BHC	4.009	3.399	188.6E6	899.7E6	53.563	50.232
3)	MA gamma-BHC...	4.340	3.736	183.5E6	761.7E6	52.694	45.672
4)	MA Heptachlor	4.941	4.092	190.4E6	750.2E6	54.785	43.609
5)	MB Aldrin	5.283	4.378	186.8E6	722.3E6	52.904	42.283m
6)	B beta-BHC	4.524	4.030	69278452	323.6E6	43.704	40.957m
7)	B delta-BHC	4.773	4.269	126.6E6	512.7E6	34.797	29.198
8)	B Heptachlo...	5.703	4.884	163.7E6	651.3E6	50.098	41.070
9)	A Endosulfan I	6.087	5.259	157.0E6	608.9E6	52.819	42.073
10)	B trans-Chl...	5.958	5.137	148.1E6	675.2E6	46.312	40.880
11)	B cis-Chlor...	6.040	5.202	165.3E6	683.9E6	50.810	42.679
12)	B 4,4'-DDE	6.209	5.388	308.9E6	1291.6E6	100.150	84.710
13)	MA Dieldrin	6.361	5.525	349.7E6	1339.0E6	106.696	87.641
14)	MA Endrin	6.588	5.801	293.5E6	1236.2E6	108.590	89.483
15)	B Endosulfa...	6.799	6.093	255.2E6	1158.7E6	91.964	83.034
16)	A 4,4'-DDD	6.718	5.943	249.2E6	1058.6E6	105.052	87.623
17)	MA 4,4'-DDT	7.033	6.197	269.5E6	1130.4E6	108.710m	87.433
18)	B Endrin al...	6.927	6.272	192.1E6	795.2E6	87.381	74.098
19)	B Endosulfa...	7.162	6.496	249.7E6	1184.8E6	92.559	88.293
20)	A Methoxychlor	7.507	6.770	675.3E6	2364.4E6	500.356	408.965
21)	B Endrin ke...	7.644	7.005	295.7E6	1210.5E6	96.956	81.010

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
Data File : PD086850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Nov 2024 13:38
Operator : AR\AJ
Sample : P4872-07MSD
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 00:16:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

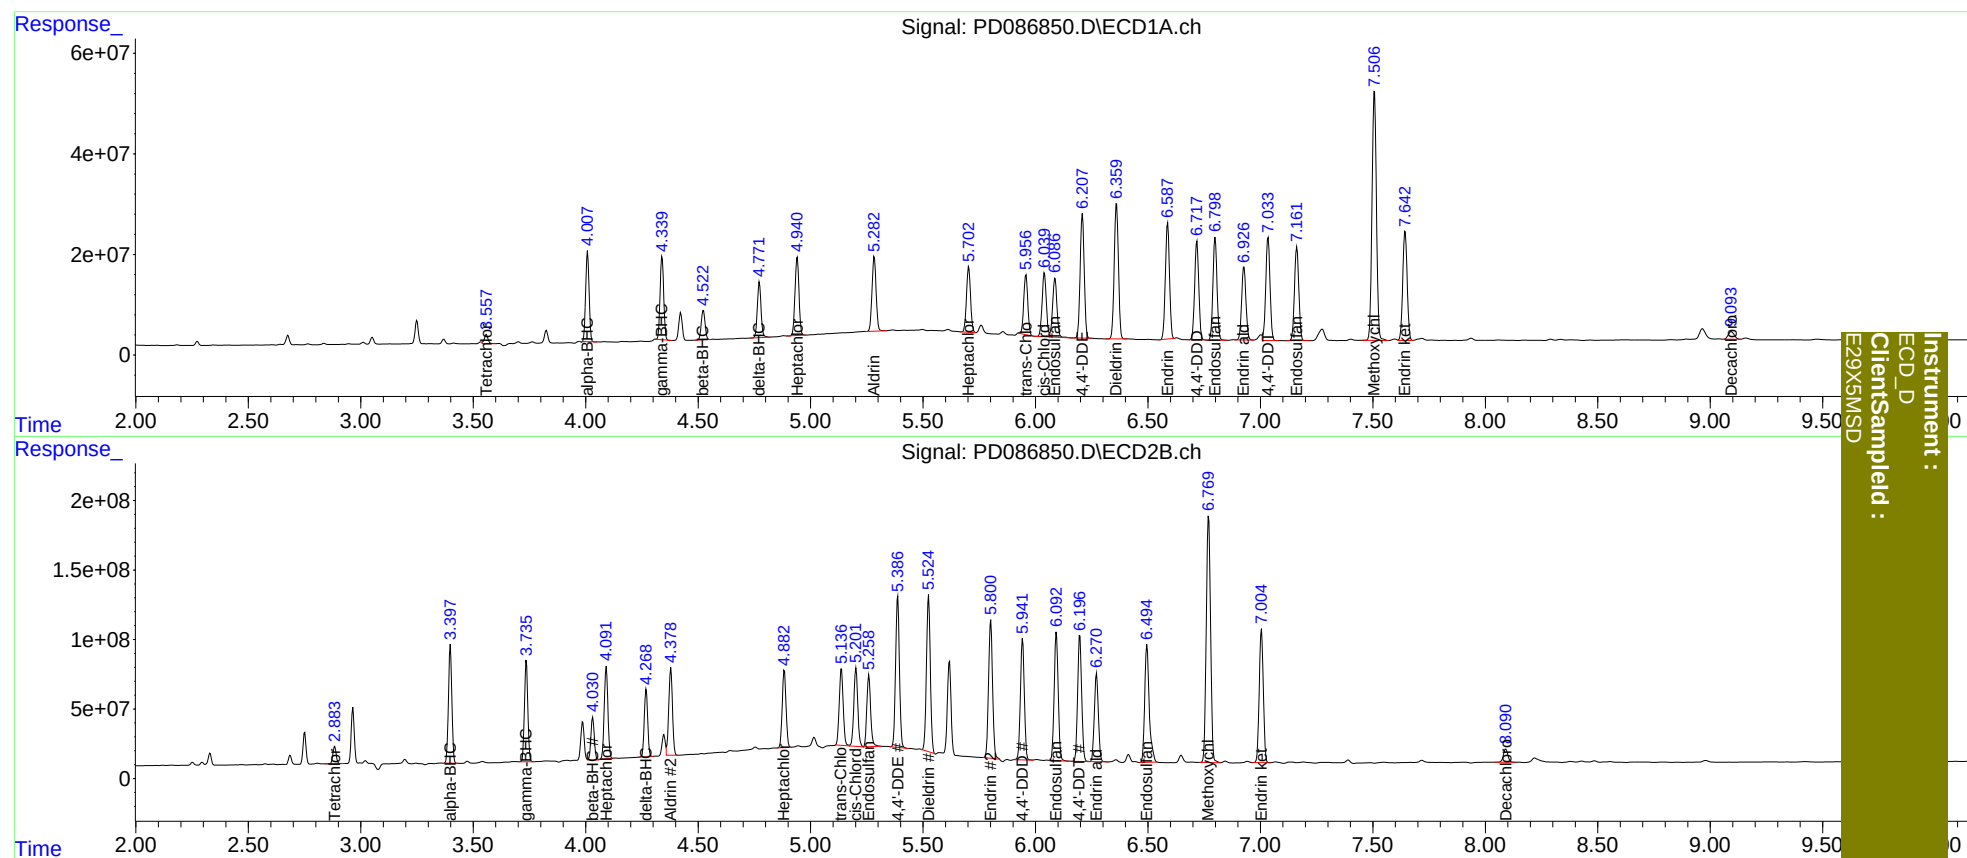

Instrument :
ECD_D
ClientSampled :
E29X5MSD