

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
 Data File : PD086877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 01:08
 Operator : AR\AJ
 Sample : P4872-06MS
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29X5MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 04:55:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.558	2.885	21974487	133.9E6	11.950m	11.605
2)	SA Decachlor...	9.096	8.092	29554396	143.5E6	11.100	11.258
Target Compounds							
2)	A alpha-BHC	4.010	3.399	205.3E6	887.8E6	58.310	49.570
3)	MA gamma-BHC...	4.341	3.737	195.7E6	826.2E6	56.192	49.538
4)	MA Heptachlor	4.942	4.092	195.3E6	806.8E6	56.210	46.902
5)	MB Aldrin	5.284	4.379	198.1E6	811.6E6	56.100	47.510
6)	B beta-BHC	4.524	4.032	73267899	351.1E6	46.221	44.440
7)	B delta-BHC	4.774	4.269	132.8E6	567.3E6	36.479	32.311
8)	B Heptachlo...	5.705	4.884	175.6E6	736.5E6	53.721	46.441
9)	A Endosulfan I	6.088	5.259	165.3E6	686.3E6	55.581	47.418
10)	B trans-Chl...	5.959	5.138	163.0E6	768.3E6	50.975	46.512
11)	B cis-Chlor...	6.040	5.202	176.2E6	756.7E6	54.172	47.218
12)	B 4,4'-DDE	6.210	5.388	327.8E6	1434.5E6	106.269	94.082
13)	MA Dieldrin	6.361	5.525	372.7E6	1470.3E6	113.697	96.233
14)	MA Endrin	6.588	5.802	304.4E6	1334.2E6	112.602	96.579
15)	B Endosulfa...	6.800	6.094	282.7E6	1255.0E6	101.870	89.934
16)	A 4,4'-DDD	6.718	5.943	275.5E6	1186.2E6	116.145	98.185
17)	MA 4,4'-DDT	7.034	6.198	257.7E6	1139.7E6	103.958m	88.150
18)	B Endrin al...	6.928	6.272	215.8E6	913.0E6	98.184	85.074
19)	B Endosulfa...	7.163	6.496	262.4E6	1273.4E6	97.254	94.900
20)	A Methoxychlor	7.508	6.771	661.8E6	2426.9E6	490.355	419.775
21)	B Endrin ke...	7.645	7.006	312.1E6	1302.1E6	102.310	87.142

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112124\
Data File : PD086877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 01:08
Operator : AR\AJ
Sample : P4872-06MS
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 04:55:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

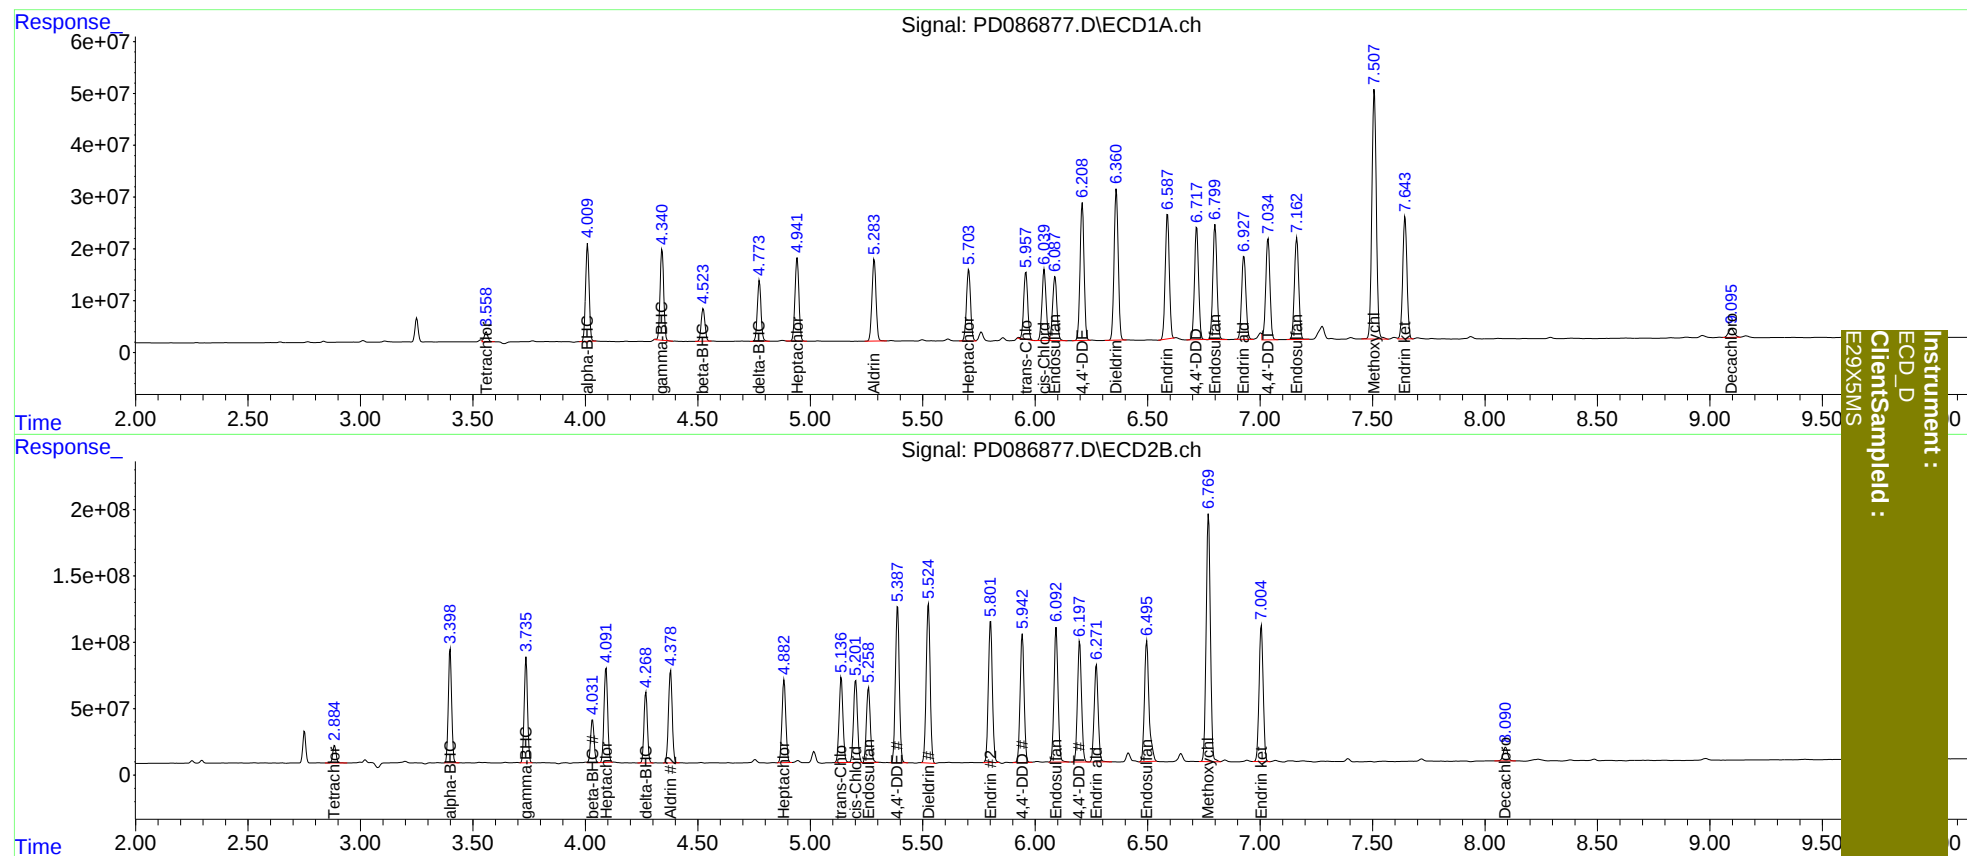

Instrument :
ECD_D
ClientSampled :
E29X5MS