

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112125\
 Data File : PD091343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2025 14:21
 Operator : AR\AJ
 Sample : Q3697-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 MOO-25-0332

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/26/2025
 Supervised By :mohammad ahmed 11/26/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 00:48:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 15 04:46:13 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.871	47760124	553.5E6	13.849m	15.112m
28) SA Decachlor...	9.060	8.056	85728846	604.2E6	17.208	15.266

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112125\
Data File : PD091343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2025 14:21
Operator : AR\AJ
Sample : Q3697-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
MOO-25-0332


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/26/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 00:48:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111525.M
Quant Title : GC Extractables
QLast Update : Sat Nov 15 04:46:13 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

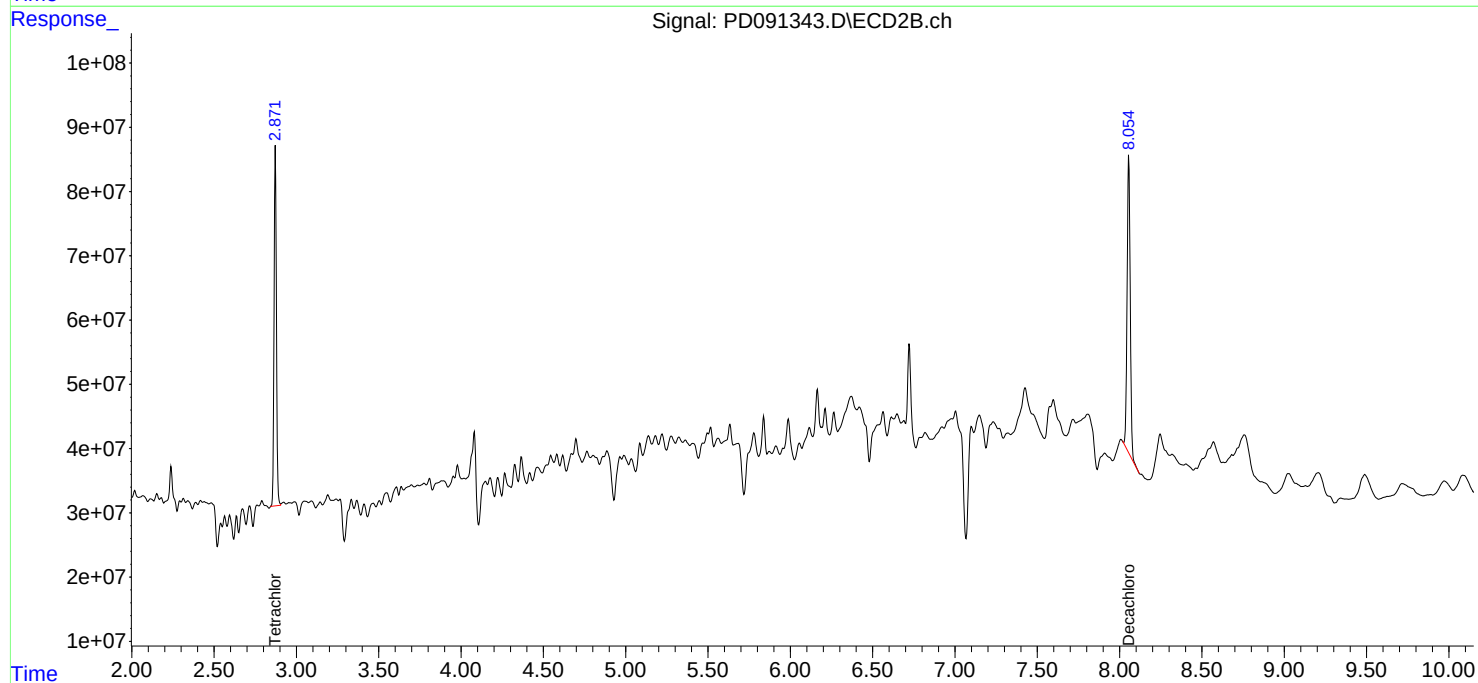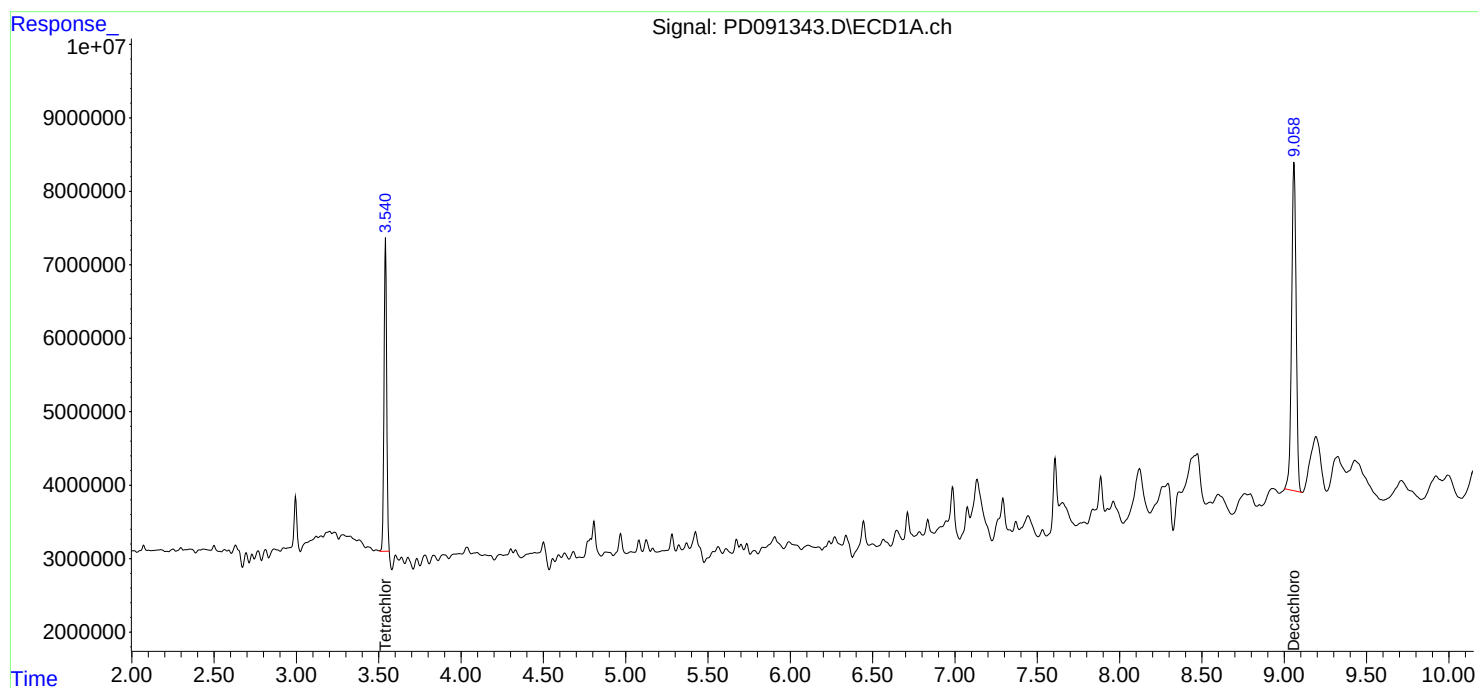

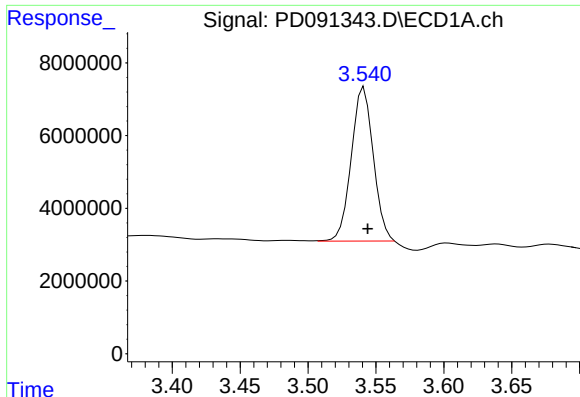


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 47760124
Conc: 13.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
MOO-25-0332


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/26/2025
Supervised By :mohammad ahmed 11/26/2025

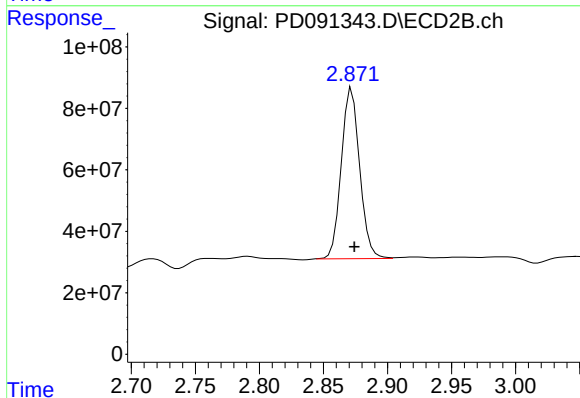


#1 Tetrachloro-m-xylene

R.T.: 2.871 min
Delta R.T.: -0.003 min
Response: 553549083
Conc: 15.11 ng/ml m

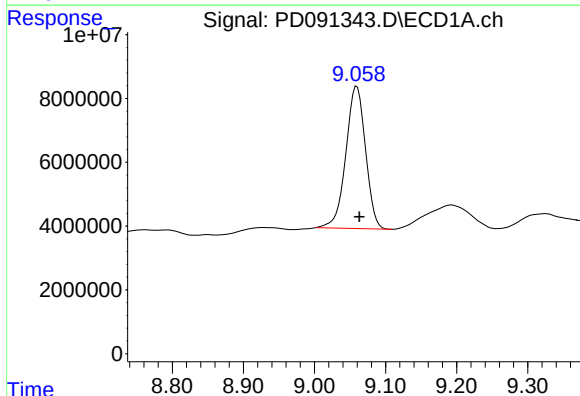

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: -0.004 min
Response: 85728846
Conc: 17.21 ng/ml

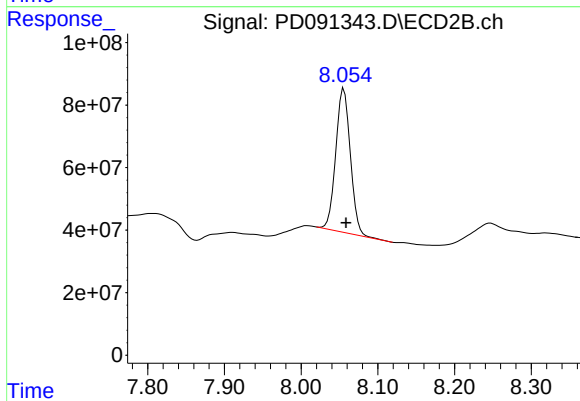

#28 Decachlorobiphenyl

R.T.: 8.056 min
Delta R.T.: -0.003 min
Response: 604156630
Conc: 15.27 ng/ml