

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112219\
 Data File : PD056184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 21:46
 Operator : SG\AJ
 Sample : PIBLK38
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK38

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 22:24:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	16892670	24210974	22.441	23.103
27)	SA Decachlor...	7.963	8.998	36316520	44739925	44.554	39.399
Target Compounds							
6)	B beta-BHC	0.000	4.849f	0	673623	N.D.	0.963
16)	A 4,4'-DDD	0.000	6.737f	0	361626	N.D.	0.324


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112219\
Data File : PD056184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 21:46
Operator : SG\AJ
Sample : PIBLK38
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK38

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 22:24:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

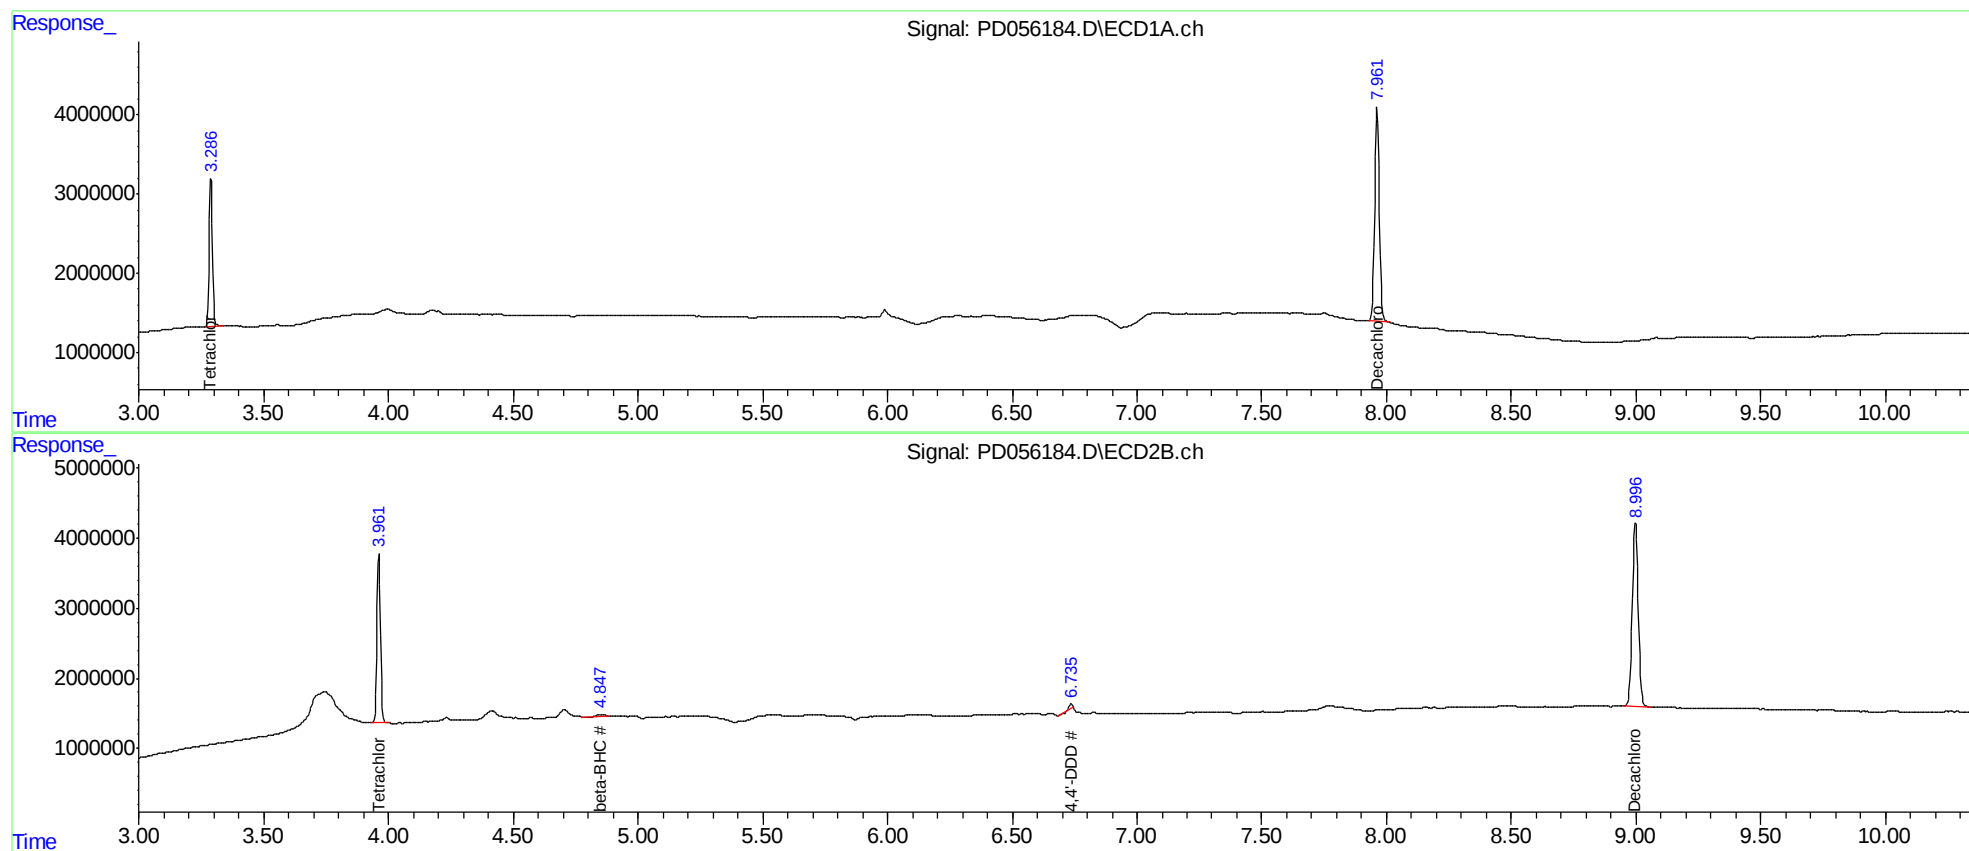


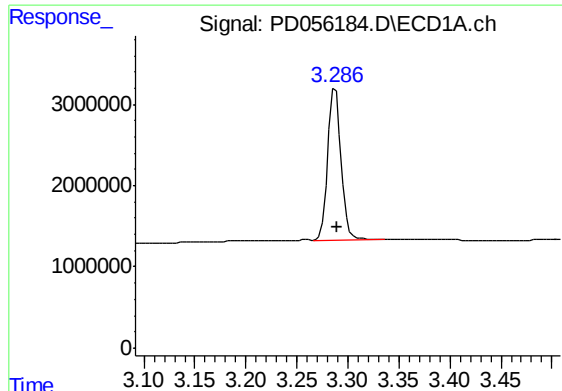

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: -0.001 min
Response: 16892670
Conc: 22.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK38

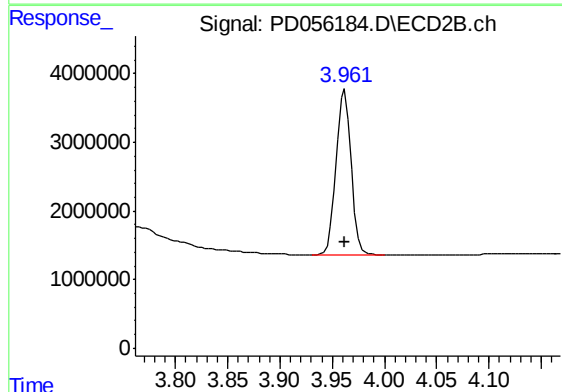


#1 Tetrachloro-m-xylene

R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 24210974
Conc: 23.10 ng/ml

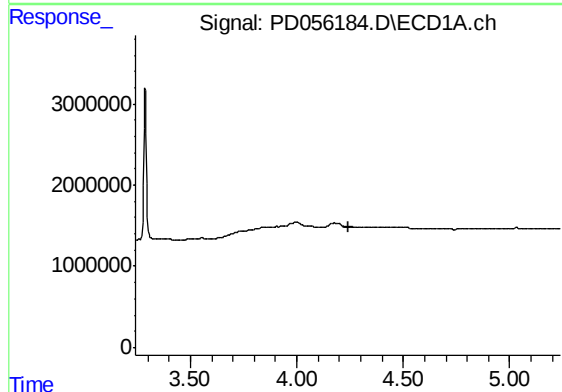


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.240 min
Response: 0
Conc: N.D.

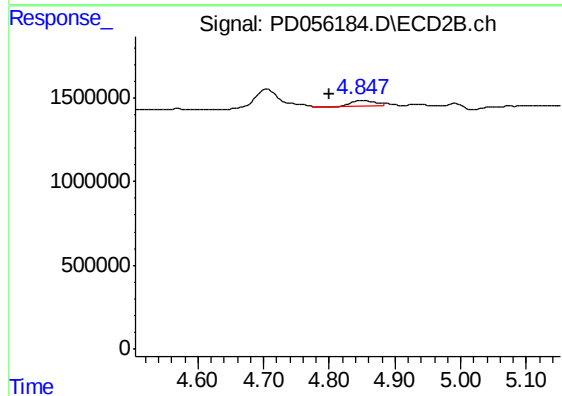

#6 beta-BHC


R.T.: 4.849 min
Delta R.T.: 0.050 min
Response: 673623
Conc: 0.96 ng/ml

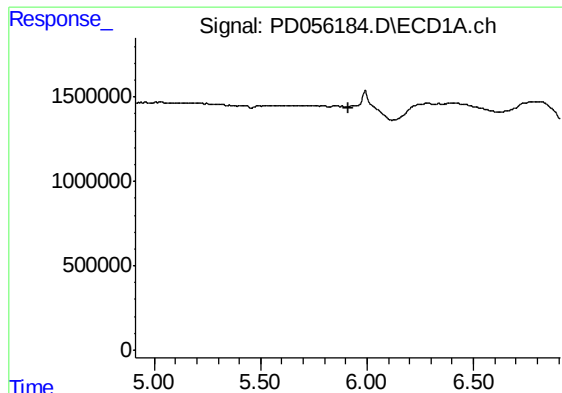

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
PIBLK38

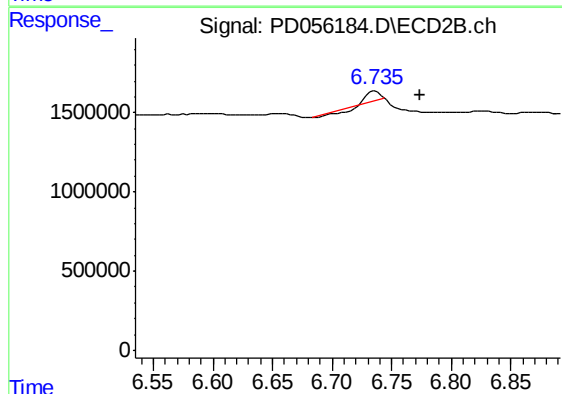


#16 4,4'-DDD

R.T.: 6.737 min
Delta R.T.: -0.038 min
Response: 361626
Conc: 0.32 ng/ml

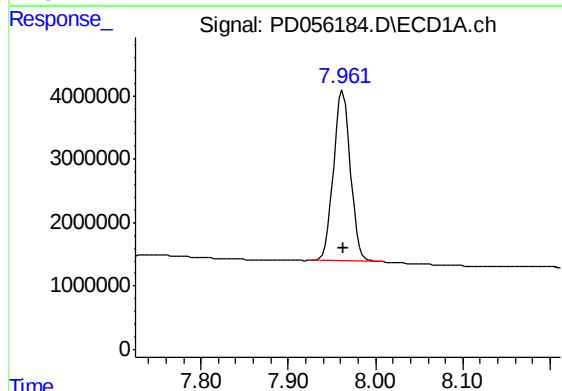

#27 Decachlorobiphenyl

R.T.: 7.963 min
Delta R.T.: 0.000 min
Response: 36316520
Conc: 44.55 ng/ml

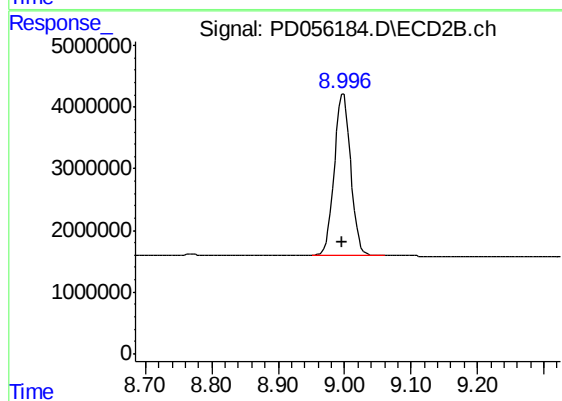

#27 Decachlorobiphenyl

R.T.: 8.998 min
Delta R.T.: 0.001 min
Response: 44739925
Conc: 39.40 ng/ml