

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112219\
 Data File : PD056172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 18:57
 Operator : SG\AJ
 Sample : K5889-07MS
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 JLLQ1MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 22:21:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.962	10352671	15521402	13.753	14.811
27)	SA Decachlor...	7.963	9.000	13143637	15351702	16.125	13.519
Target Compounds							
3)	MA gamma-BHC...	3.990	4.632	57107926	79646190	55.832	56.532
4)	MA Heptachlor	4.276	5.138	52496100	78938911	55.445	54.278
5)	MB Aldrin	4.515	5.441	50556776	74577588	54.569	54.352
13)	MA Dieldrin	5.523	6.436	105.1E6	156.0E6	111.785	110.345
14)	MA Endrin	5.776	6.653	92891319	134.3E6	115.791	116.683
17)	MA 4,4'-DDT	6.146	7.073	80326971	123.3E6	123.957	113.385

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112219\
Data File : PD056172.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 18:57
Operator : SG\AJ
Sample : K5889-07MS
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 22:21:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

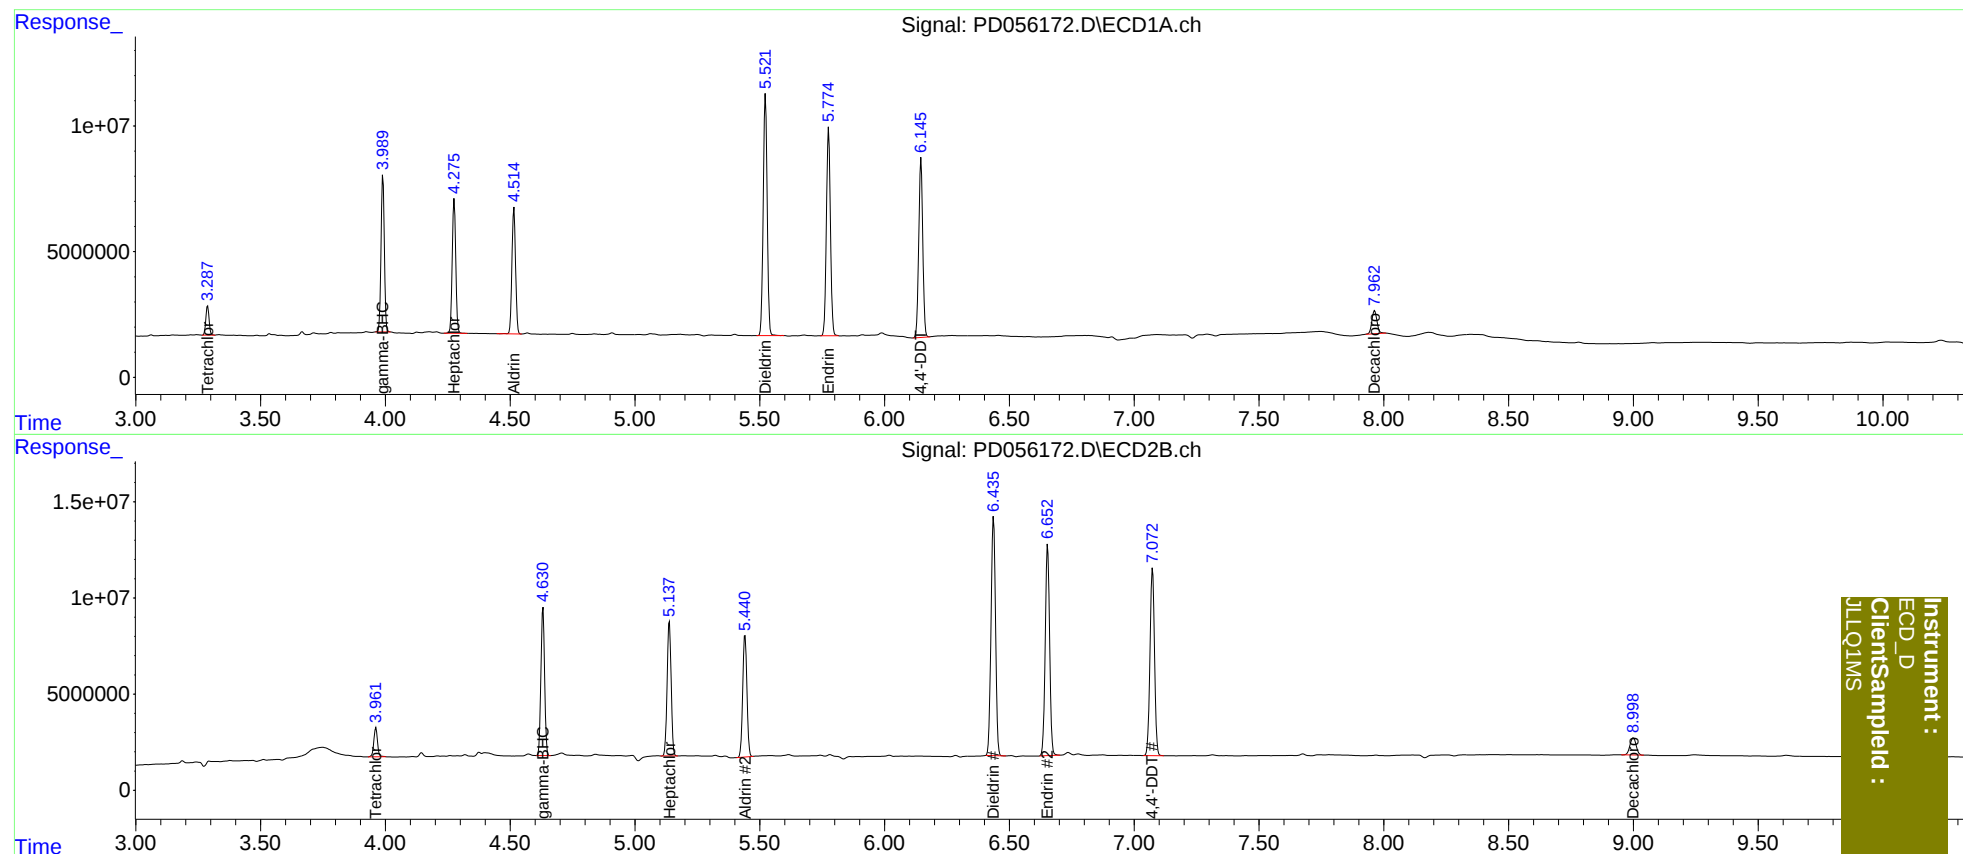

Instrument :
ECD_D
ClientSampled :
JLLO1MS