

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112219\
 Data File : PD056164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2019 16:54
 Operator : SG\AJ
 Sample : PB124972BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS72

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 22:19:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 02 07:20:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.293	3.961	14301078	21483430	18.998	20.500
27)	SA Decachlor...	7.969	9.000	30690811	39609760	37.652	34.881
Target Compounds							
3)	MA gamma-BHC...	3.996	4.631	41982983	63077452	41.045	44.772
8)	B Heptachlo...	4.958	5.826	42552827	64436285	47.659	47.747
10)	B trans-Chl...	5.180	6.059	43836744	67207443	48.345	47.115
12)	B 4,4'-DDE	5.406	6.289	88214663	134.3E6	101.463	99.673
13)	MA Dieldrin	5.529	6.437	90767838	139.1E6	96.500	98.368
14)	MA Endrin	5.782	6.654	79107058	119.4E6	98.609	103.707
19)	B Endosulfa...	6.435	7.209	47761571	72759052	60.872	60.349

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112219\
Data File : PD056164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2019 16:54
Operator : SG\AJ
Sample : PB124972BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 22:19:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110319CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 02 07:20:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

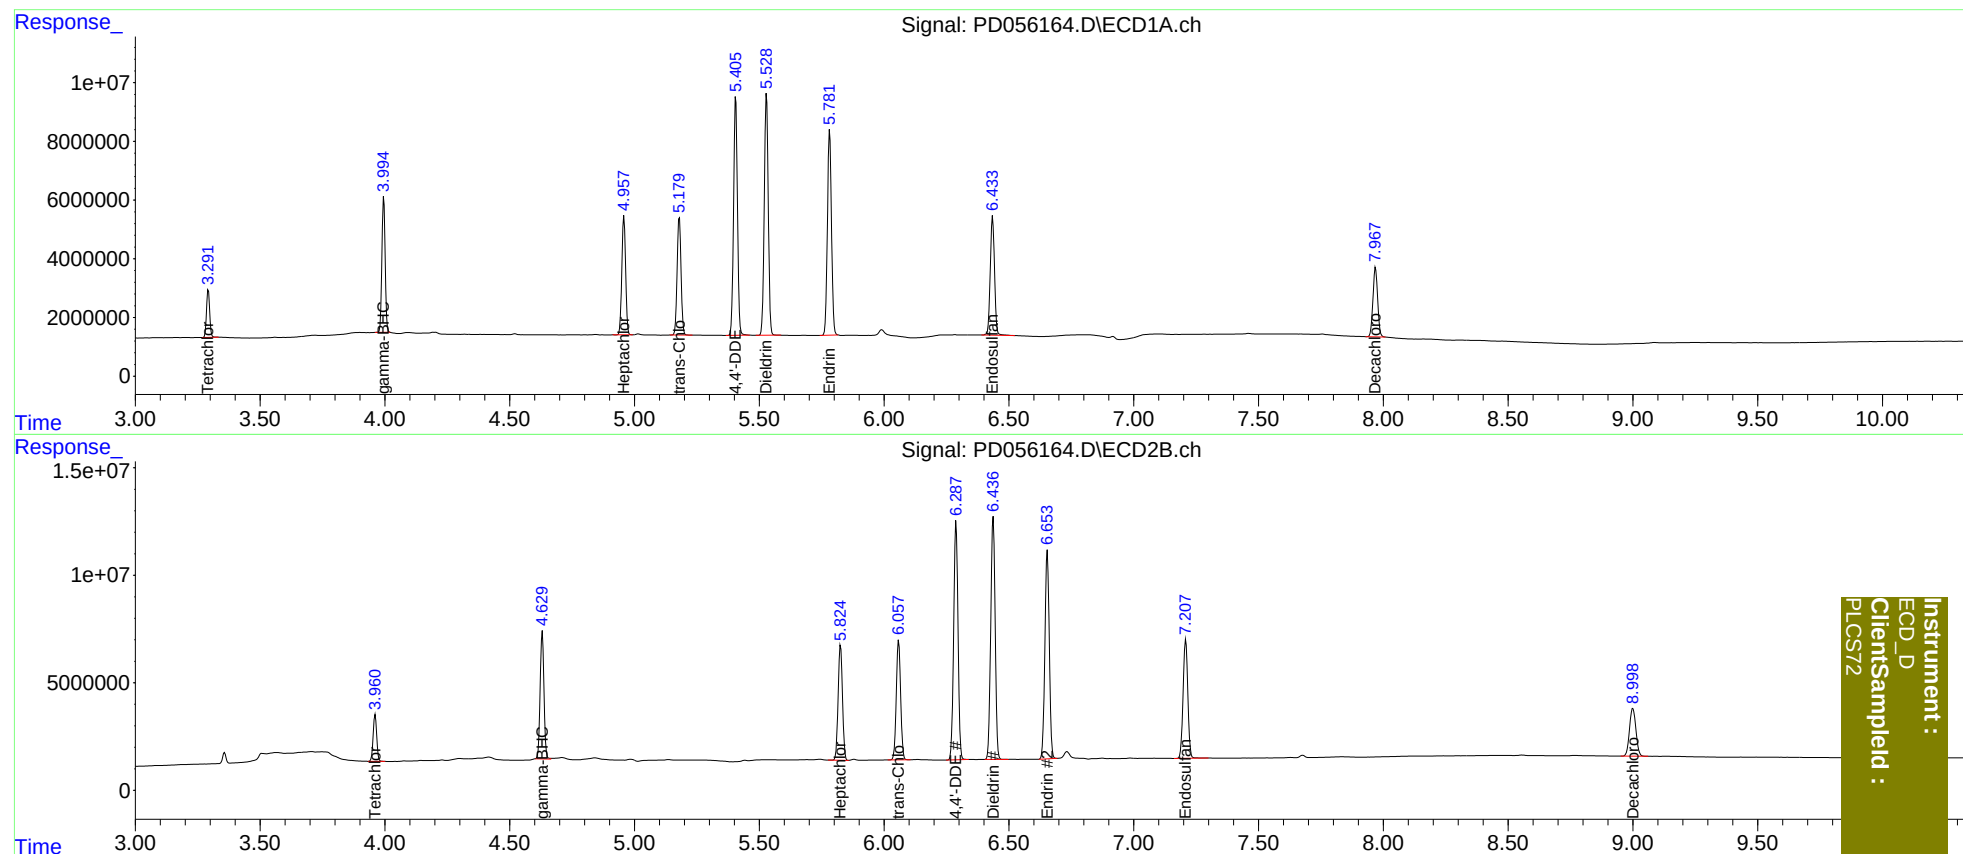

Instrument :
ECD_D
ClientSampled :
PLC572