

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112222\
 Data File : PD073183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 15:16
 Operator : AR\AJ
 Sample : N4955-07
 Misc : TOX LOD 50PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/23/2022
 Supervised By :Ankita Jodhani 11/23/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 01:14:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111622.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 21 09:25:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.706	3.459	40493556	1209.1E6	19.114	21.952
7) SA Decachlor...	7.836	8.914	43274752	286.4E6	21.070	22.062
Target Compounds						
2) Toxaphene-1	5.254	5.766	725358	5616829	49.044	42.546
3) Toxaphene-2	5.611	6.145	931712	11474886	59.689	50.348
4) Toxaphene-3	6.527	7.056	2034170	26692647	45.871	60.395 #
5) Toxaphene-4	6.655	7.144	5326522	19069411	70.706m	58.742
6) Toxaphene-5	6.967	7.842	2283406	18454968	54.107	56.220

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112222\
Data File : PD073183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 15:16
Operator : AR\AJ
Sample : N4955-07
Misc : TOX LOD 50PPB
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 01:14:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111622.M
Quant Title : GC Extractables
QLast Update : Mon Nov 21 09:25:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

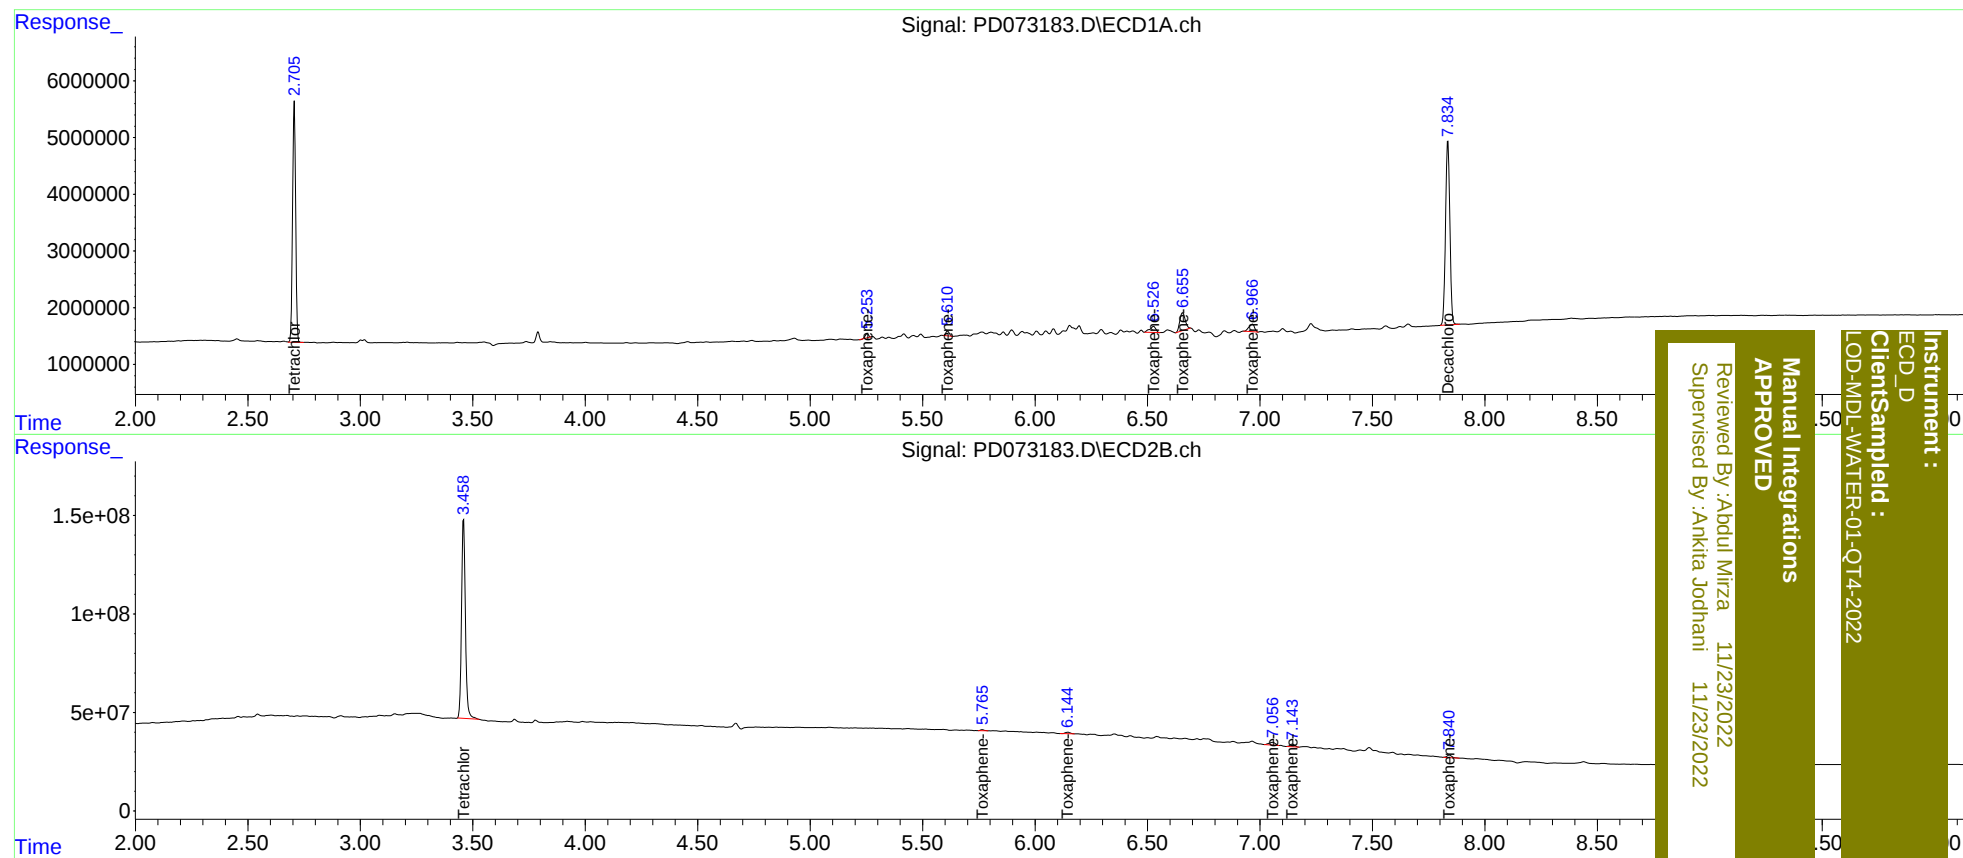

Reviewed By: Abdul Mirza 11/23/2022
Supervised By: Ankita Jodhani 11/23/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
LOD-MDL-WATER-01-QT4-2022