

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112222\
 Data File : PD073188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2022 17:35
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 23 01:14:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111622.M
 Quant Title : GC Extractables
 QLast Update : Mon Nov 21 09:25:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.703	3.458	102.0E6	2855.3E6	48.162	51.838
7) SA Decachlor...	7.830	8.910	102.1E6	691.1E6	49.688	53.239
Target Compounds						
2) Toxaphene-1	5.248	5.765	7088386	68977994	479.273	522.489
3) Toxaphene-2	5.607	6.142	8074286	123.2E6	517.268	540.418
4) Toxaphene-3	6.521	7.055	24873510	250.2E6	560.898	566.125
5) Toxaphene-4	6.651	7.141	41076577	179.8E6	545.264	553.716
6) Toxaphene-5	6.961	7.838	23899026	187.7E6	566.304	571.913

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112222\
Data File : PD073188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2022 17:35
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 23 01:14:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX111622.M
Quant Title : GC Extractables
QLast Update : Mon Nov 21 09:25:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

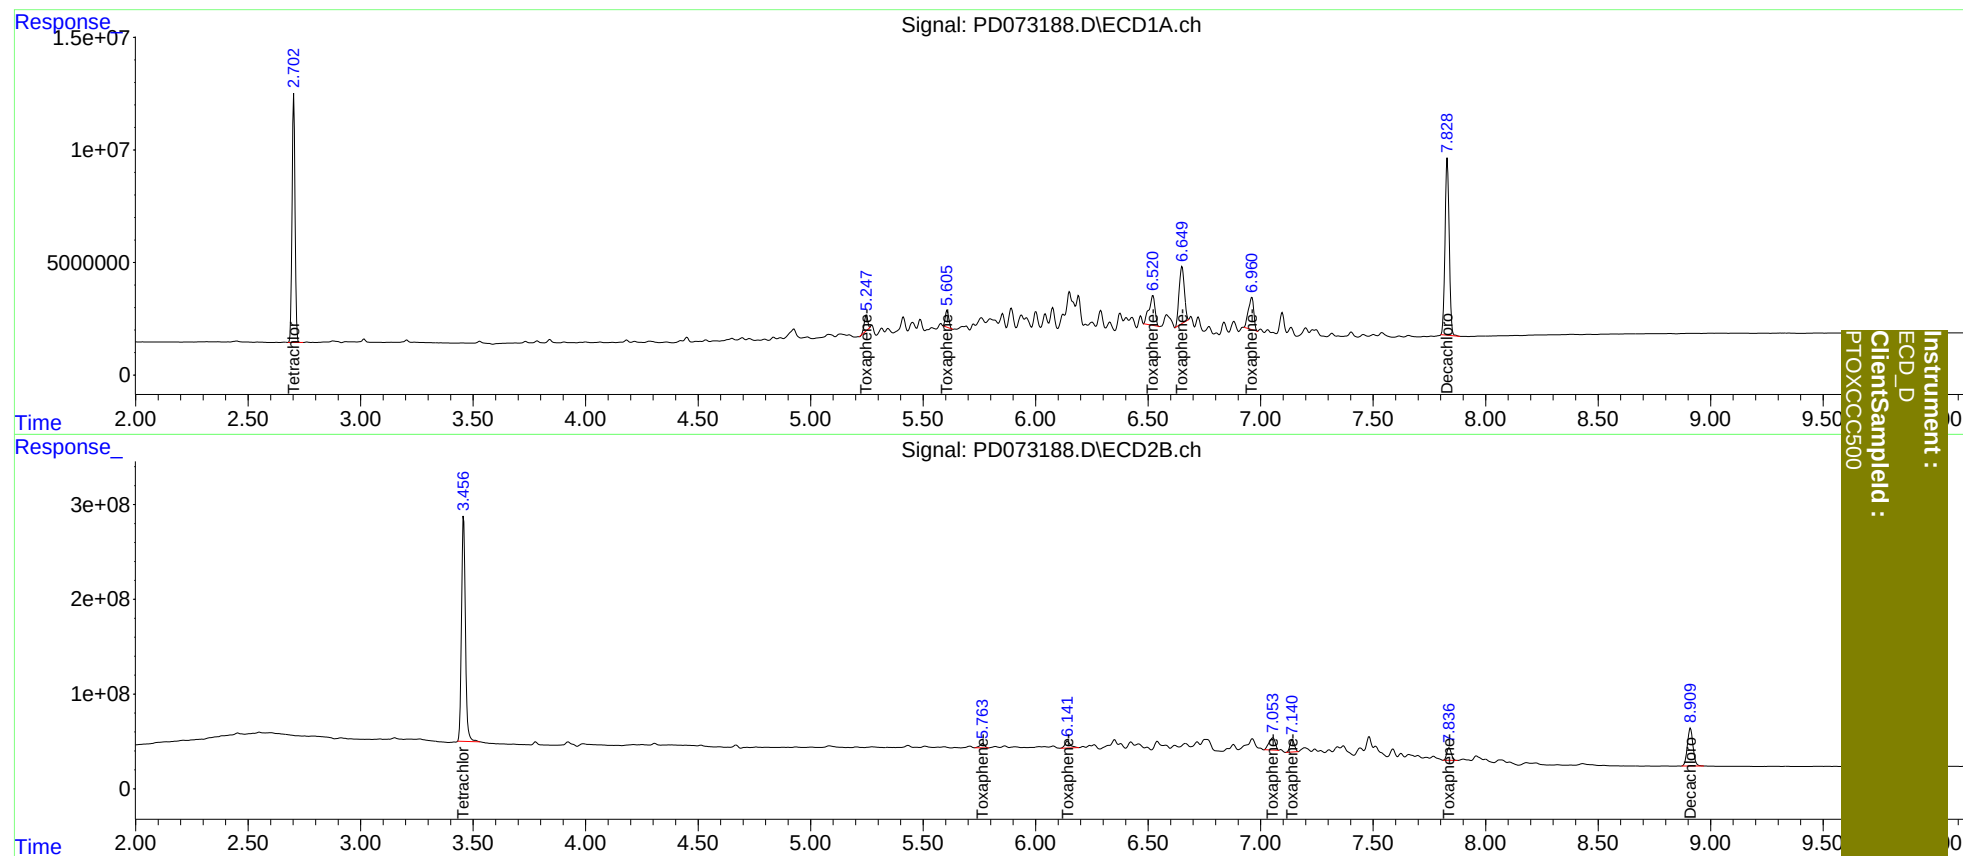

Instrument :
ECD_D
ClientSampled :
PTOXCCC500