

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
 Data File : PD079813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2023 17:00
 Operator : AR\AJ
 Sample : 05455-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:37:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	29508196	47384960	20.206	20.717
27)	SA Decachlor...	9.119	7.948	41758016	57035133	23.532	23.889
Target Compounds							
5)	MB Aldrin	0.000	4.227f	0	454293	N.D.	0.140
8)	B Heptachlo...	0.000	4.831f	0	612680	N.D.	0.198
9)	A Endosulfan I	0.000	5.166	0	286130	N.D.	0.103
10)	B trans-Chl...	0.000	4.943f	0	508588	N.D.	0.171
14)	MA Endrin	0.000	5.686	0	425542	N.D.	0.155
15)	B Endosulfa...	6.806	5.923f	6166279	1075322	3.241	0.414 #
16)	A 4,4'-DDD	6.806f	0.000	6166279	0	3.807	N.D. #
18)	B Endrin al...	0.000	6.159	0	1038281	N.D.	0.513
21)	B Endrin ke...	0.000	6.907f	0	96754	N.D.	<MDL
26)	Toxaphene-5	0.000	7.035f	0	222489	N.D.	6.664


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
Data File : PD079813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2023 17:00
Operator : AR\AJ
Sample : 05455-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:37:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

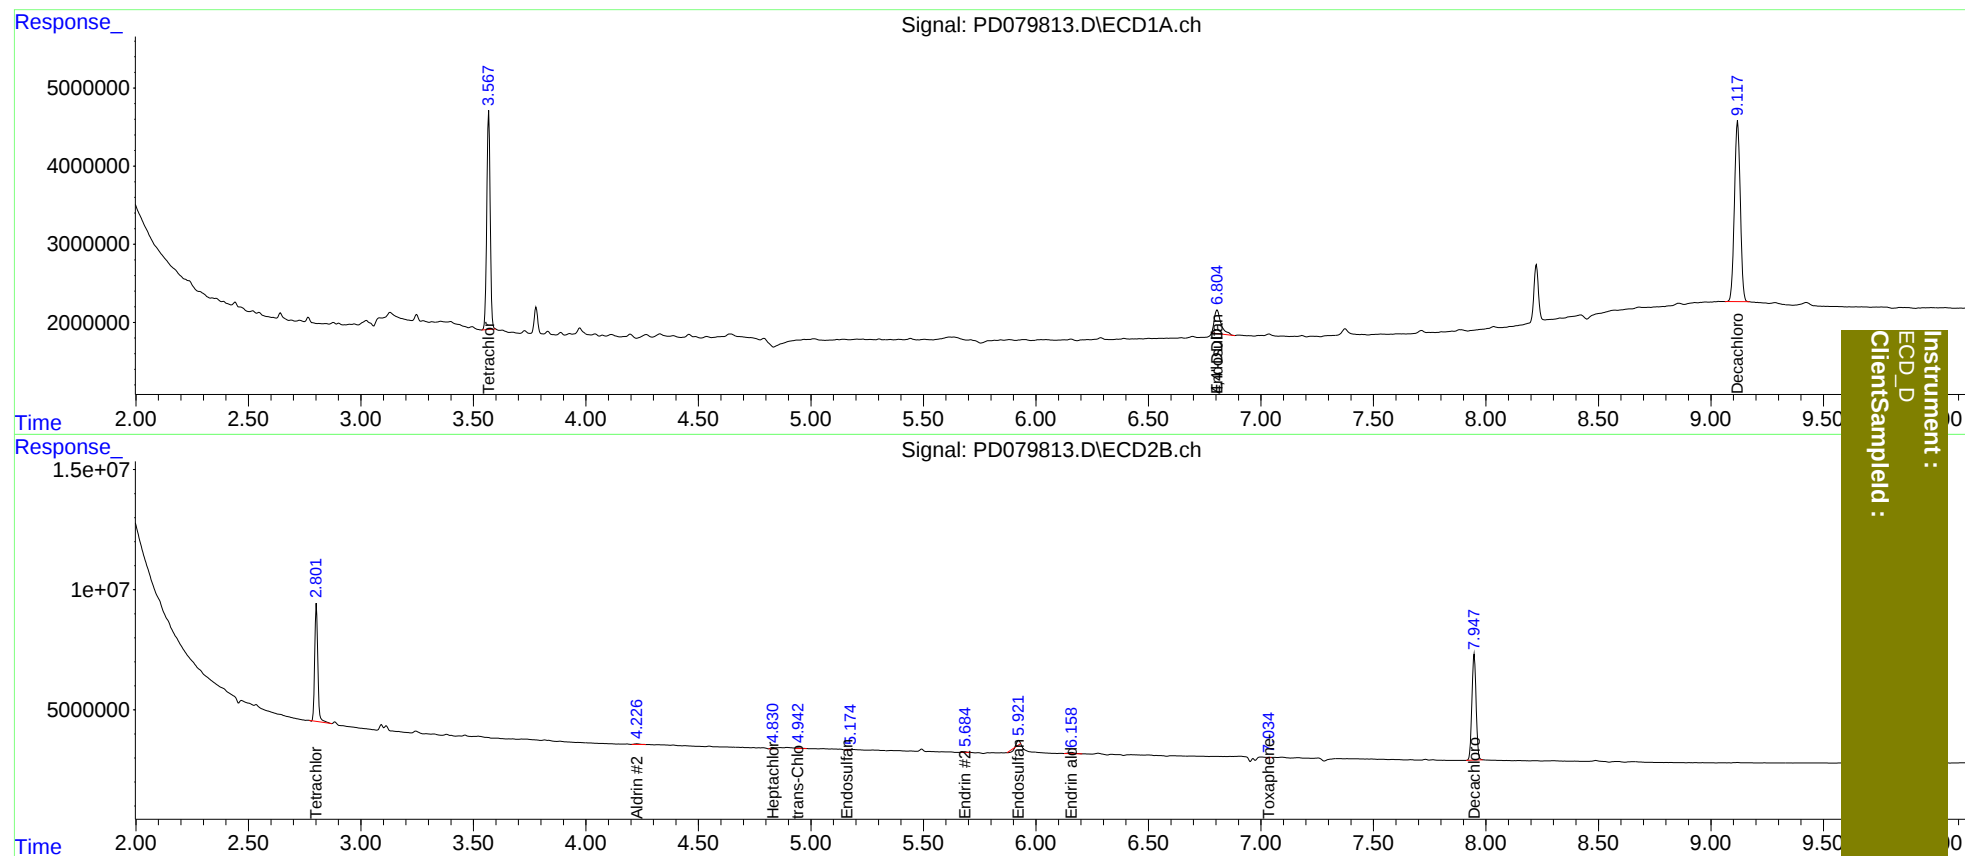


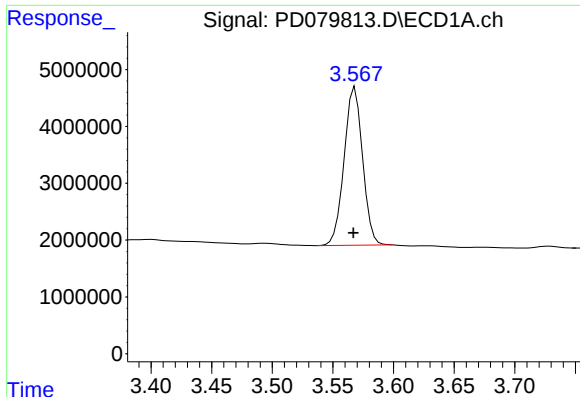

#1 Tetrachloro-m-xylene


R.T.: 3.568 min
Delta R.T.: 0.001 min
Response: 29508196
Conc: 20.21 ng/ml

Instrument :
ECD_D
ClientSampleId :

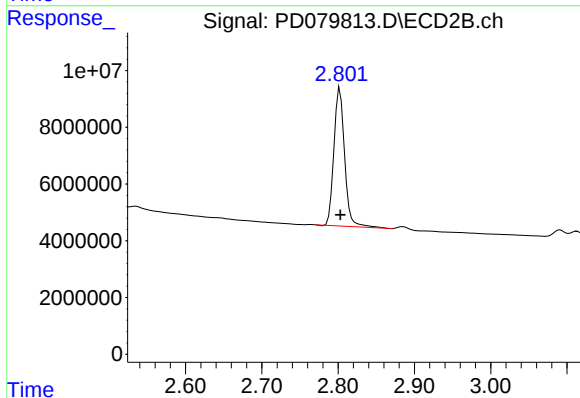


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: 0.000 min
Response: 47384960
Conc: 20.72 ng/ml

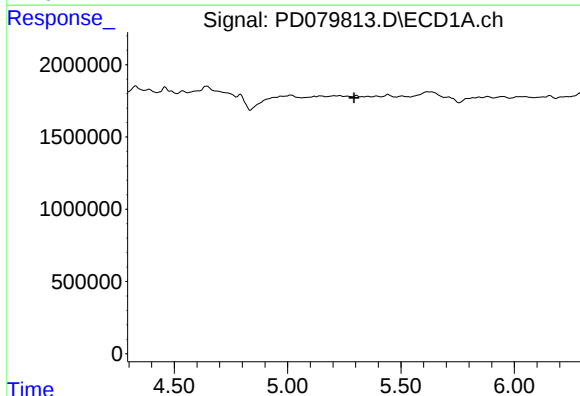


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.294 min
Response: 0
Conc: N.D.

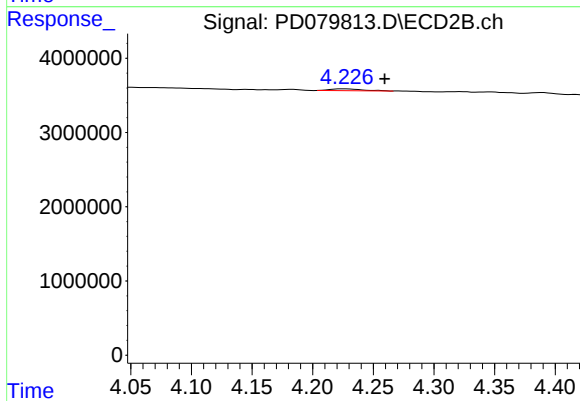

#5 Aldrin


R.T.: 4.227 min
Delta R.T.: -0.033 min
Response: 454293
Conc: 0.14 ng/ml

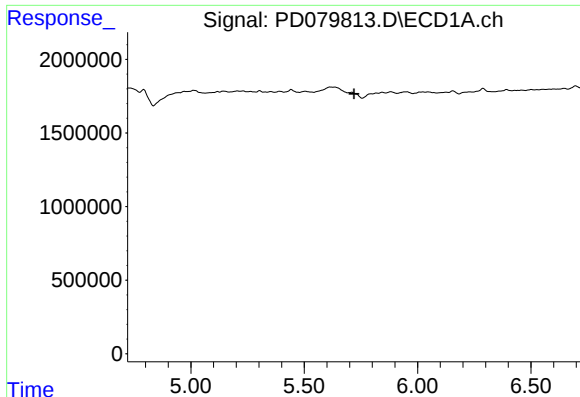

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.720 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

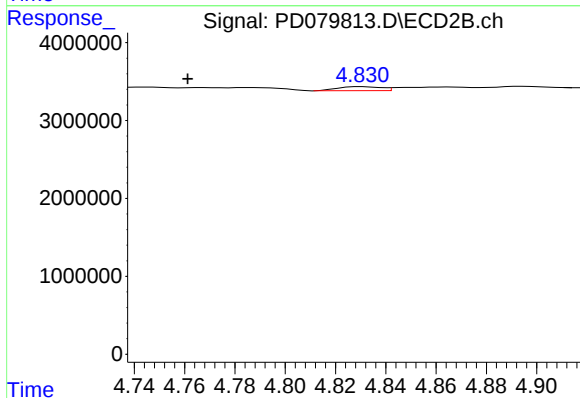


#8 Heptachlor epoxide

R.T.: 4.831 min
Delta R.T.: 0.070 min
Response: 612680
Conc: 0.20 ng/ml

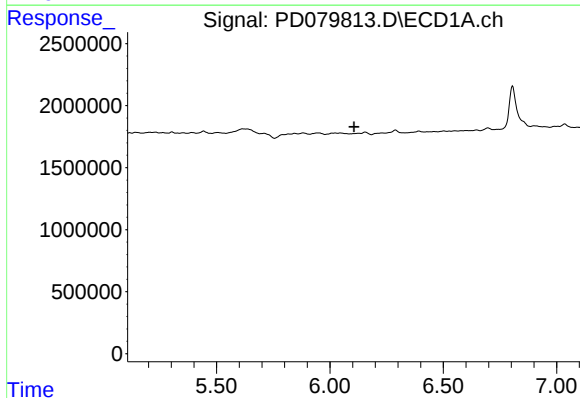


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.106 min
Response: 0
Conc: N.D.

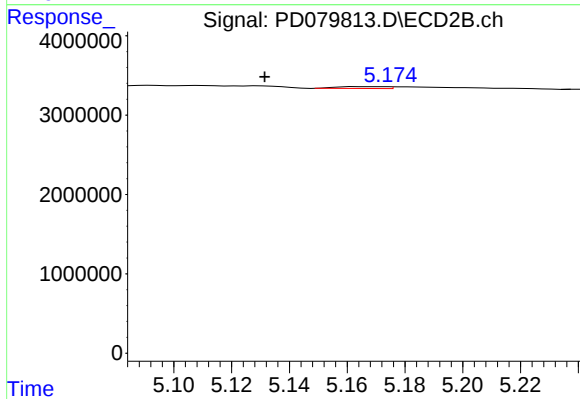

#9 Endosulfan I


R.T.: 5.166 min
Delta R.T.: 0.035 min
Response: 286130
Conc: 0.10 ng/ml

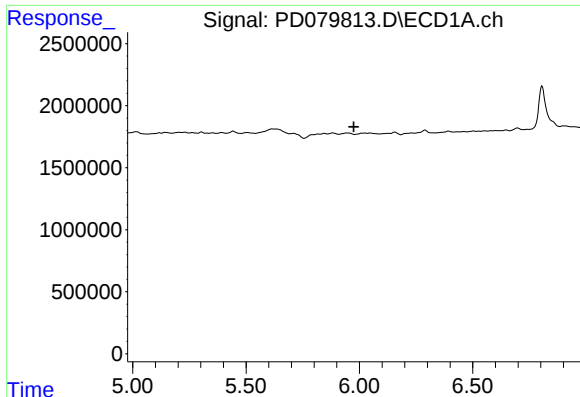

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

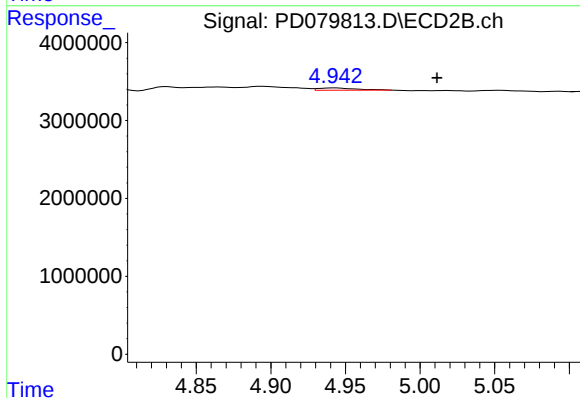


#10 trans-Chlordane

R.T.: 4.943 min
Delta R.T.: -0.068 min
Response: 508588
Conc: 0.17 ng/ml

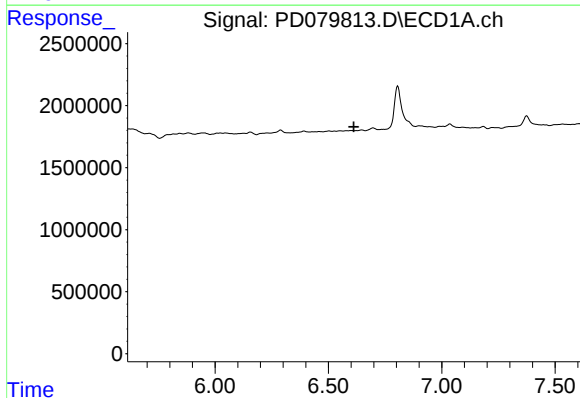


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

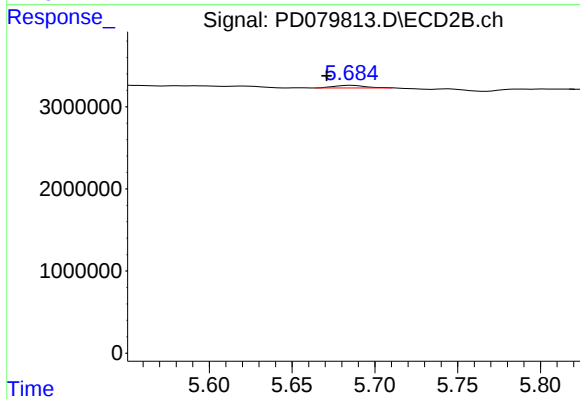

#14 Endrin


R.T.: 5.686 min
Delta R.T.: 0.015 min
Response: 425542
Conc: 0.16 ng/ml

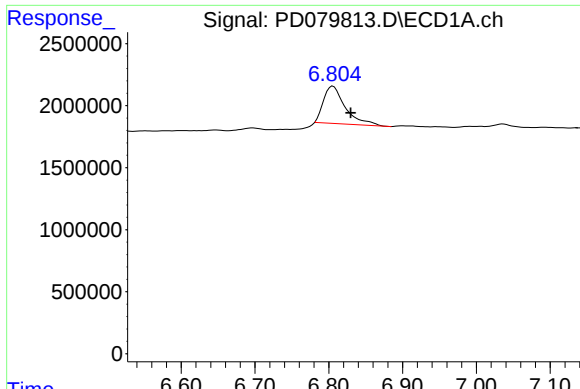

#15 Endosulfan II


R.T.: 6.806 min
Delta R.T.: -0.024 min
Response: 6166279
Conc: 3.24 ng/ml

Instrument :
ECD_D
ClientSampleId :

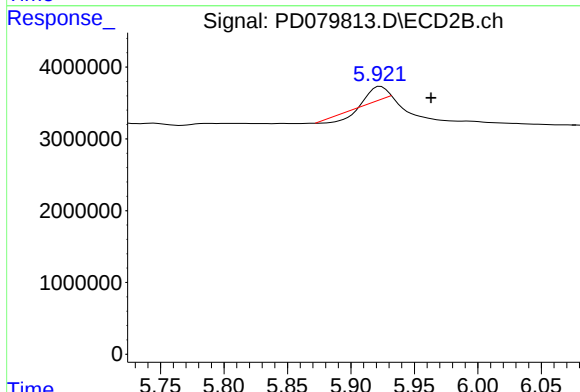


#15 Endosulfan II

R.T.: 5.923 min
Delta R.T.: -0.040 min
Response: 1075322
Conc: 0.41 ng/ml

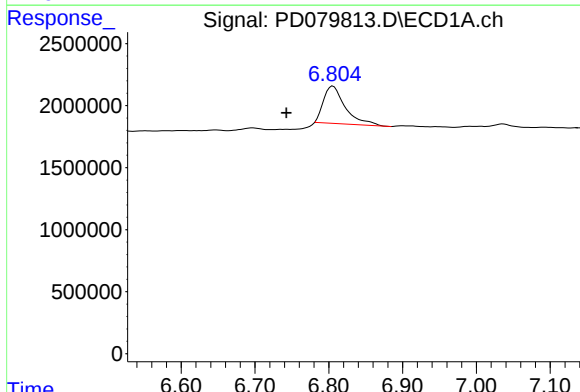


#16 4,4'-DDD

R.T.: 6.806 min
Delta R.T.: 0.063 min
Response: 6166279
Conc: 3.81 ng/ml

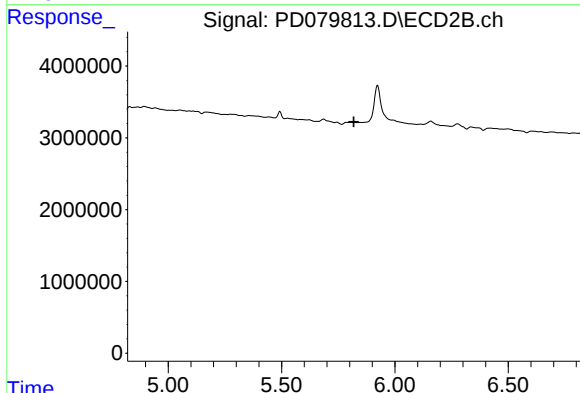

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T. : 5.818 min
Response: 0
Conc: N.D.

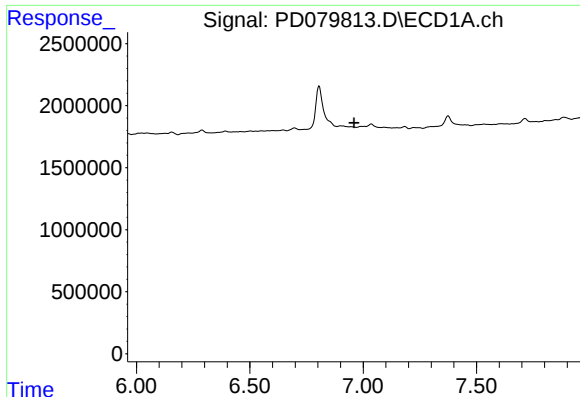

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 6.959 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

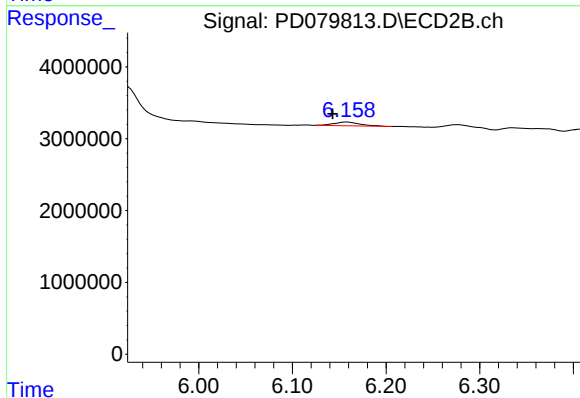


#18 Endrin aldehyde

R.T.: 6.159 min
Delta R.T.: 0.016 min
Response: 1038281
Conc: 0.51 ng/ml

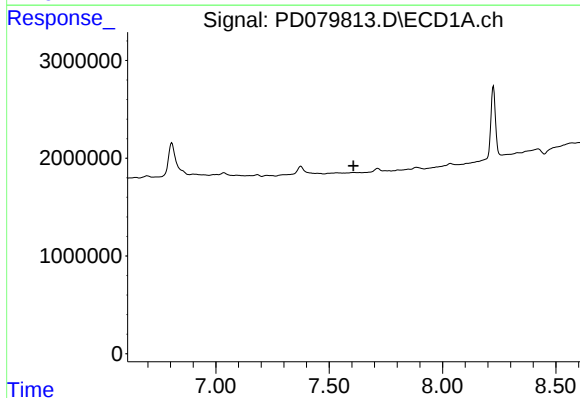


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T.: 7.608 min
Response: 0
Conc: N.D.

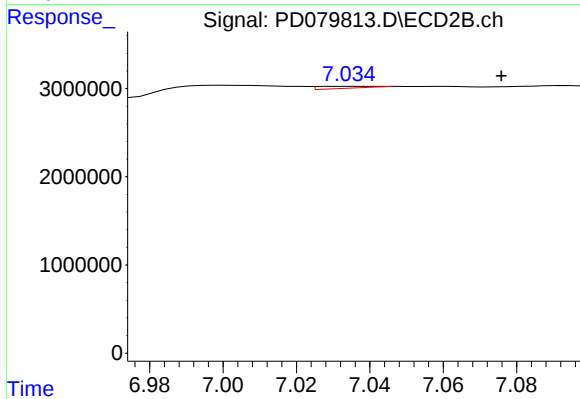

#26 Toxaphene-5


R.T.: 7.035 min
Delta R.T.: -0.041 min
Response: 222489
Conc: 6.66 ng/ml

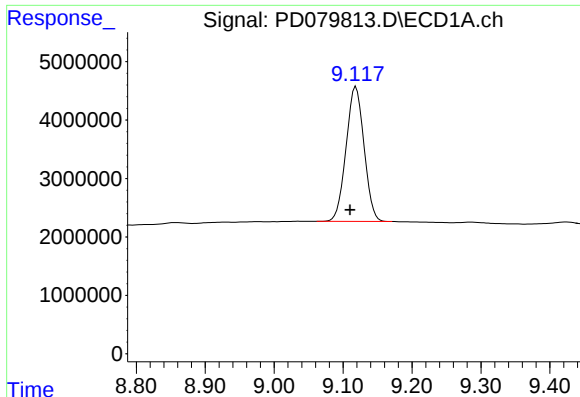

#27 Decachlorobiphenyl

R.T.: 9.119 min
Delta R.T.: 0.008 min
Response: 41758016
Conc: 23.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

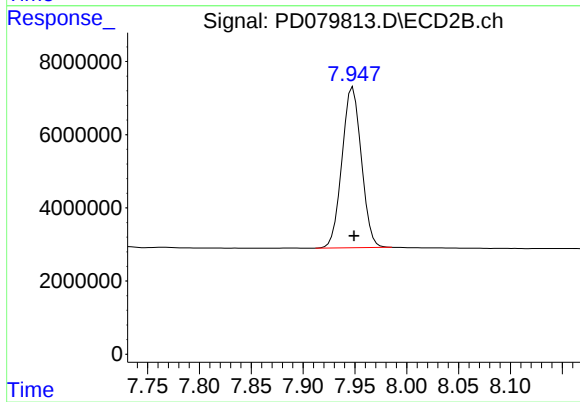

#27 Decachlorobiphenyl

R.T.: 7.948 min
Delta R.T.: -0.001 min
Response: 57035133
Conc: 23.89 ng/ml