

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
 Data File : PD079823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2023 19:13
 Operator : AR\AJ
 Sample : 05455-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:48:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	28623015	43561539	19.600	19.045
27)	SA Decachlor...	9.118	7.948	41627397	57222667	23.458	23.968
Target Compounds							
2)	A alpha-BHC	0.000	3.305	0	414476	N.D.	0.114
3)	MA gamma-BHC...	0.000	3.674f	0	279281	N.D.	<MDL
6)	B beta-BHC	0.000	3.892f	0	758347	N.D.	0.463
7)	B delta-BHC	4.794	0.000	6362246	0	2.553	N.D. #
9)	A Endosulfan I	0.000	5.166	0	236747	N.D.	<MDL
14)	MA Endrin	0.000	5.687	0	288725	N.D.	0.105
15)	B Endosulfa...	6.804	5.924f	4435187	985939	2.331	0.380 #
16)	A 4,4'-DDD	6.804f	0.000	4435187	0	2.738	N.D. #
18)	B Endrin al...	0.000	6.158	0	481191	N.D.	0.238
20)	A Methoxychlor	0.000	6.680f	0	530644	N.D.	0.413
24)	Toxaphene-3	0.000	6.680f	0	530644	N.D.	9.215


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
Data File : PD079823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2023 19:13
Operator : AR\AJ
Sample : 05455-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:48:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

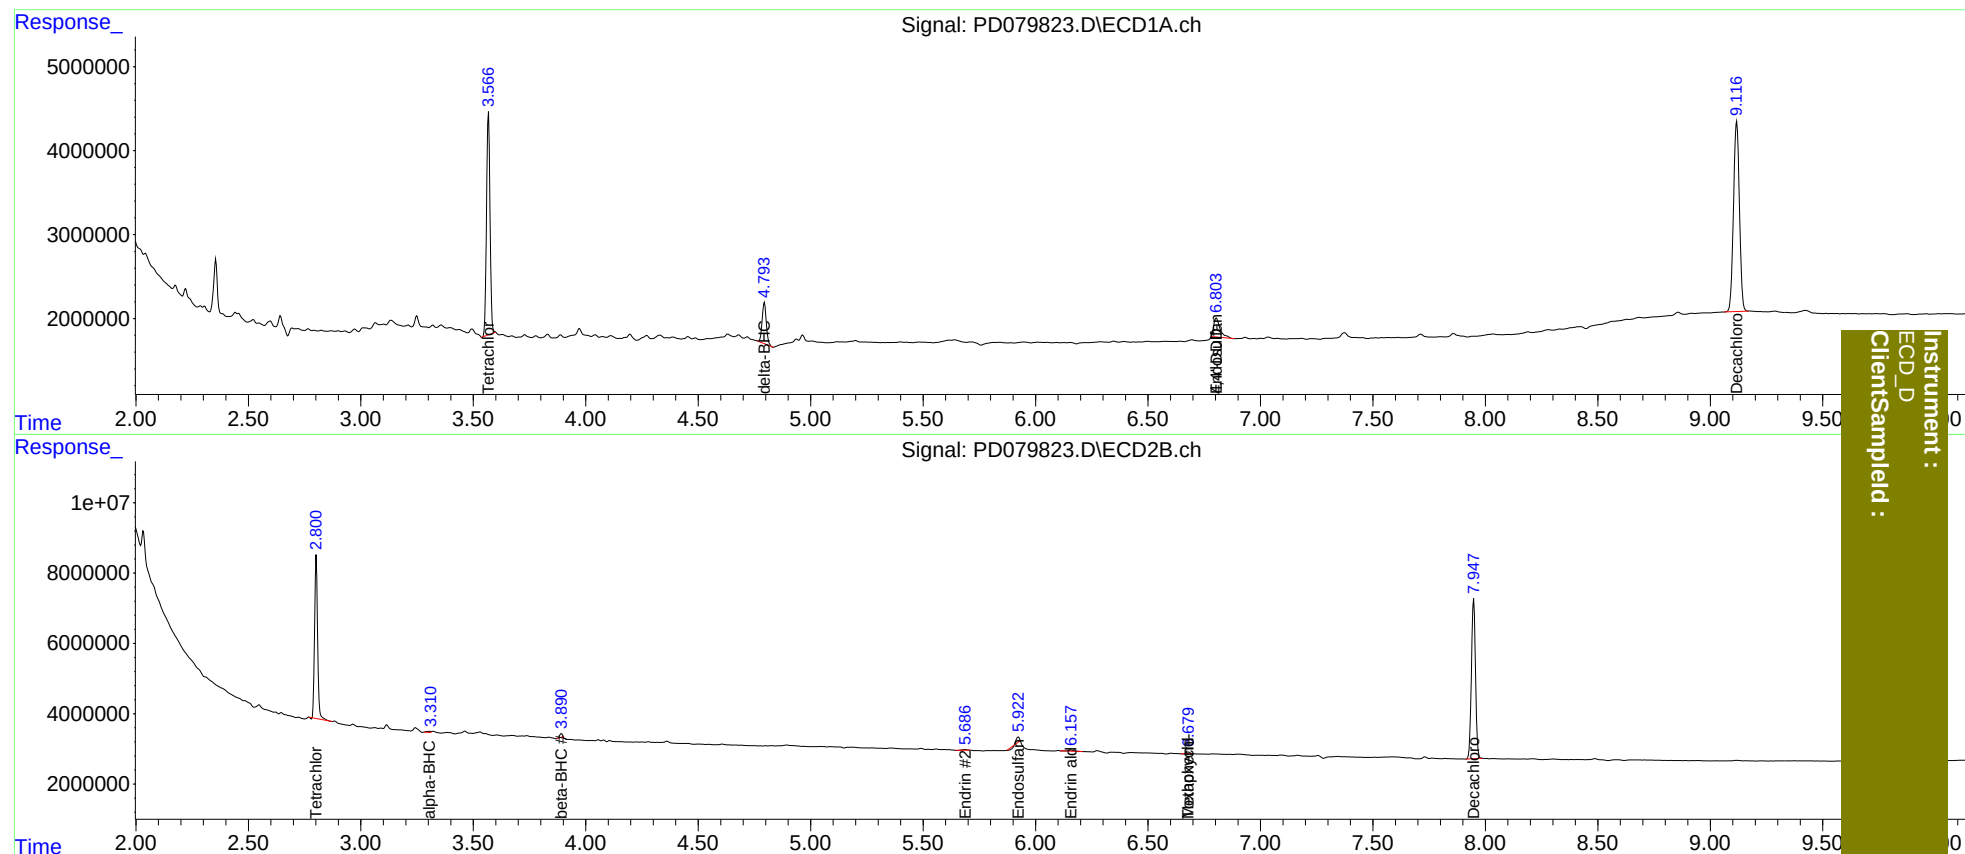


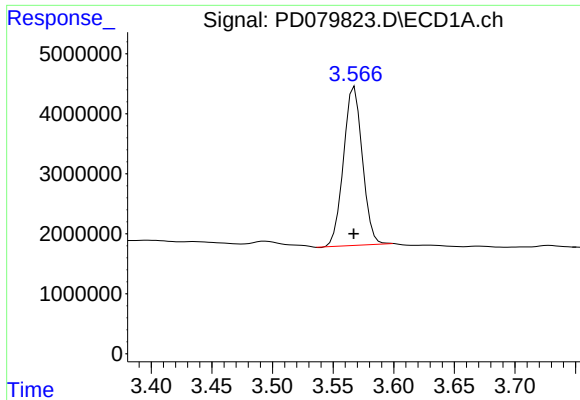

#1 Tetrachloro-m-xylene


R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 28623015
Conc: 19.60 ng/ml

Instrument :
ECD_D
ClientSampleId :

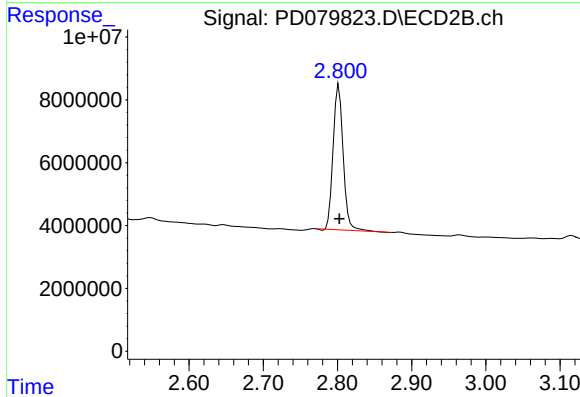


#1 Tetrachloro-m-xylene

R.T.: 2.802 min
Delta R.T.: -0.001 min
Response: 43561539
Conc: 19.04 ng/ml

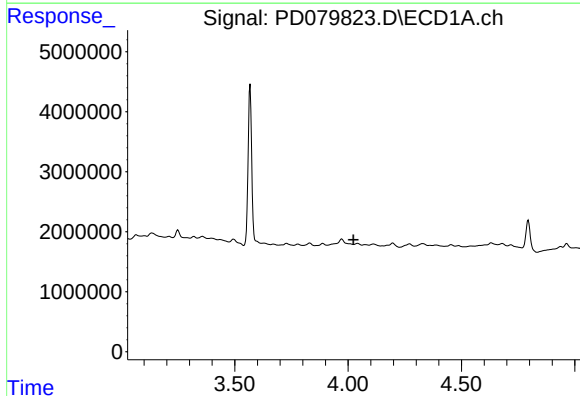


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.024 min
Response: 0
Conc: N.D.

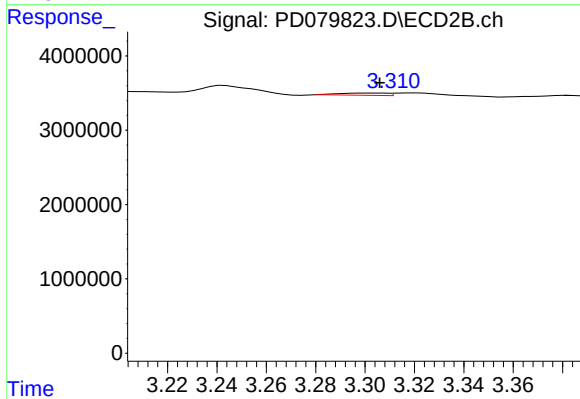

#2 alpha-BHC


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 414476
Conc: 0.11 ng/ml

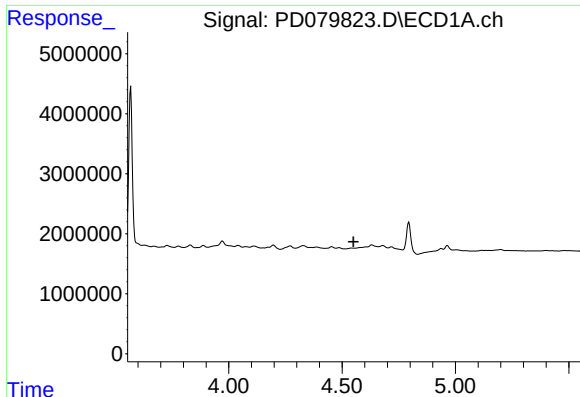

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

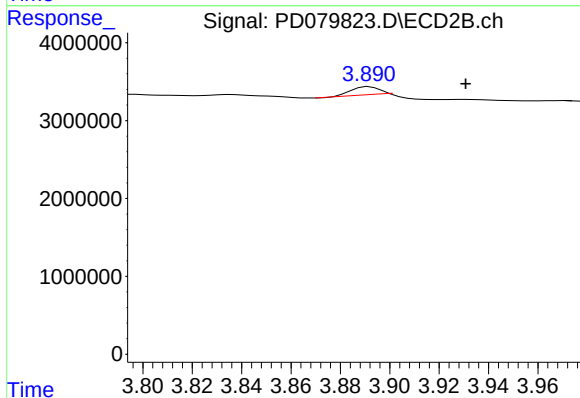


#6 beta-BHC

R.T.: 3.892 min
Delta R.T.: -0.039 min
Response: 758347
Conc: 0.46 ng/ml

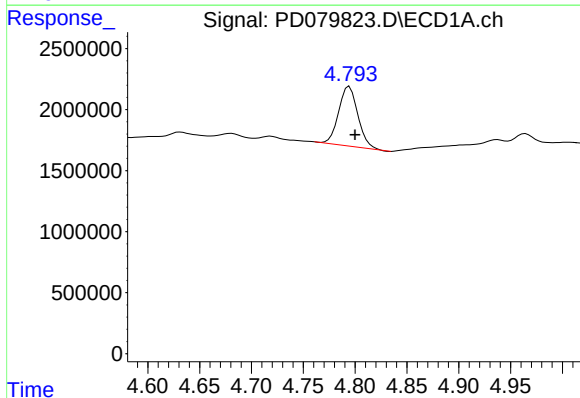


#7 delta-BHC

R.T.: 4.794 min
Delta R.T.: -0.005 min
Response: 6362246
Conc: 2.55 ng/ml

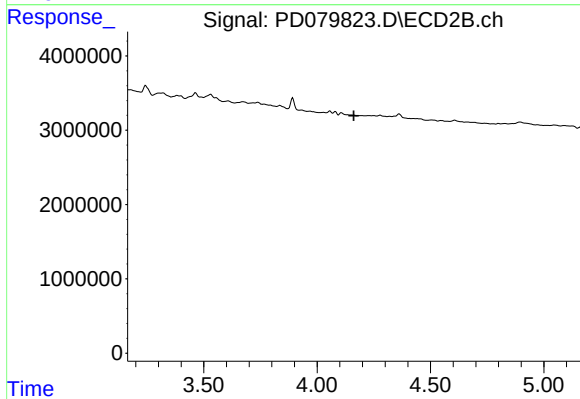

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.162 min
Response: 0
Conc: N.D.

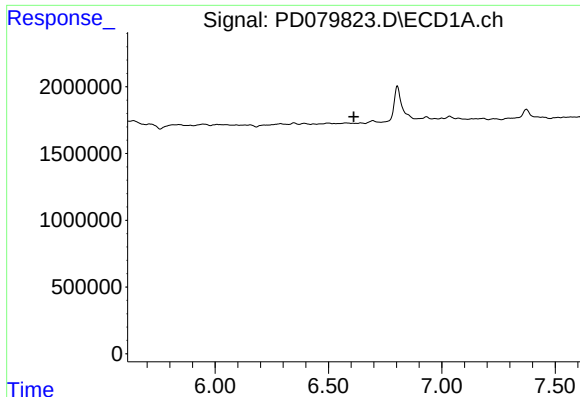

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.612 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

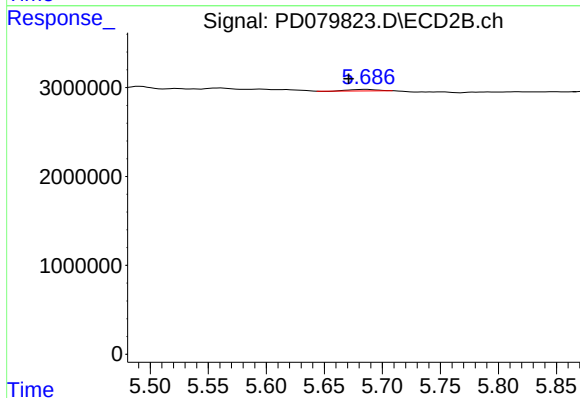


#14 Endrin

R.T.: 5.687 min
Delta R.T.: 0.016 min
Response: 288725
Conc: 0.11 ng/ml

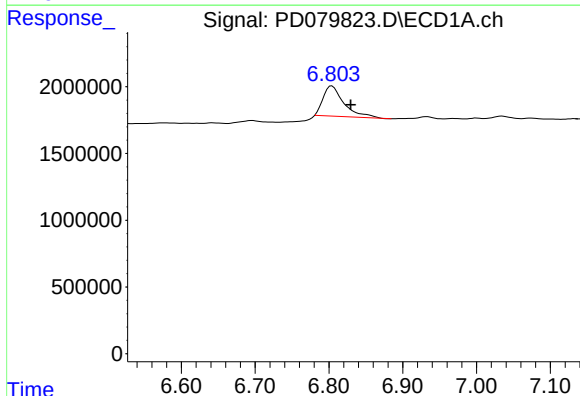


#15 Endosulfan II

R.T.: 6.804 min
Delta R.T.: -0.026 min
Response: 4435187
Conc: 2.33 ng/ml

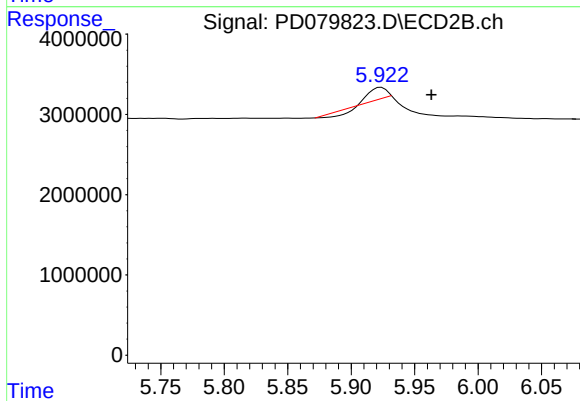

#15 Endosulfan II


R.T.: 5.924 min
Delta R.T.: -0.039 min
Response: 985939
Conc: 0.38 ng/ml

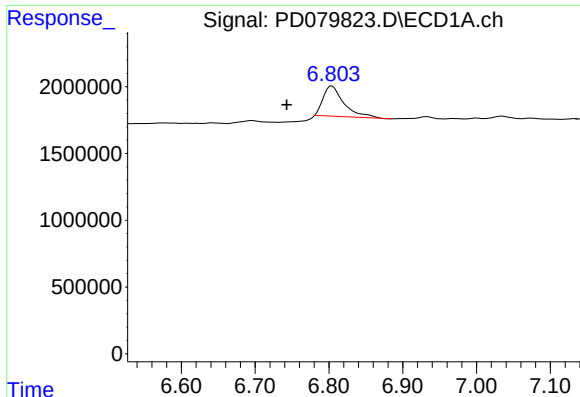

#16 4,4'-DDD


R.T.: 6.804 min
Delta R.T.: 0.061 min
Response: 4435187
Conc: 2.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

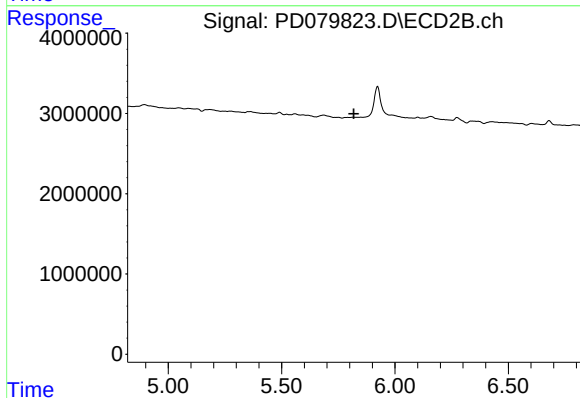


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.818 min
Response: 0
Conc: N.D.

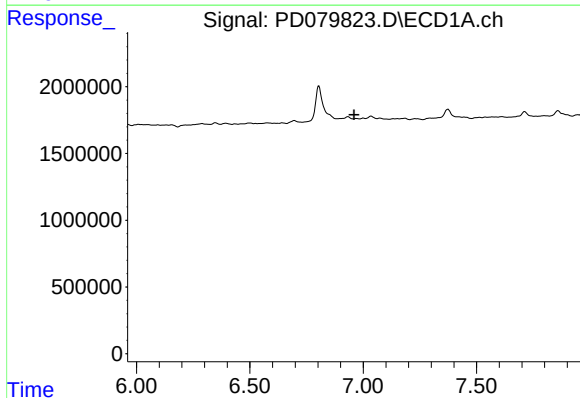


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.959 min
Response: 0
Conc: N.D.

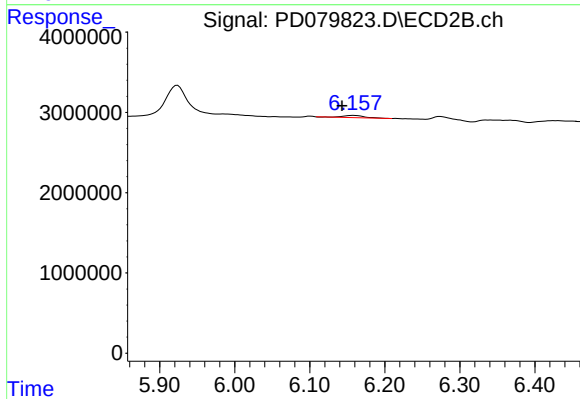

#18 Endrin aldehyde


R.T.: 6.158 min
Delta R.T.: 0.015 min
Response: 481191
Conc: 0.24 ng/ml

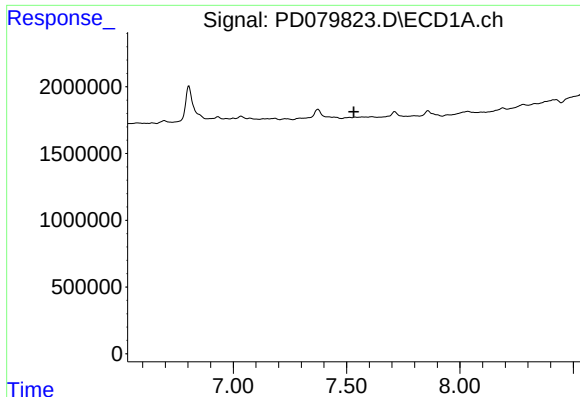

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.532 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

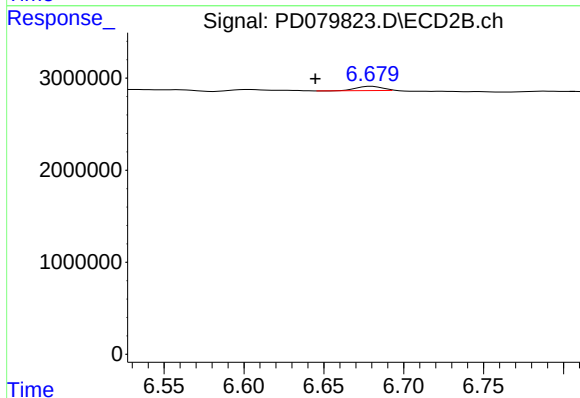


#20 Methoxychlor

R.T.: 6.680 min
Delta R.T.: 0.035 min
Response: 530644
Conc: 0.41 ng/ml

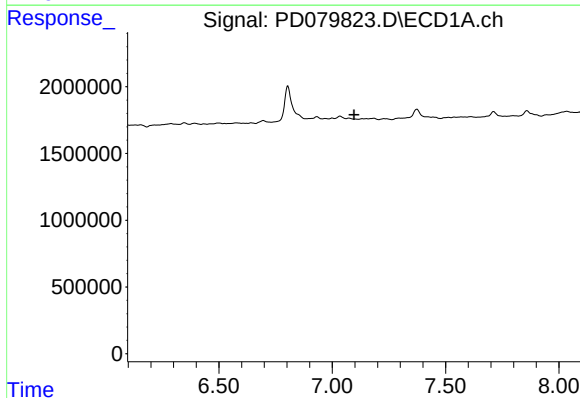


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T.: 7.096 min
Response: 0
Conc: N.D.

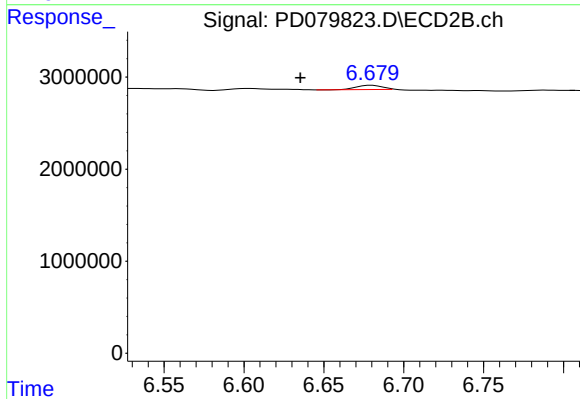

#24 Toxaphene-3


R.T.: 6.680 min
Delta R.T.: 0.045 min
Response: 530644
Conc: 9.22 ng/ml

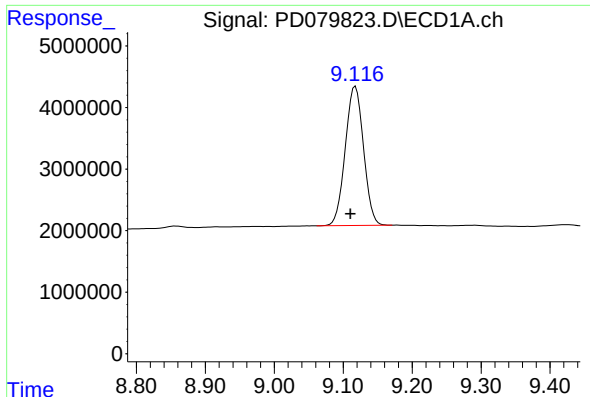

#27 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: 0.007 min
Response: 41627397
Conc: 23.46 ng/ml

Instrument :
ECD_D
ClientSampleId :

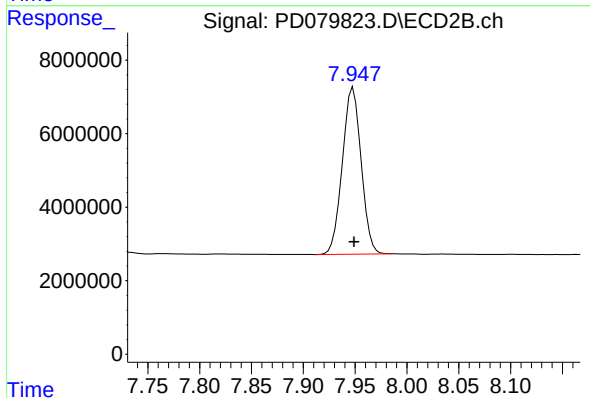

#27 Decachlorobiphenyl

R.T.: 7.948 min
Delta R.T.: -0.001 min
Response: 57222667
Conc: 23.97 ng/ml