

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
 Data File : PD079811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2023 16:33
 Operator : AR\AJ
 Sample : PB157368BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS368

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/24/2023
 Supervised By :Ankita Jodhani 11/27/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:34:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.569	2.801	34670196	57241719	23.741	25.026
27)	SA Decachlor...	9.119	7.948	64114269	87692135	36.130	36.730
Target Compounds							
2)	A alpha-BHC	4.026	3.304	8820152	13053757	3.560	3.600
3)	MA gamma-BHC...	4.360	3.634	8807833	13089178	3.728	3.810
4)	MA Heptachlor	4.953	3.976	10157865	13005145	4.056	3.898
5)	MB Aldrin	5.297	4.257	11701032	16661334	4.990	5.121
6)	B beta-BHC	4.553	3.929	5449911	6710839	5.019	4.098
7)	B delta-BHC	4.803	4.160	11838522	16097292	4.751	4.505
8)	B Heptachlo...	5.723	4.760	11303424	15396250	5.099	4.978
9)	A Endosulfan I	6.110	5.130	8803707	10894488	4.259	3.930
10)	B trans-Chl...	5.979	5.010	11244295	15242124	5.285	5.134
11)	B cis-Chlor...	6.059	5.074	11121496	14898571	5.106	4.908
12)	B 4,4'-DDE	6.230	5.263	19268465	27451370	9.760	9.804
13)	MA Dieldrin	6.386	5.395	17472136	25186407	7.942	7.910
14)	MA Endrin	6.617	5.670	14828381	22759013	8.127	8.310
15)	B Endosulfa...	6.832	5.961	20940490	26858075	11.007m	10.341m
16)	A 4,4'-DDD	6.747	5.817	12398778	18894407	7.654	8.026
17)	MA 4,4'-DDT	7.063	6.069	13211165	17374065	7.755	7.233
18)	B Endrin al...	6.964	6.142	15205109	22718691	10.201	11.227
19)	B Endosulfa...	7.199	6.365	18977413	25529626	10.192	10.274
20)	A Methoxychlor	7.537	6.644	38534438	55156018	41.801	42.911
21)	B Endrin ke...	7.686	6.871	19977465	28550270	10.225	10.042

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
Data File : PD079811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2023 16:33
Operator : AR\AJ
Sample : PB157368BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:34:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

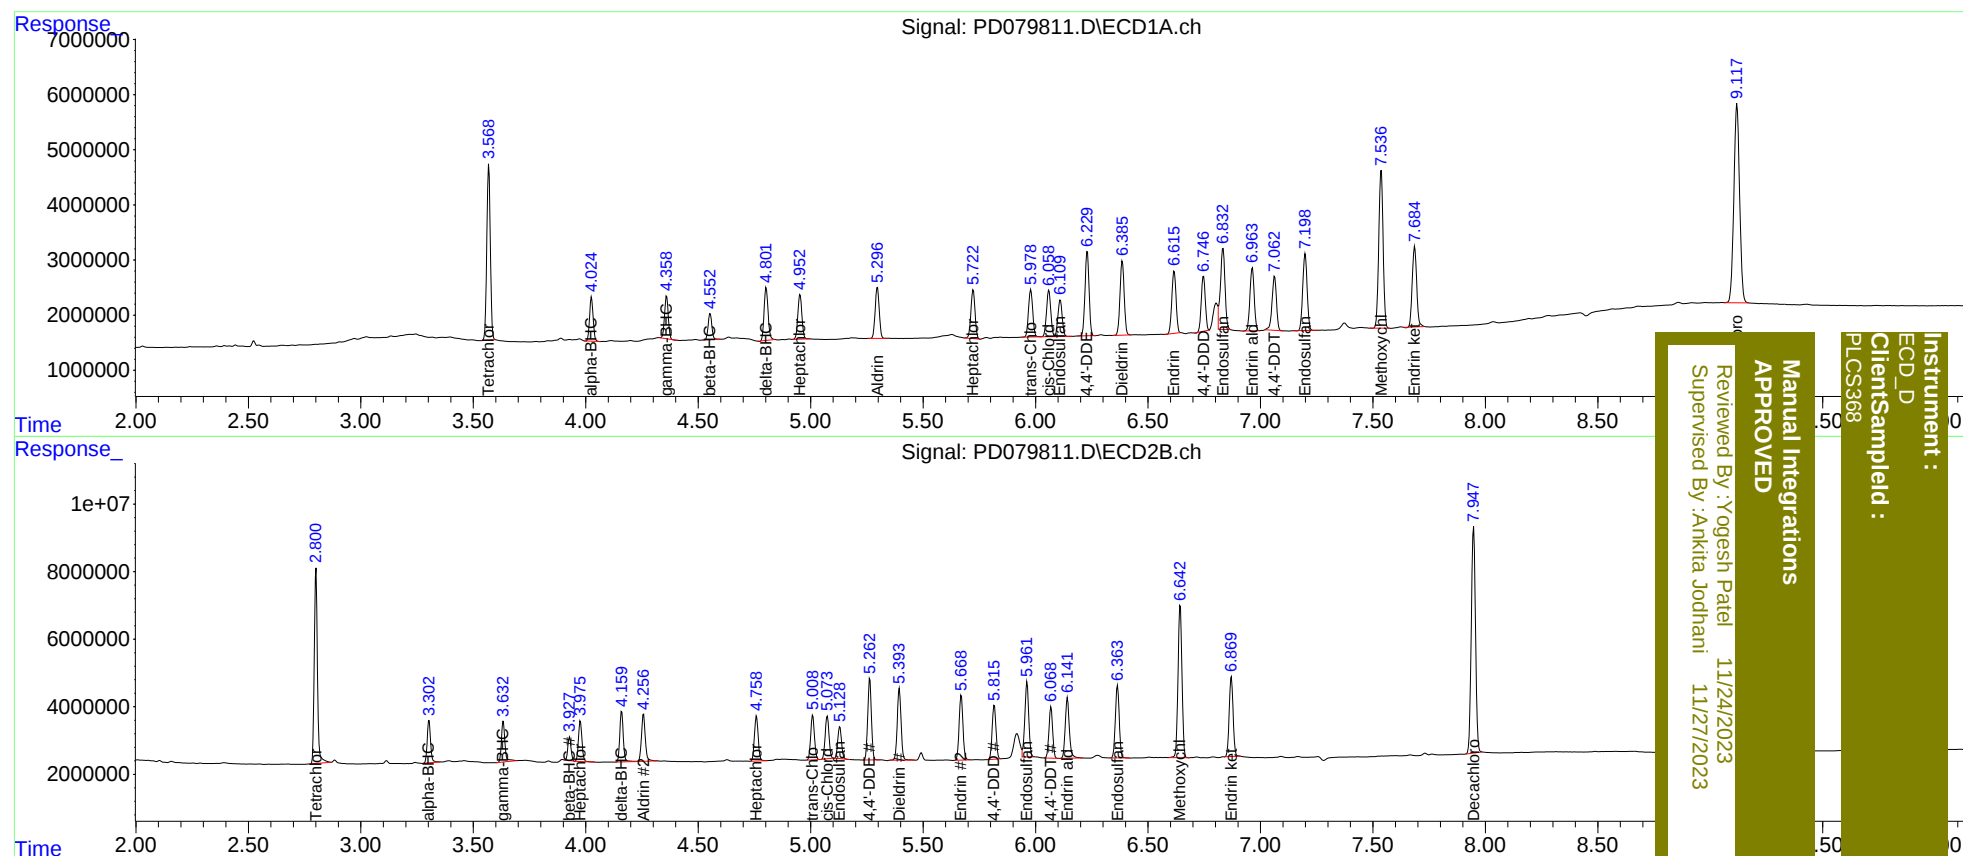

Instrument :
ECD_D
ClientSampled :
PLCS368

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/24/2023
Supervised By : Ankita Jodhani 11/27/2023