

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
 Data File : PD079817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Nov 2023 17:53
 Operator : AR\AJ
 Sample : 05455-10MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E05N3MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 20:41:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 07:14:58 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.568	2.802	31856127	49669674	21.814	21.715
27)	SA Decachlor...	9.118	7.948	44667425	62731874	25.171	26.275
Target Compounds							
2)	A alpha-BHC	4.025	3.305	134.8E6	203.8E6	54.398	56.211
3)	MA gamma-BHC...	4.359	3.635	122.2E6	183.5E6	51.724	53.420
4)	MA Heptachlor	4.952	3.977	122.2E6	181.2E6	48.791	54.310
5)	MB Aldrin	5.296	4.257	117.7E6	176.1E6	50.184	54.111
6)	B beta-BHC	4.552	3.929	50549078	76806632	46.555	46.900
7)	B delta-BHC	4.802	4.161	120.7E6	189.7E6	48.455	53.099
8)	B Heptachlo...	5.722	4.759	109.2E6	166.3E6	49.241	53.765
9)	A Endosulfan I	6.108	5.130	103.3E6	149.7E6	49.967	53.985
10)	B trans-Chl...	5.978	5.010	105.5E6	160.6E6	49.595	54.111
11)	B cis-Chlor...	6.058	5.074	107.6E6	160.5E6	49.390	52.876
12)	B 4,4'-DDE	6.228	5.263	206.2E6	317.7E6	104.459	113.455
13)	MA Dieldrin	6.384	5.394	225.1E6	347.9E6	102.348	109.244
14)	MA Endrin	6.615	5.669	193.5E6	312.0E6	106.061	113.926
15)	B Endosulfa...	6.833	5.962	195.3E6	287.0E6	102.634	110.498
16)	A 4,4'-DDD	6.745	5.816	168.2E6	264.8E6	103.802	112.468
17)	MA 4,4'-DDT	7.061	6.068	181.6E6	268.2E6	106.594	111.667
18)	B Endrin al...	6.963	6.141	141.4E6	213.4E6	94.845	105.466
19)	B Endosulfa...	7.197	6.364	183.3E6	269.4E6	98.432	108.434
20)	A Methoxychlor	7.535	6.643	453.9E6	648.0E6	492.351	504.100
21)	B Endrin ke...	7.684	6.870	198.9E6	309.0E6	101.778	108.699

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112223\
Data File : PD079817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Nov 2023 17:53
Operator : AR\AJ
Sample : 05455-10MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 20:41:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110623CLP.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 07:14:58 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

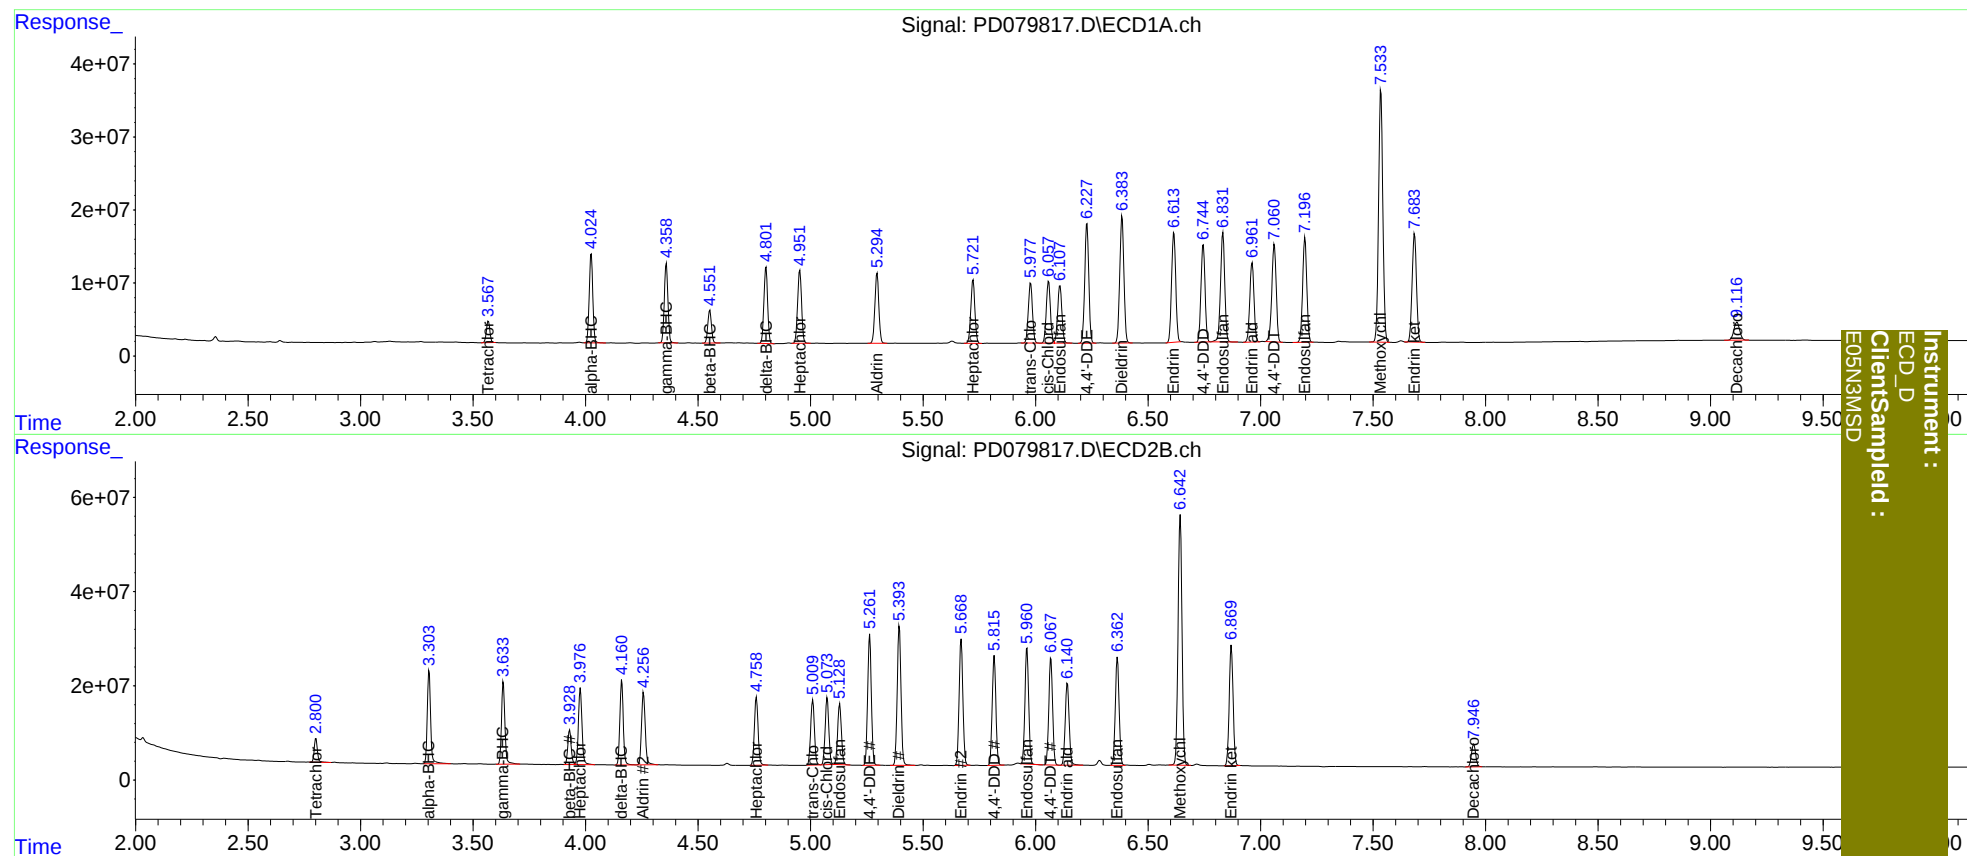

Instrument :
ECD_D
ClientSampled :
E05N8MSD