

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112224\
 Data File : PD086887.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 10:51
 Operator : AR\AJ
 Sample : PB165096BS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS096

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :Ankita Jodhani 11/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:34:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.885	37086938	233.1E6	20.168	20.201
27)	SA Decachlor...	9.095	8.092	54690619	255.3E6	20.541	20.028
Target Compounds							
2)	A alpha-BHC	4.009	3.399	17787949	106.3E6	5.052	5.937
3)	MA gamma-BHC...	4.341	3.736	17860111	99890996	5.128	5.989
4)	MA Heptachlor	4.942	4.092	18120999	97519954	5.215	5.669
5)	MB Aldrin	5.284	4.379	18772151	101.1E6	5.316	5.921
6)	B beta-BHC	4.524	4.032	8246835	45013942	5.202	5.698
7)	B delta-BHC	4.773	4.269	18322600	100.1E6	5.035	5.701
8)	B Heptachlo...	5.704	4.884	17322145	92216464	5.300	5.815
9)	A Endosulfan I	6.088	5.259	16670638	87687999	5.607	6.058
10)	B trans-Chl...	5.959	5.138	16689063	95294119	5.218	5.769
11)	B cis-Chlor...	6.041	5.203	17728793	94130046	5.450	5.874
12)	B 4,4'-DDE	6.209	5.389	30669599	173.2E6	9.944	11.359
13)	MA Dieldrin	6.361	5.526	34708937	179.9E6	10.589	11.775
14)	MA Endrin	6.588	5.802	26076312	153.1E6	9.647	11.083
15)	B Endosulfa...	6.800	6.094	28840854	161.5E6	10.394	11.574
16)	A 4,4'-DDD	6.719	5.944	26257848	155.8E6	11.068	12.893
17)	MA 4,4'-DDT	7.034	6.198	22109278	125.4E6	8.919m	9.697
18)	B Endrin al...	6.928	6.273	25026118	130.0E6	11.386	12.116
19)	B Endosulfa...	7.163	6.496	29160508	157.8E6	10.809	11.762
20)	A Methoxychlor	7.509	6.771	65533196	308.5E6	48.553	53.363
21)	B Endrin ke...	7.645	7.005	32687417	176.4E6	10.716	11.803

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112224\
Data File : PD086887.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 10:51
Operator : AR\AJ
Sample : PB165096BS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:34:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

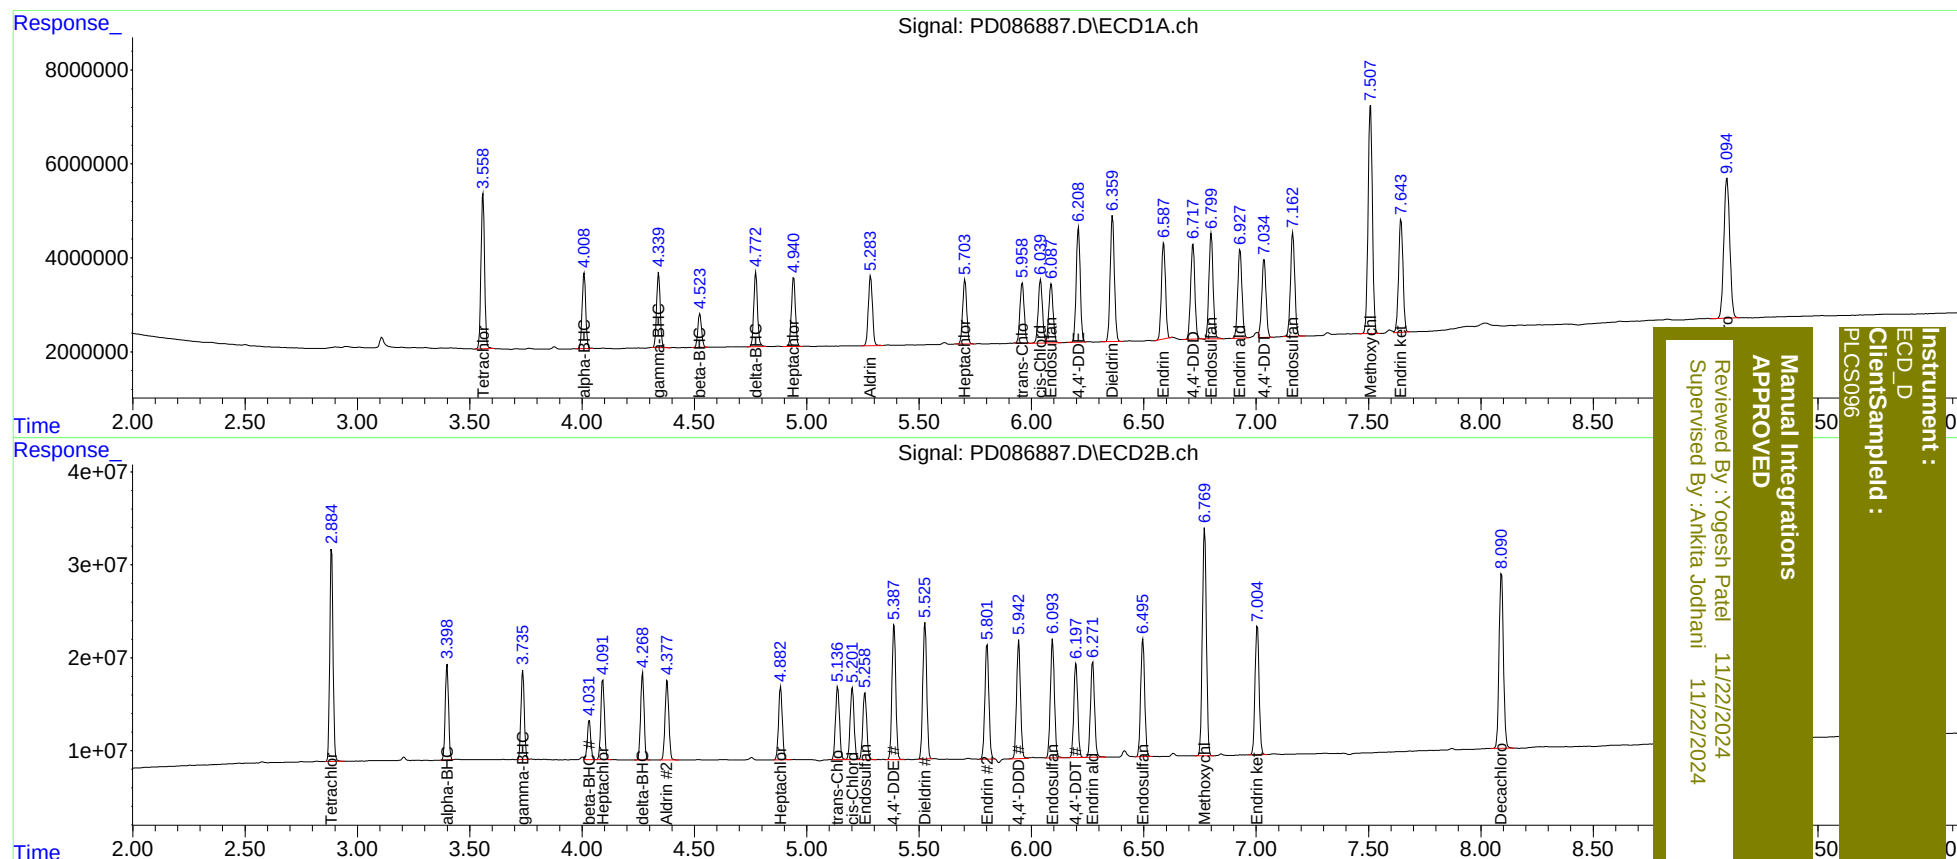

Manual Integrations
APPROVED
Reviewed By : Yogesh Patel 11/22/2024
Supervised By : Ankita Jodhani 11/22/2024

Instrument :
ECD_D
Client Sampled :
PLCS096