

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112224\
 Data File : PD086884.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Nov 2024 09:41
 Operator : AR\AJ
 Sample : P4872-06MS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 E29X5MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/22/2024
 Supervised By :Ankita Jodhani 11/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 22 00:33:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 20 02:52:29 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.559	2.885	22441049	136.2E6	12.203m	11.805
27)	SA Decachlor...	9.098	8.093	31070448	146.5E6	11.670	11.492
Target Compounds							
2)	A alpha-BHC	4.010	3.400	210.3E6	901.4E6	59.716	50.329
3)	MA gamma-BHC...	4.342	3.737	200.6E6	838.8E6	57.605	50.294
4)	MA Heptachlor	4.943	4.093	201.0E6	781.5E6	57.856	45.430
5)	MB Aldrin	5.286	4.379	202.7E6	827.5E6	57.404	48.440
6)	B beta-BHC	4.526	4.032	74995640	355.1E6	47.311	44.946
7)	B delta-BHC	4.775	4.270	135.8E6	574.5E6	37.301	32.720
8)	B Heptachlo...	5.704	4.884	187.6E6	740.6E6	57.391m	46.699
9)	A Endosulfan I	6.090	5.259	170.4E6	552.5E6	57.297	38.173 #
10)	B trans-Chl...	5.959	5.138	175.3E6	783.2E6	54.820m	47.414
11)	B cis-Chlor...	6.042	5.203	181.0E6	773.0E6	55.633	48.237
12)	B 4,4'-DDE	6.211	5.389	332.5E6	1458.9E6	107.820	95.682
13)	MA Dieldrin	6.363	5.526	381.8E6	1493.4E6	116.493	97.746
14)	MA Endrin	6.590	5.803	312.7E6	1354.6E6	115.687	98.059
15)	B Endosulfa...	6.801	6.094	289.9E6	1276.9E6	104.469	91.510
16)	A 4,4'-DDD	6.719	5.944	281.8E6	1170.4E6	118.790m	96.874
17)	MA 4,4'-DDT	7.036	6.198	261.4E6	1120.0E6	105.440m	86.632
18)	B Endrin al...	6.931	6.273	222.0E6	922.6E6	101.016	85.973
19)	B Endosulfa...	7.165	6.496	269.0E6	1283.0E6	99.705	95.609
20)	A Methoxychlor	7.509	6.771	682.0E6	2297.8E6	505.255	397.448
21)	B Endrin ke...	7.646	7.006	320.1E6	1310.3E6	104.957	87.693

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112224\
Data File : PD086884.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Nov 2024 09:41
Operator : AR\AJ
Sample : P4872-06MS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 22 00:33:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112024CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 20 02:52:29 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

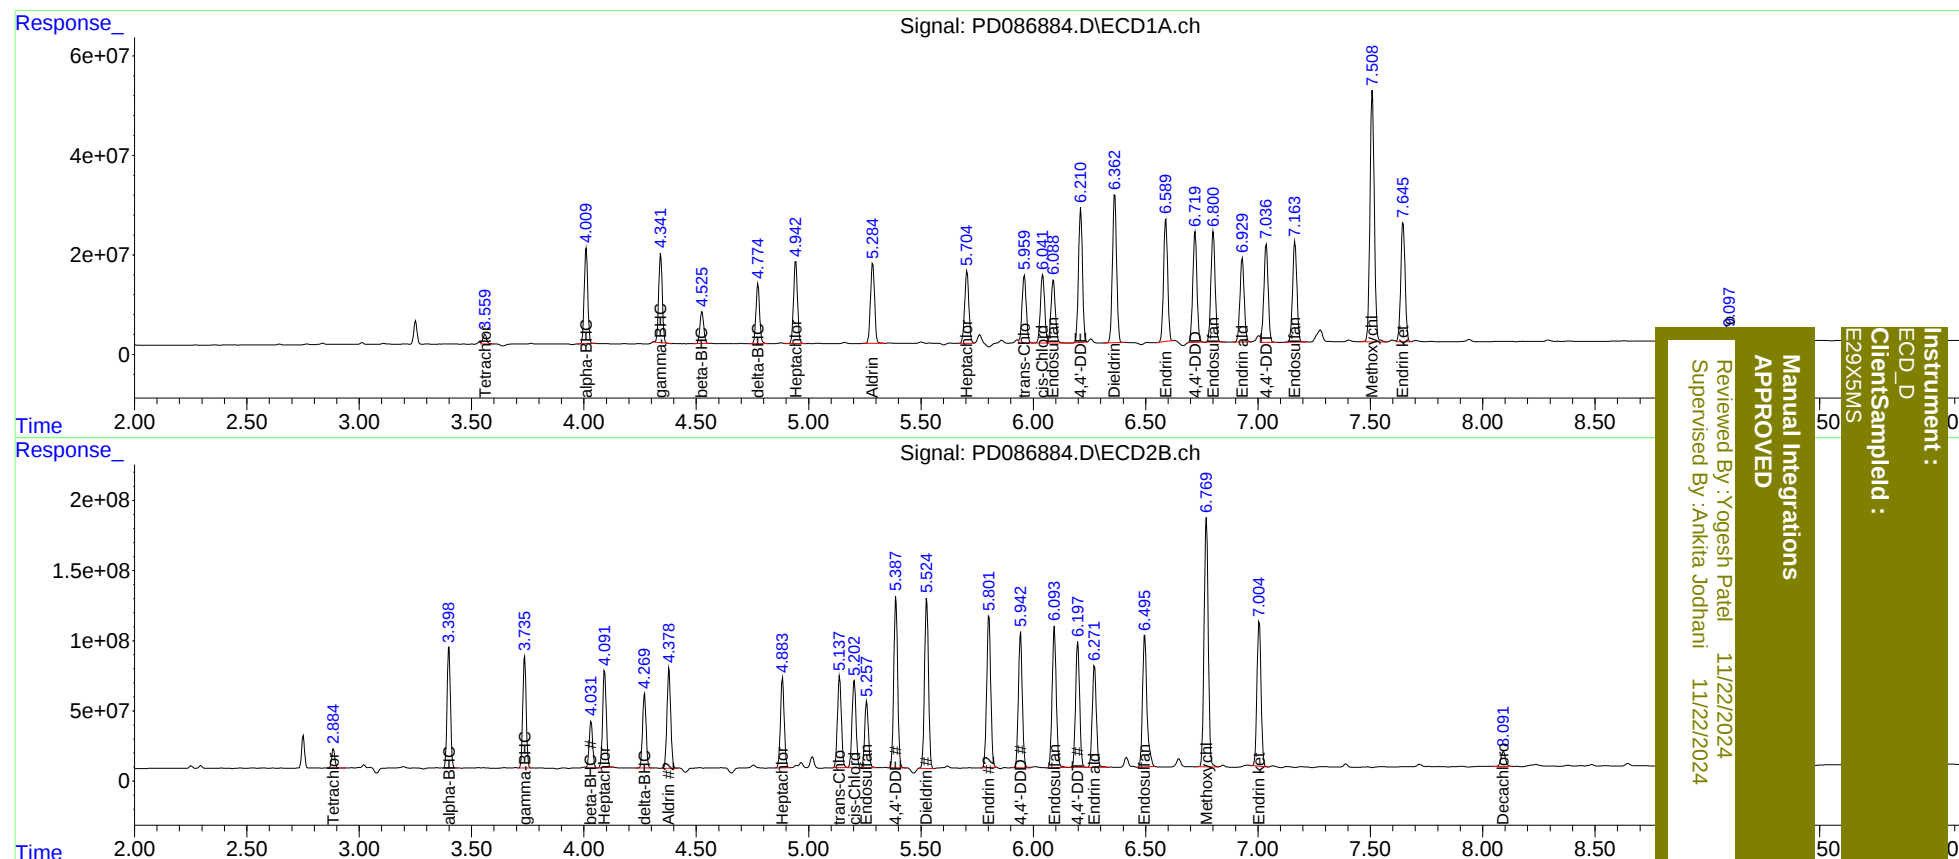

Instrument :
ECD_D
ClientSampled :
E29X5MS

Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 11/22/2024
Supervised By : Ankita Jodhani 11/22/2024