

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
 Data File : PD060247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 15:04
 Operator : DD\AJ
 Sample : L4793-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BA0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 00:29:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.505	4.024	20562808	70900215	23.995	23.785
27)	SA Decachlor...	8.302	9.110	34019913	91386350	40.944	37.148
Target Compounds							
2)	A alpha-BHC	0.000	4.383f	0	1507367	N.D.	0.338
9)	A Endosulfan I	0.000	6.223f	0	5195355	N.D.	1.621
10)	B trans-Chl...	0.000	6.149	0	9728180	N.D.	2.831
11)	B cis-Chlor...	0.000	6.223	0	5195355	N.D.	1.513
12)	B 4,4'-DDE	0.000	6.319f	0	1155501	N.D.	0.357
14)	MA Endrin	6.155f	0.000	275319	0	0.305	N.D. #
15)	B Endosulfa...	6.301f	6.950	1088280	5170043	1.207	1.829 #
19)	B Endosulfa...	6.679f	0.000	1388557	0	1.589	N.D. #
20)	A Methoxychlor	7.052f	0.000	1276482	0	2.999	N.D. #
21)	B Endrin ke...	0.000	7.755	0	6463363	N.D.	2.216
23)	Toxaphene-2	0.000	6.648	0	4207261	N.D.	223.860
24)	Toxaphene-3	6.301	0.000	1088280	0	154.145	N.D. #
26)	Toxaphene-5	7.128	7.755	760901	6463363	44.989	190.099 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
Data File : PD060247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 15:04
Operator : DD\AJ
Sample : L4793-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BA0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 00:29:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

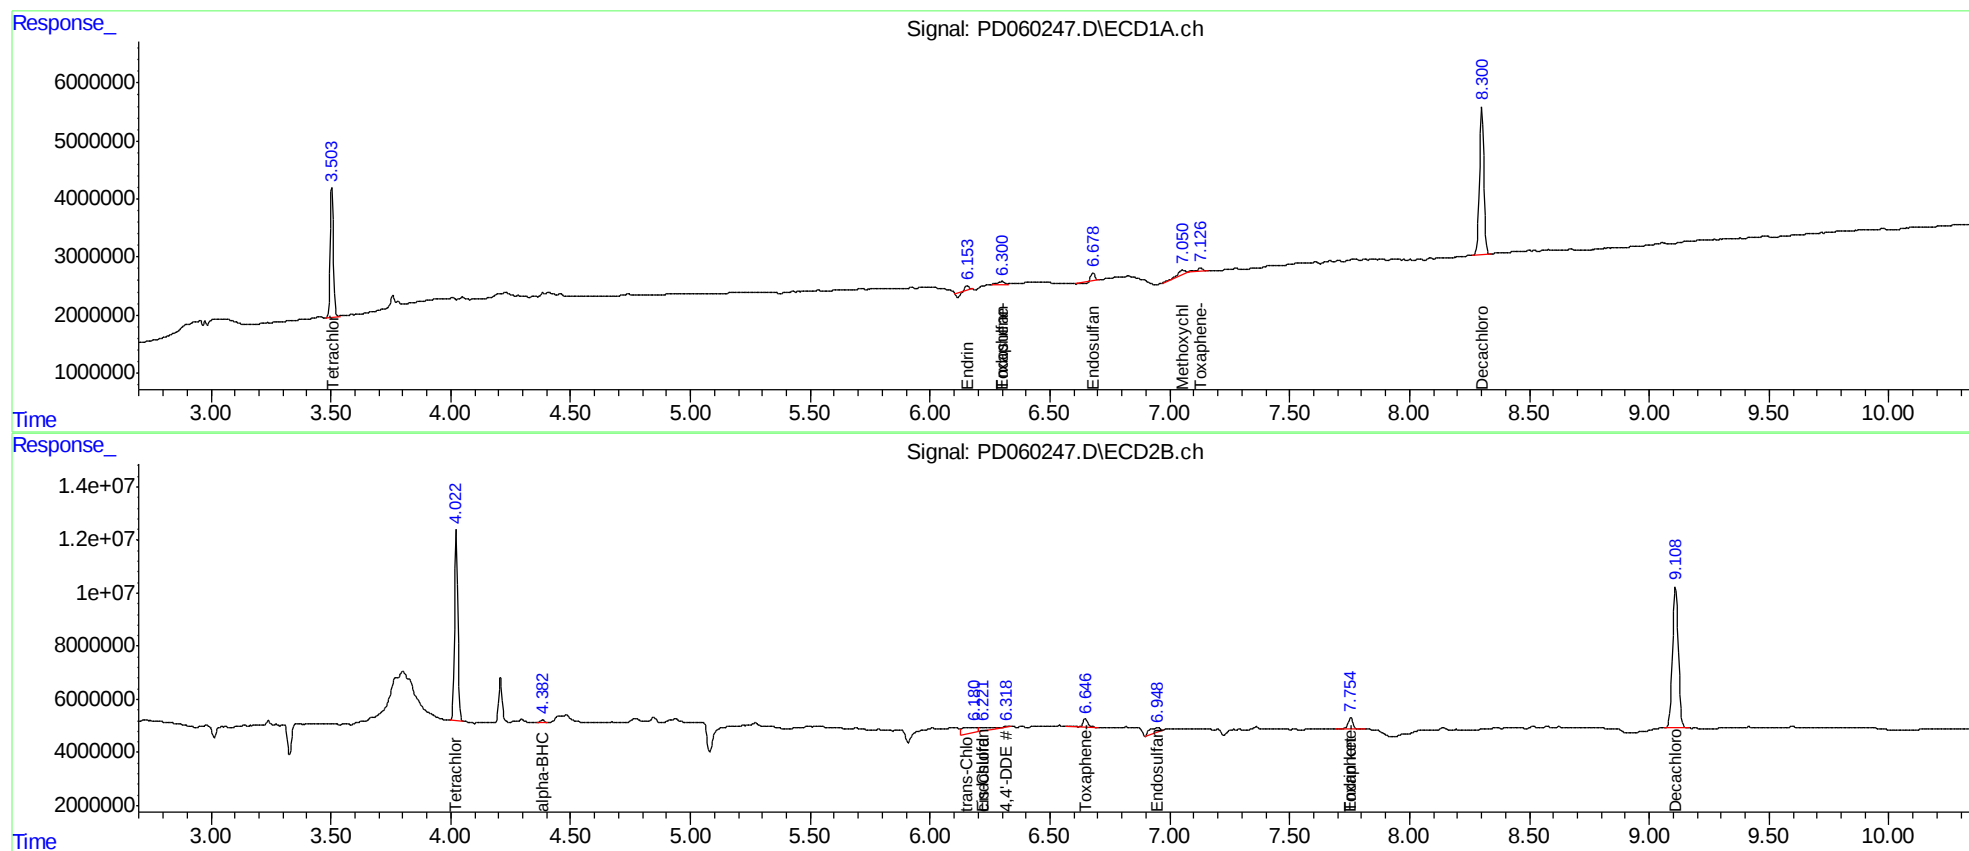


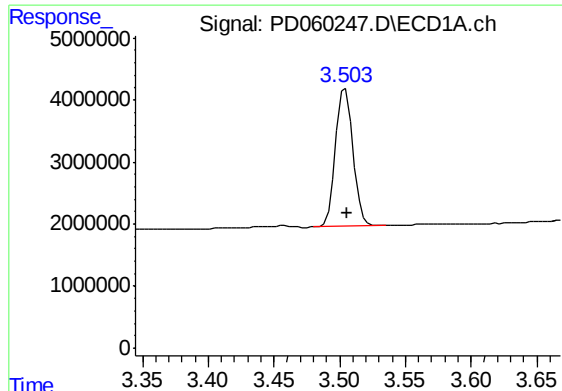

#1 Tetrachloro-m-xylene


R.T.: 3.505 min
Delta R.T.: -0.001 min
Response: 20562808
Conc: 23.99 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BA0

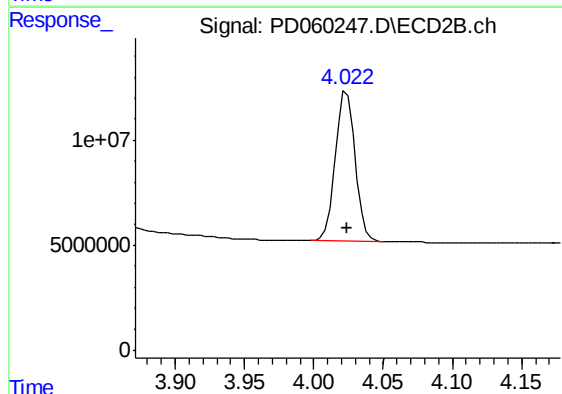


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 70900215
Conc: 23.78 ng/ml

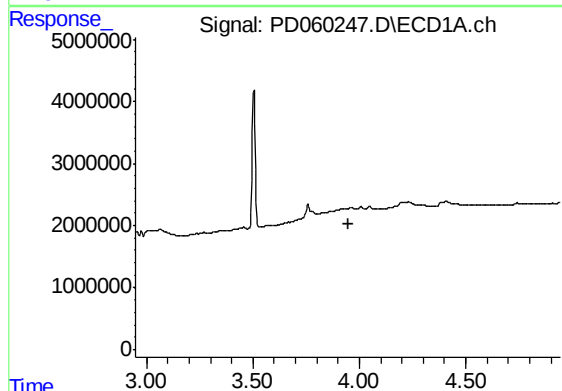


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.947 min
Response: 0
Conc: N.D.

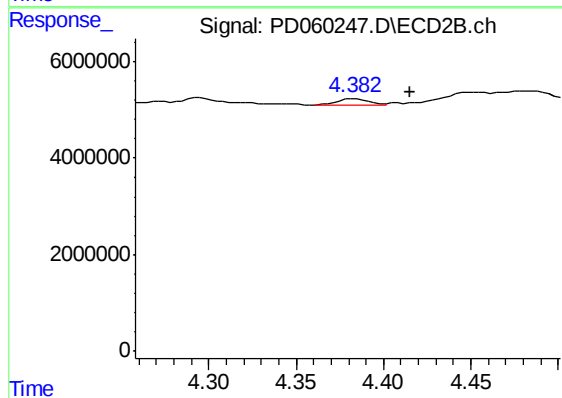

#2 alpha-BHC


R.T.: 4.383 min
Delta R.T.: -0.032 min
Response: 1507367
Conc: 0.34 ng/ml

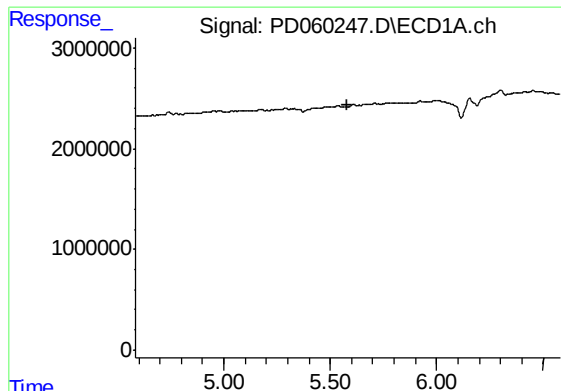

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.582 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BA0

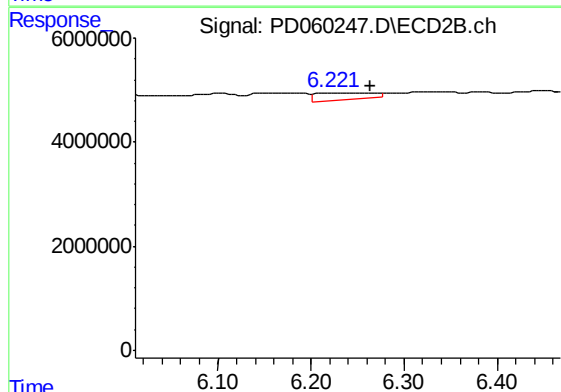


#9 Endosulfan I

R.T.: 6.223 min
Delta R.T.: -0.041 min
Response: 5195355
Conc: 1.62 ng/ml

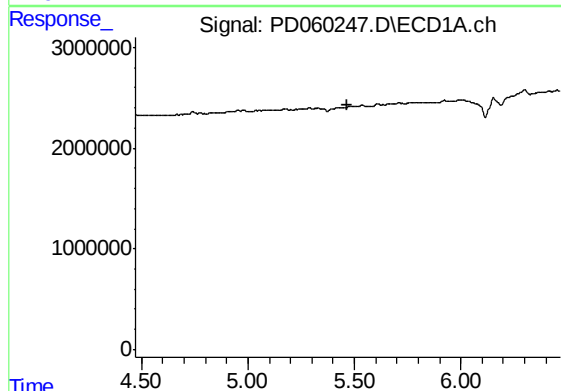


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.469 min
Response: 0
Conc: N.D.

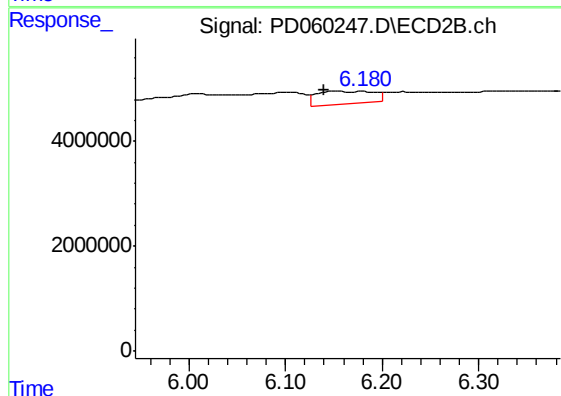

#10 trans-Chlordane


R.T.: 6.149 min
Delta R.T.: 0.010 min
Response: 9728180
Conc: 2.83 ng/ml

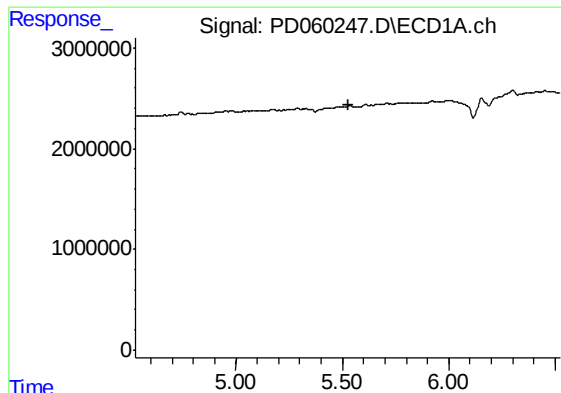

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.528 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BA0

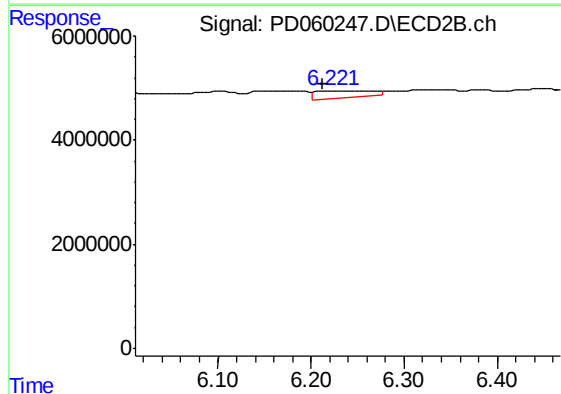


#11 cis-Chlordane

R.T.: 6.223 min
Delta R.T.: 0.010 min
Response: 5195355
Conc: 1.51 ng/ml

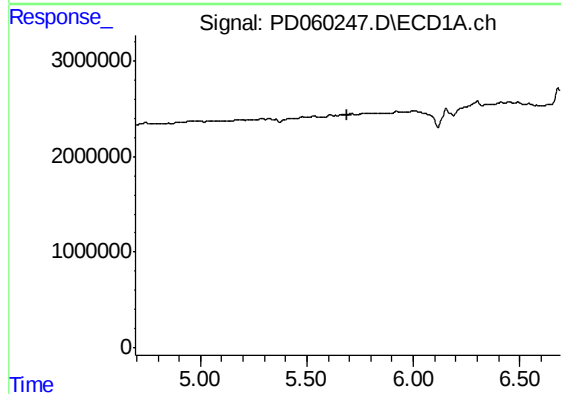


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.692 min
Response: 0
Conc: N.D.

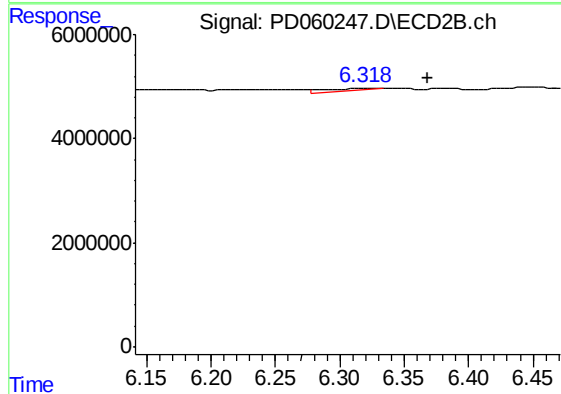

#12 4,4'-DDE


R.T.: 6.319 min
Delta R.T.: -0.049 min
Response: 1155501
Conc: 0.36 ng/ml

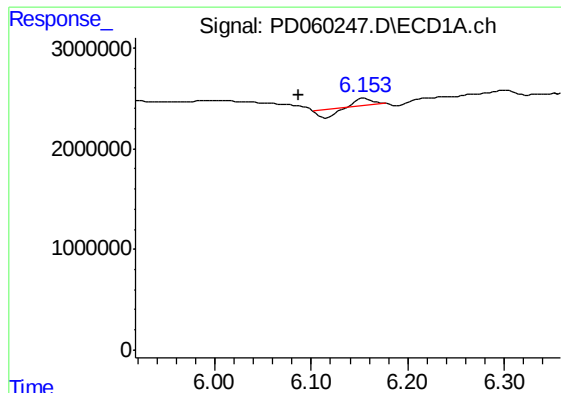

#14 Endrin


R.T.: 6.155 min
Delta R.T.: 0.068 min
Response: 275319
Conc: 0.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BA0

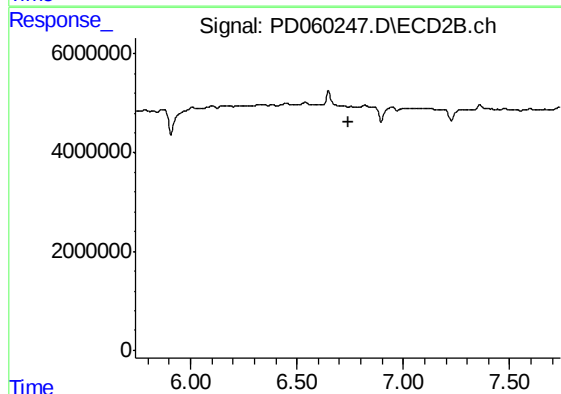


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.740 min
Response: 0
Conc: N.D.

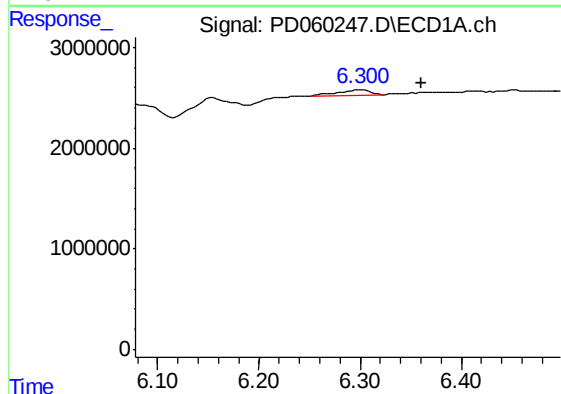


#15 Endosulfan II

R.T.: 6.301 min
Delta R.T.: -0.059 min
Response: 1088280
Conc: 1.21 ng/ml

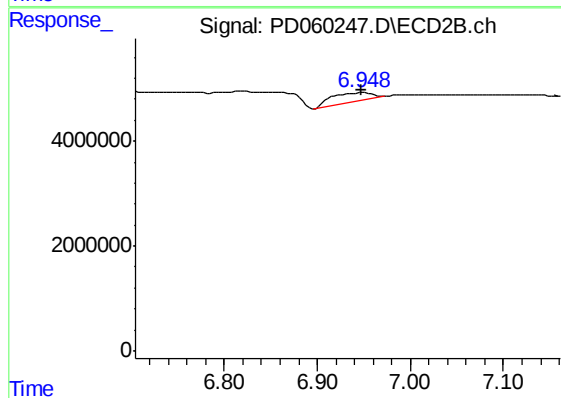

#15 Endosulfan II


R.T.: 6.950 min
Delta R.T.: 0.003 min
Response: 5170043
Conc: 1.83 ng/ml

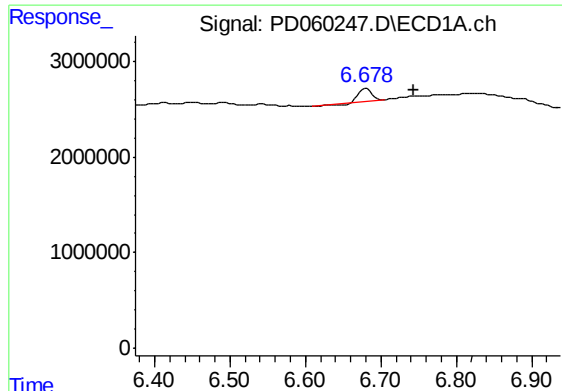

#19 Endosulfan Sulfate


R.T.: 6.679 min
Delta R.T.: -0.065 min
Response: 1388557
Conc: 1.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BA0

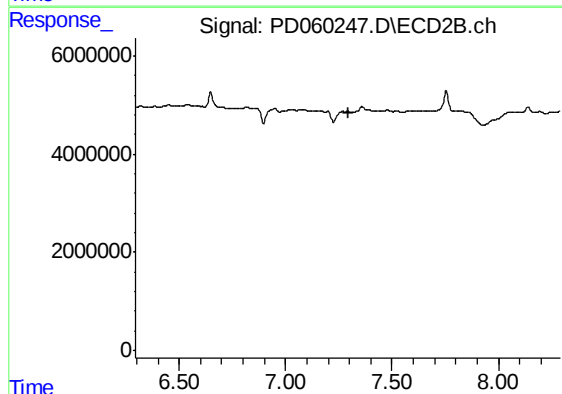


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.294 min
Response: 0
Conc: N.D.

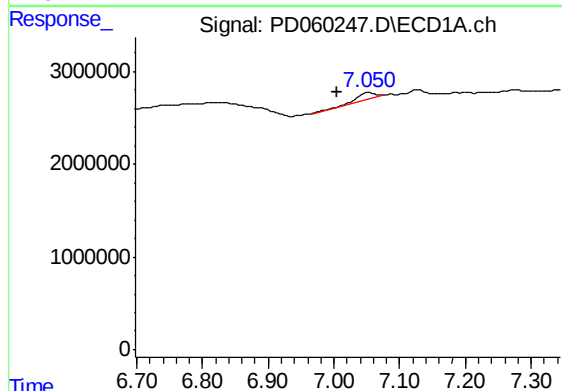


#20 Methoxychlor

R.T.: 7.052 min
Delta R.T.: 0.047 min
Response: 1276482
Conc: 3.00 ng/ml

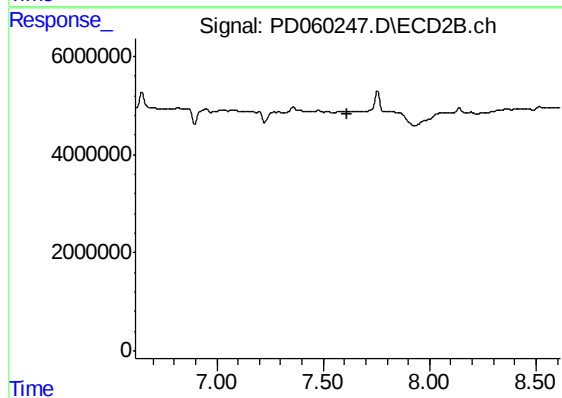

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.615 min
Response: 0
Conc: N.D.

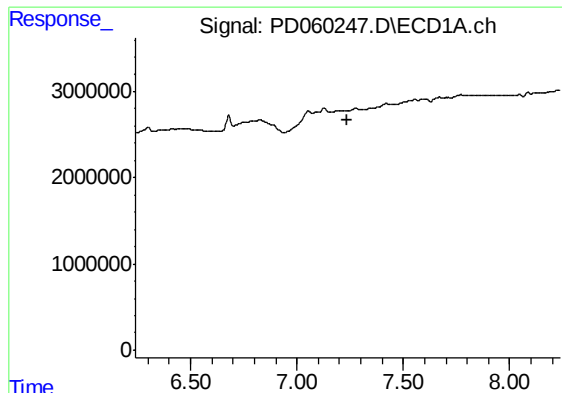

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.239 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BA0

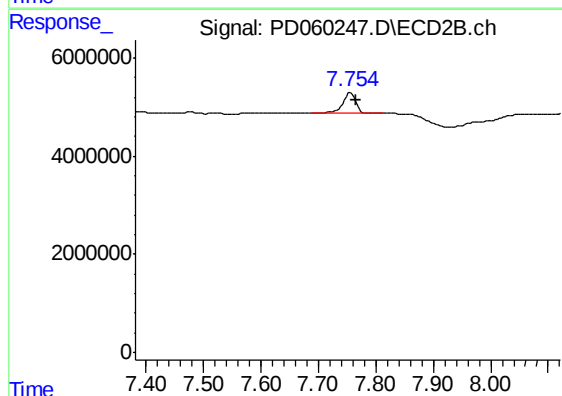


#21 Endrin ketone

R.T.: 7.755 min
Delta R.T.: -0.011 min
Response: 6463363
Conc: 2.22 ng/ml

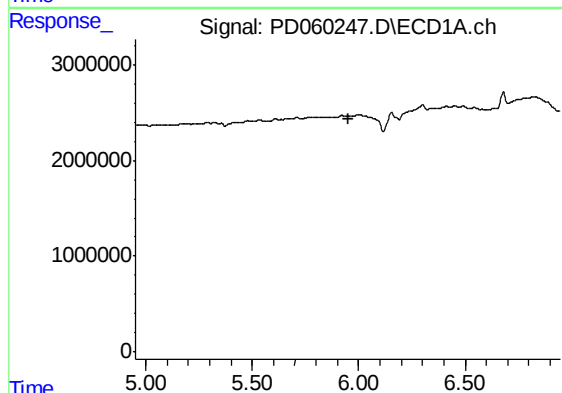


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T.: 5.951 min
Response: 0
Conc: N.D.

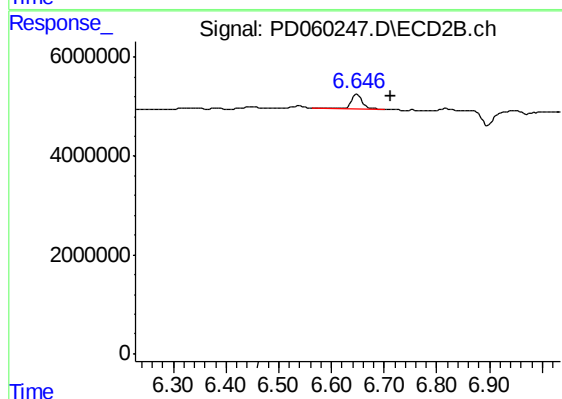

#23 Toxaphene-2


R.T.: 6.648 min
Delta R.T.: -0.064 min
Response: 4207261
Conc: 223.86 ng/ml

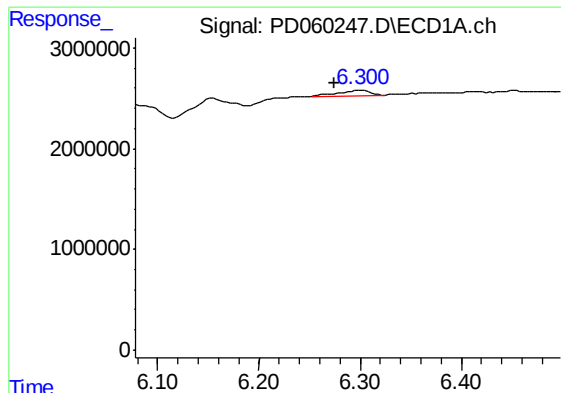

#24 Toxaphene-3


R.T.: 6.301 min
Delta R.T.: 0.026 min
Response: 1088280
Conc: 154.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BA0

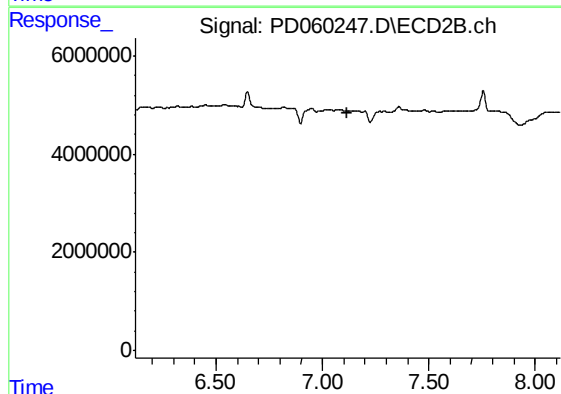


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.119 min
Response: 0
Conc: N.D.

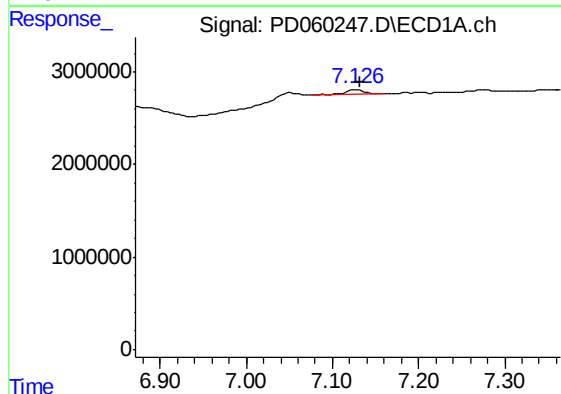


#26 Toxaphene-5

R.T.: 7.128 min
Delta R.T.: -0.005 min
Response: 760901
Conc: 44.99 ng/ml

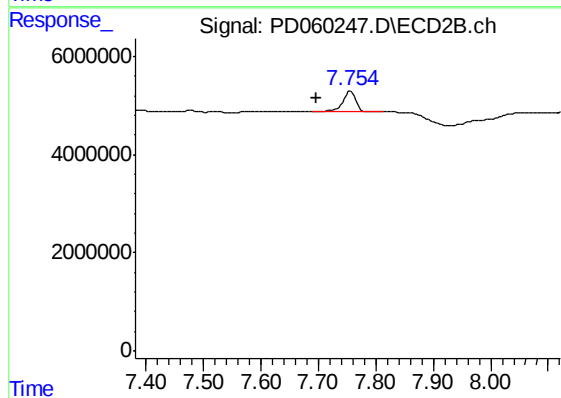

#26 Toxaphene-5


R.T.: 7.755 min
Delta R.T.: 0.060 min
Response: 6463363
Conc: 190.10 ng/ml

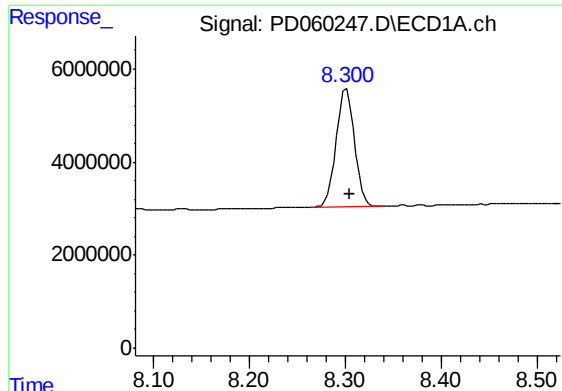

#27 Decachlorobiphenyl

R.T.: 8.302 min
Delta R.T.: -0.003 min
Response: 34019913
Conc: 40.94 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BA0

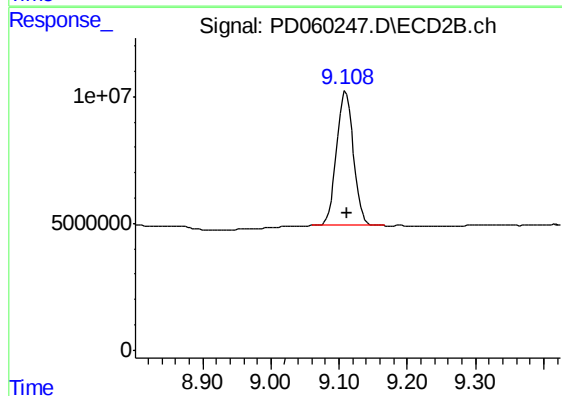

#27 Decachlorobiphenyl

R.T.: 9.110 min
Delta R.T.: -0.002 min
Response: 91386350
Conc: 37.15 ng/ml