

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
 Data File : PD060257.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 17:24
 Operator : DD\AJ
 Sample : L4793-08
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BB2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 00:33:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.024	15782638	52858102	18.417	17.732
27)	SA Decachlor...	8.301	9.108	28451572	72513738	34.242	29.477
Target Compounds							
2)	A alpha-BHC	0.000	4.383f	0	2003764	N.D.	0.450
6)	B beta-BHC	0.000	4.915f	0	3375816	N.D.	1.817
9)	A Endosulfan I	5.602	6.242	257085	552941	0.253	0.173 #
10)	B trans-Chl...	5.478	6.149	850795	5943175	0.801	1.730 #
11)	B cis-Chlor...	5.478f	6.218	850795	1030119	0.804	0.300 #
15)	B Endosulfa...	6.299f	6.949	2375609	5551623	2.634	1.964 #
19)	B Endosulfa...	6.801f	0.000	427325	0	0.489	N.D. #
20)	A Methoxychlor	7.052f	0.000	922134	0	2.167	N.D. #
21)	B Endrin ke...	0.000	7.754	0	5254368	N.D.	1.802
24)	Toxaphene-3	6.299	0.000	2375609	0	336.484	N.D. #
26)	Toxaphene-5	0.000	7.754	0	5254368	N.D.	154.540


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
Data File : PD060257.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 17:24
Operator : DD\AJ
Sample : L4793-08
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0BB2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 00:33:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

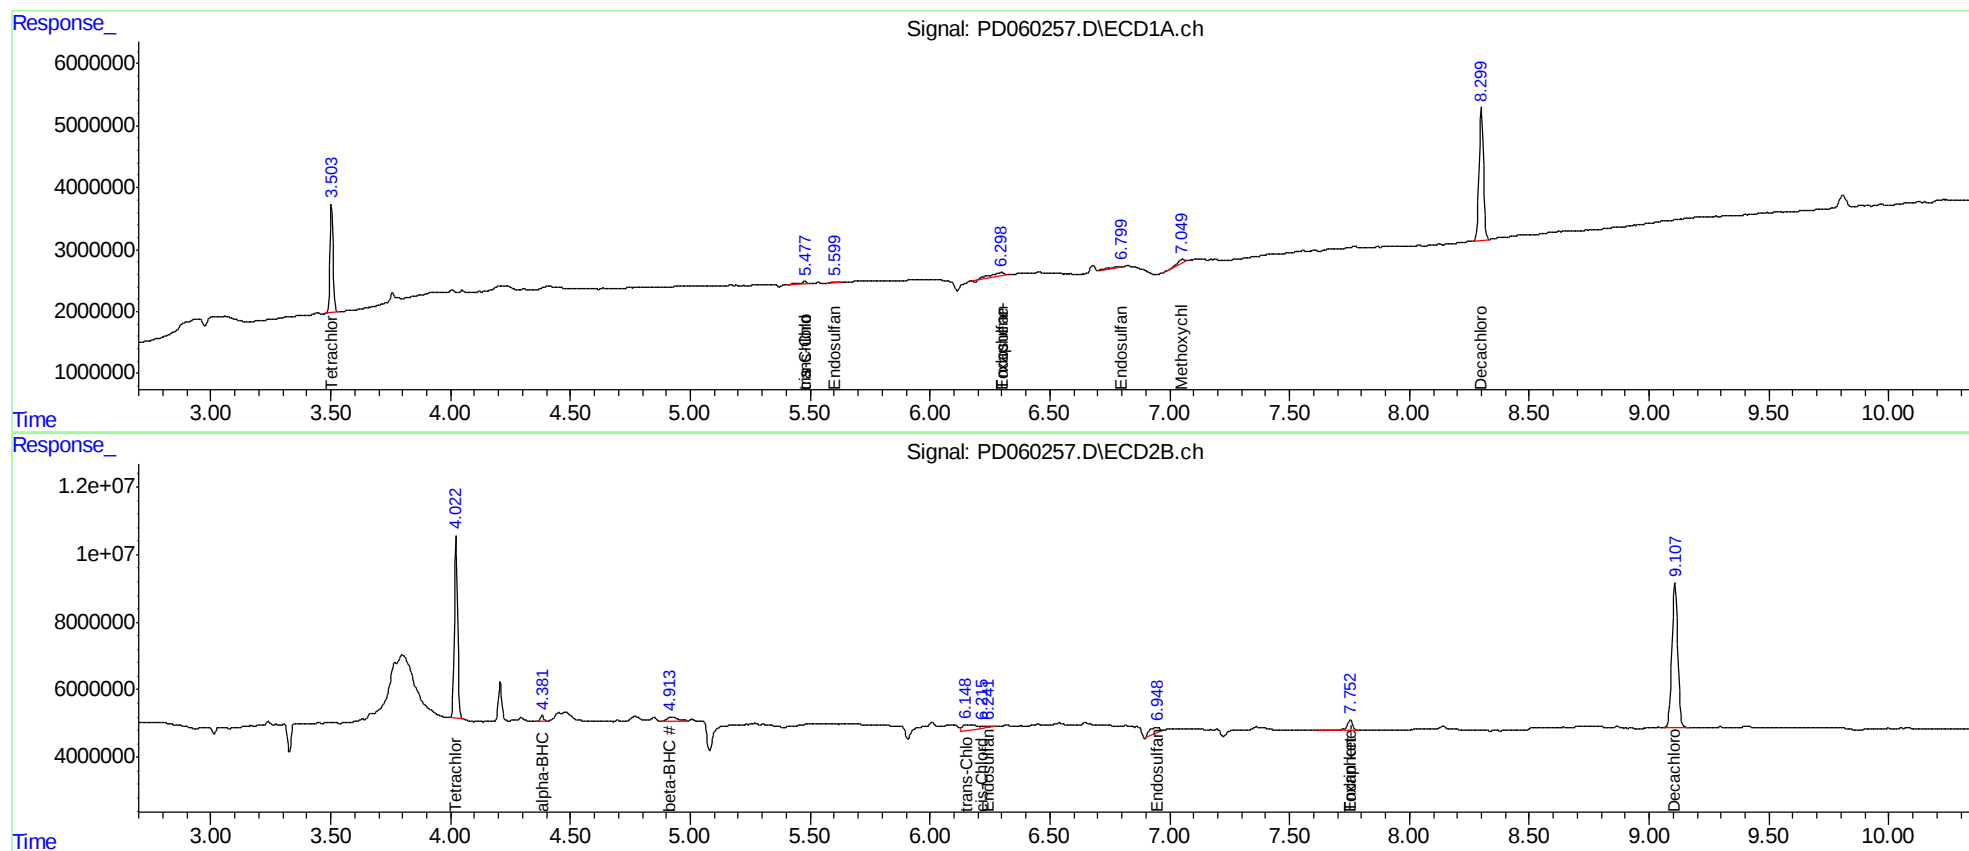


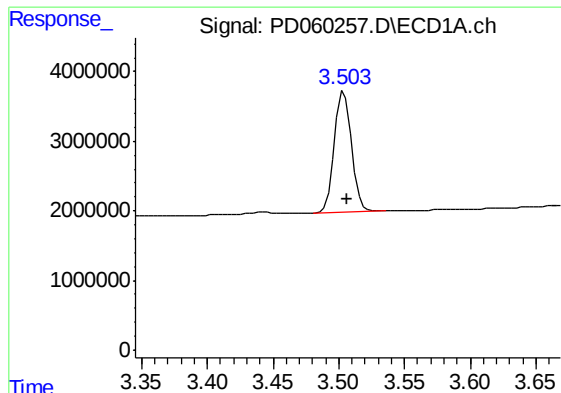

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: -0.002 min
Response: 15782638
Conc: 18.42 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BB2

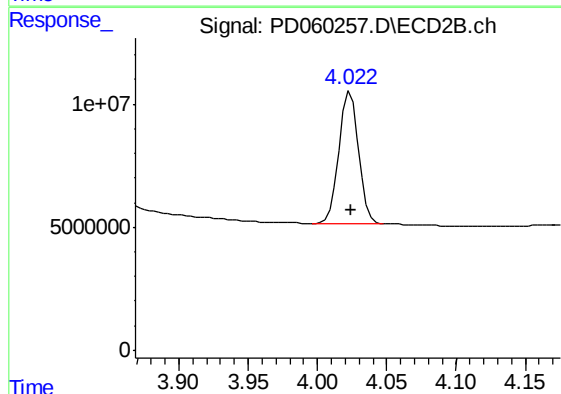


#1 Tetrachloro-m-xylene

R.T.: 4.024 min
Delta R.T.: 0.000 min
Response: 52858102
Conc: 17.73 ng/ml

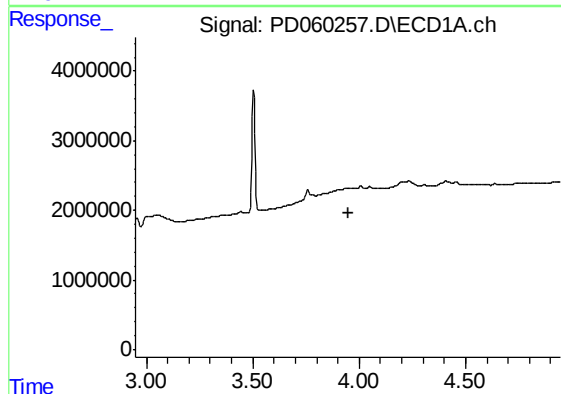


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.947 min
Response: 0
Conc: N.D.

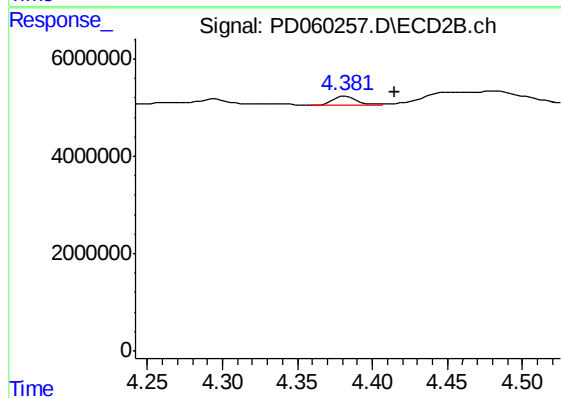

#2 alpha-BHC


R.T.: 4.383 min
Delta R.T.: -0.032 min
Response: 2003764
Conc: 0.45 ng/ml

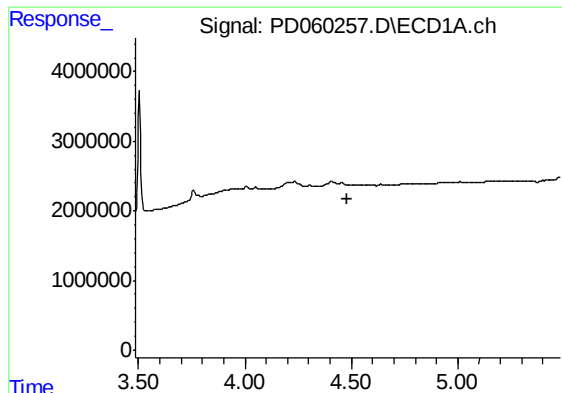

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :
C0BB2

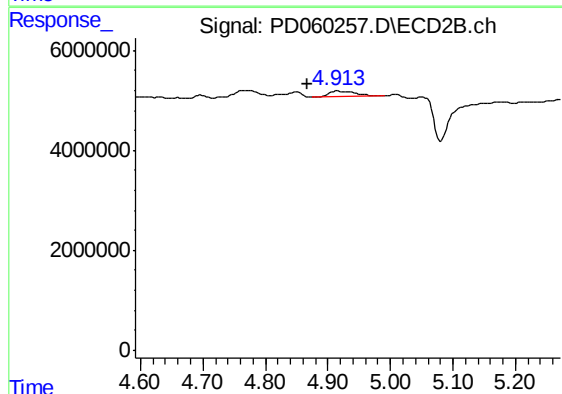


#6 beta-BHC

R.T.: 4.915 min
Delta R.T.: 0.047 min
Response: 3375816
Conc: 1.82 ng/ml

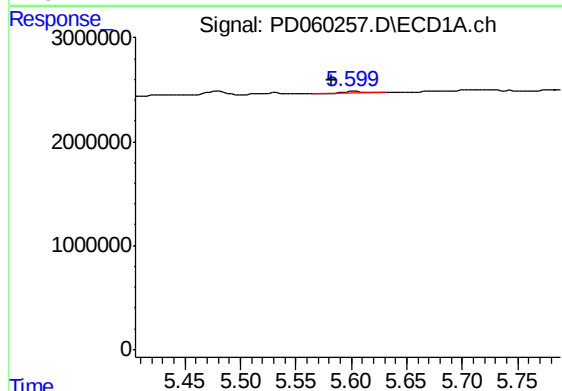


#9 Endosulfan I

R.T.: 5.602 min
Delta R.T.: 0.020 min
Response: 257085
Conc: 0.25 ng/ml

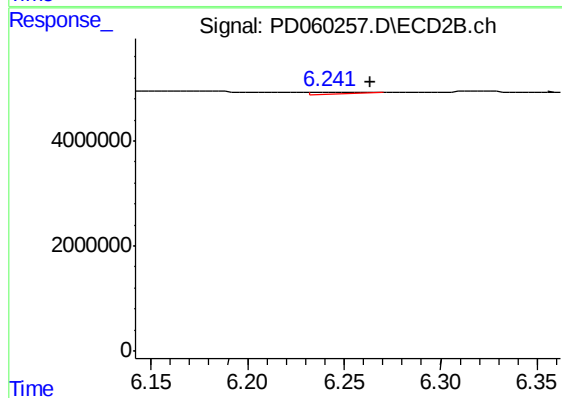

#9 Endosulfan I


R.T.: 6.242 min
Delta R.T.: -0.022 min
Response: 552941
Conc: 0.17 ng/ml

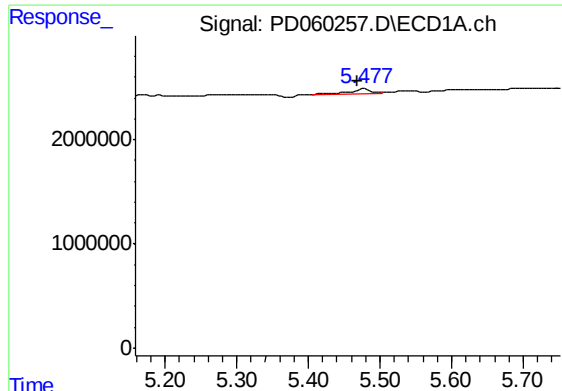

#10 trans-Chlordane


R.T.: 5.478 min
Delta R.T.: 0.010 min
Response: 850795
Conc: 0.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BB2

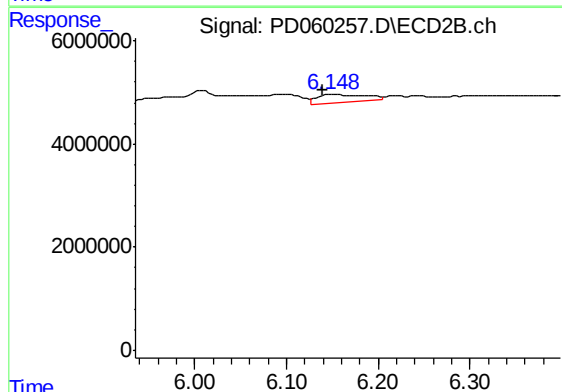


#10 trans-Chlordane

R.T.: 6.149 min
Delta R.T.: 0.009 min
Response: 5943175
Conc: 1.73 ng/ml

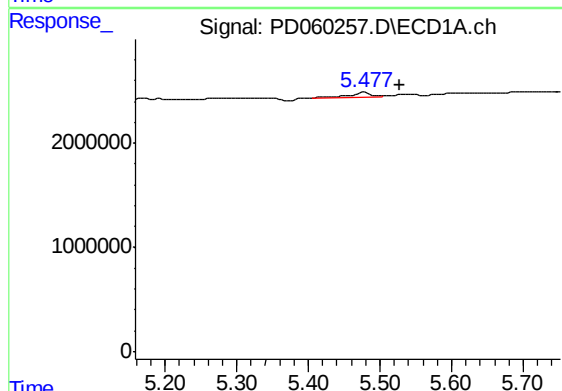


#11 cis-Chlordane

R.T.: 5.478 min
Delta R.T.: -0.049 min
Response: 850795
Conc: 0.80 ng/ml

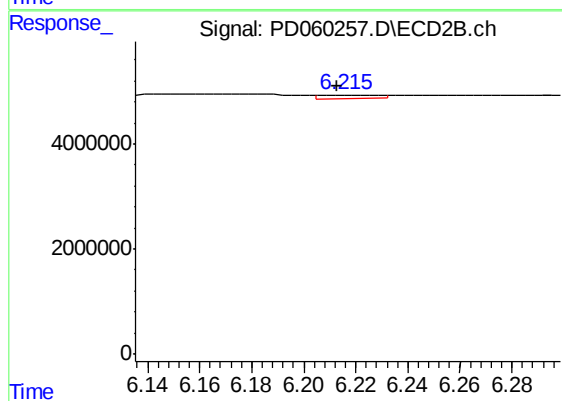

#11 cis-Chlordane


R.T.: 6.218 min
Delta R.T.: 0.005 min
Response: 1030119
Conc: 0.30 ng/ml

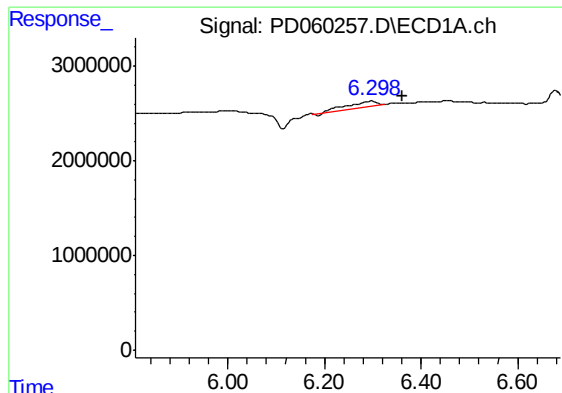

#15 Endosulfan II


R.T.: 6.299 min
Delta R.T.: -0.061 min
Response: 2375609
Conc: 2.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BB2

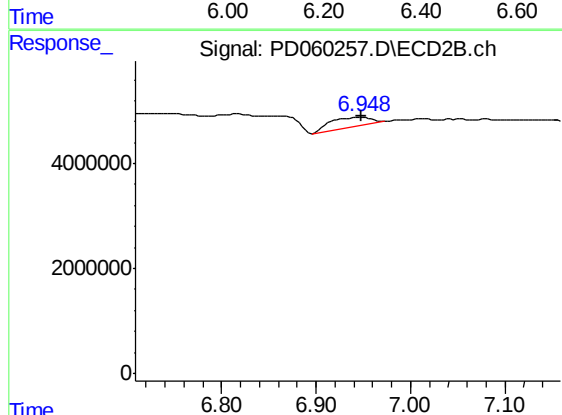


#15 Endosulfan II

R.T.: 6.949 min
Delta R.T.: 0.002 min
Response: 5551623
Conc: 1.96 ng/ml

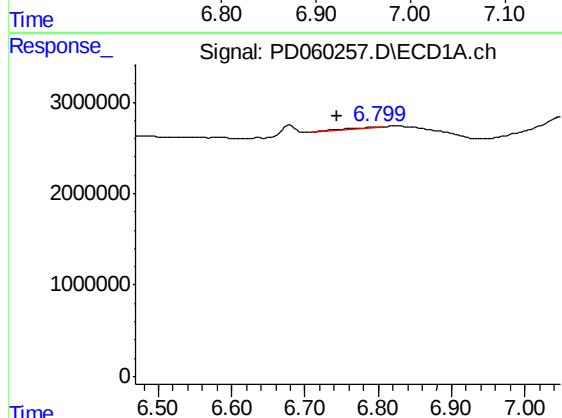


#19 Endosulfan Sulfate

R.T.: 6.801 min
Delta R.T.: 0.056 min
Response: 427325
Conc: 0.49 ng/ml

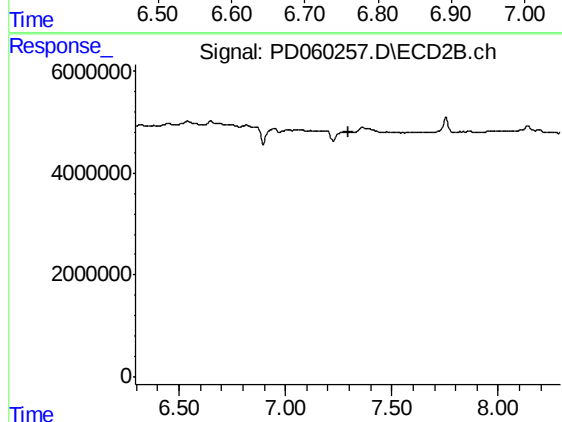

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.294 min
Response: 0
Conc: N.D.

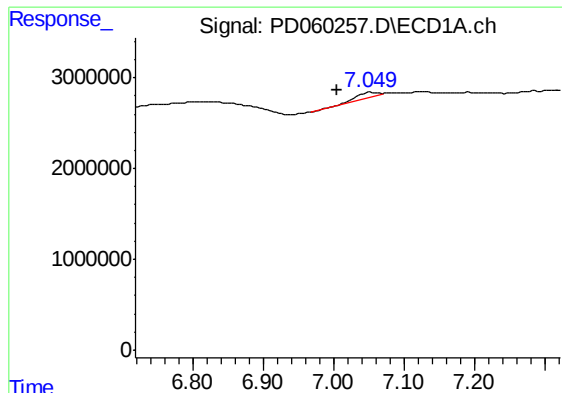

#20 Methoxychlor


R.T.: 7.052 min
Delta R.T.: 0.047 min
Response: 922134
Conc: 2.17 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BB2

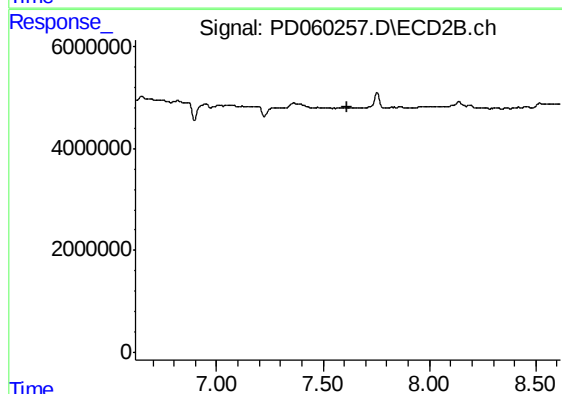


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.615 min
Response: 0
Conc: N.D.

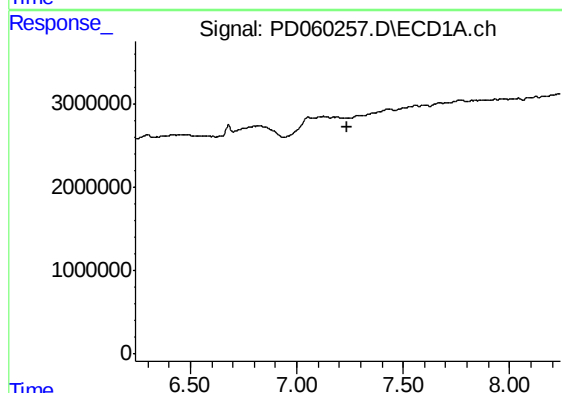


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.239 min
Response: 0
Conc: N.D.

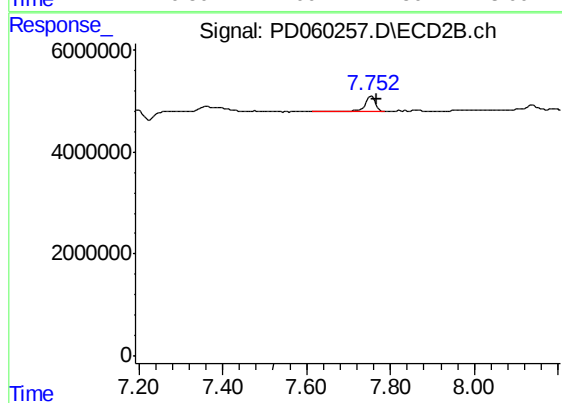

#21 Endrin ketone


R.T.: 7.754 min
Delta R.T.: -0.013 min
Response: 5254368
Conc: 1.80 ng/ml

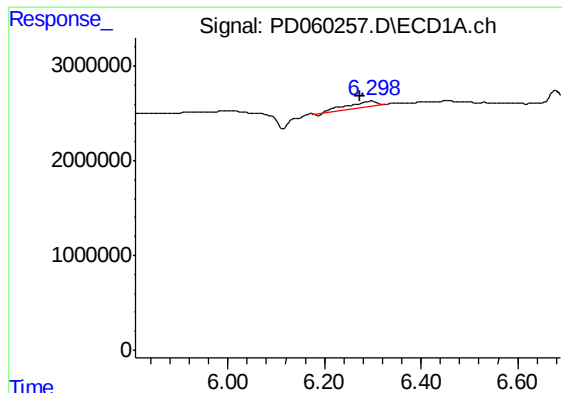

#24 Toxaphene-3


R.T.: 6.299 min
Delta R.T.: 0.025 min
Response: 2375609
Conc: 336.48 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BB2

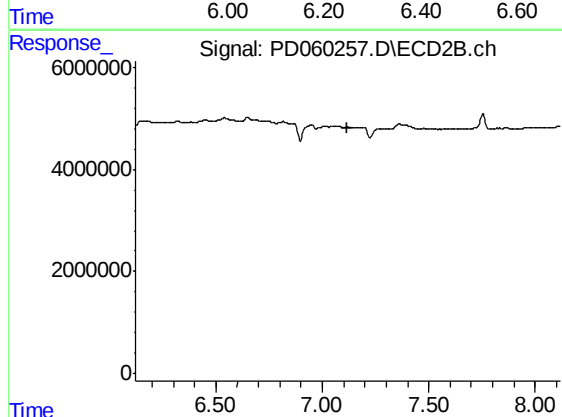


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 7.119 min
Response: 0
Conc: N.D.

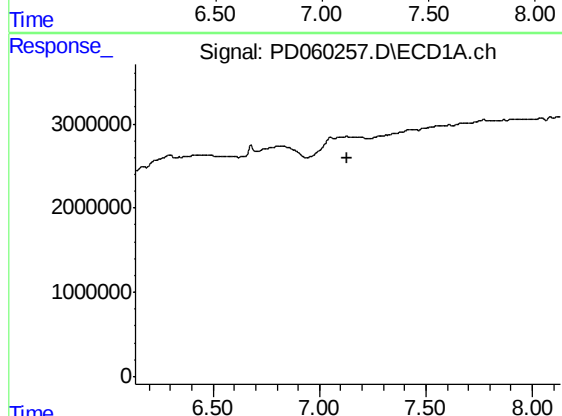


#26 Toxaphene-5

R.T.: 0.000 min
Exp R.T. : 7.133 min
Response: 0
Conc: N.D.

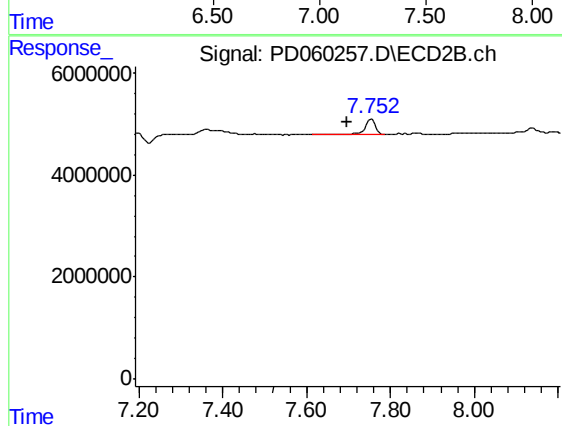

#26 Toxaphene-5


R.T.: 7.754 min
Delta R.T.: 0.058 min
Response: 5254368
Conc: 154.54 ng/ml

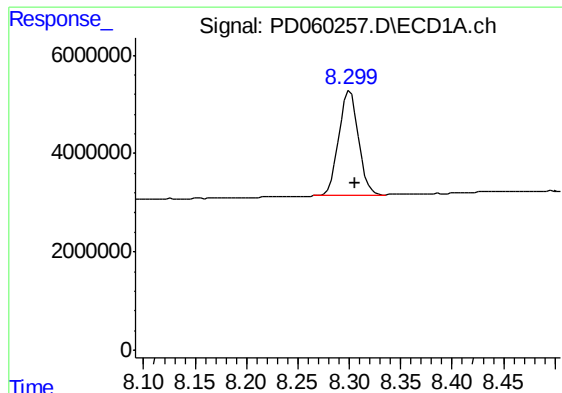

#27 Decachlorobiphenyl

R.T.: 8.301 min
Delta R.T.: -0.004 min
Response: 28451572
Conc: 34.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0BB2

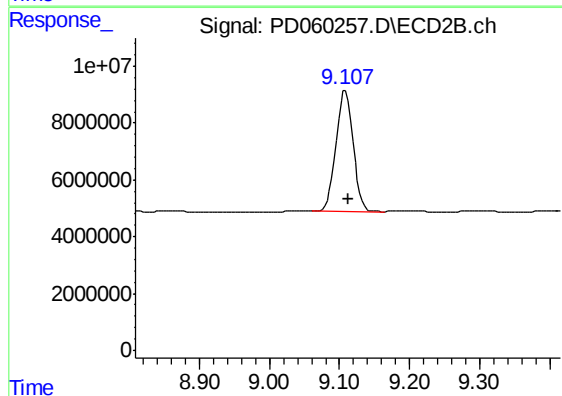

#27 Decachlorobiphenyl

R.T.: 9.108 min
Delta R.T.: -0.004 min
Response: 72513738
Conc: 29.48 ng/ml