

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
 Data File : PD060250.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 15:46
 Operator : DD\AJ
 Sample : L4793-04
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0BA5

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:51:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 00:30:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.023	7599795	24727675	8.868	8.295
27)	SA Decachlor...	8.301	9.109	10757949	26791943	12.948	10.891
Target Compounds							
10)	B trans-Chl...	5.466	6.138	9829317	47618536	9.255m	13.860m#
11)	B cis-Chlor...	5.524	6.213	13286274	114.0E6	12.559m	33.199m#
12)	B 4,4'-DDE	5.688	6.364	919180	11934366	0.899m	3.691 #
17)	MA 4,4'-DDT	6.451	7.156	1874824	2745707	2.086m	1.009m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
Data File : PD060250.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 15:46
Operator : DD\AJ
Sample : L4793-04
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 00:30:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

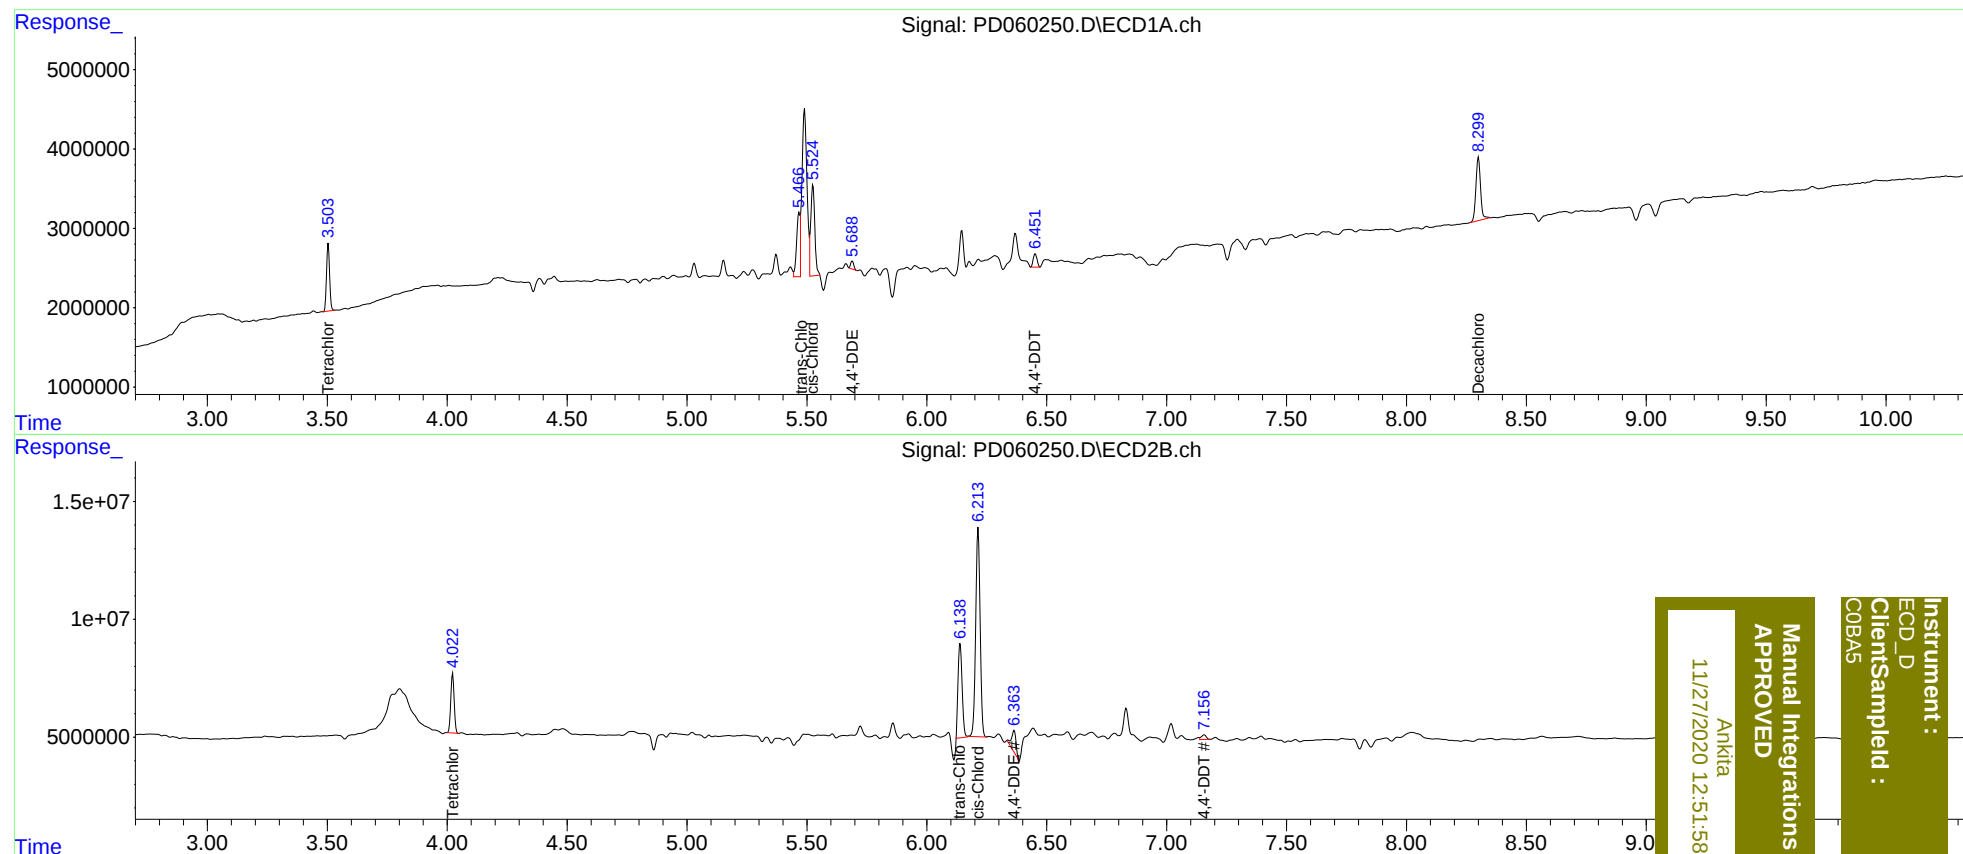

Manual Integrations
APPROVED

Ankita
11/27/2020 12:51:58 PM

Instrument :
ECD_D
ClientSampled :
COBAS