

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD112320\  
 Data File : PD060271.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 23 Nov 2020 20:54  
 Operator : DD\AJ  
 Sample : L4749-02MS  
 Misc :  
 ALS Vial : 50 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 C0B11MS

Manual Integrations  
 APPROVED

Ankita  
 11/25/2020 5:31:27 PM

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 24 00:38:33 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD110320CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Nov 04 04:05:33 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm


|                             | Compound        | RT#1  | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|-------|-------|----------|----------|--------|---------|
| -----                       |                 |       |       |          |          |        |         |
| System Monitoring Compounds |                 |       |       |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.504 | 4.023 | 14297001 | 47144716 | 16.683 | 15.816  |
| 27)                         | SA Decachlor... | 8.300 | 9.108 | 25526872 | 64956025 | 30.722 | 26.404  |
| Target Compounds            |                 |       |       |          |          |        |         |
| 3)                          | MA gamma-BHC... | 4.232 | 4.699 | 42089144 | 137.1E6  | 34.432 | 33.879  |
| 4)                          | MA Heptachlor   | 4.538 | 5.211 | 44414436 | 140.0E6  | 37.841 | 35.315  |
| 5)                          | MB Aldrin       | 4.790 | 5.516 | 43984445 | 143.7E6  | 38.311 | 38.722m |
| 10)                         | B trans-Chl...  | 5.464 | 6.136 | 1591596  | 9221516  | 1.499m | 2.684m# |
| 11)                         | B cis-Chlor...  | 5.524 | 6.212 | 3952741  | 22136290 | 3.737  | 6.447m# |
| 12)                         | B 4,4'-DDE      | 5.689 | 6.367 | 7249779  | 21446117 | 7.093  | 6.632   |
| 13)                         | MA Dieldrin     | 5.824 | 6.520 | 85219049 | 255.4E6  | 78.214 | 73.141  |
| 14)                         | MA Endrin       | 6.084 | 6.738 | 78636619 | 219.0E6  | 87.166 | 78.215  |
| 15)                         | B Endosulfa...  | 6.368 | 6.953 | 1405355  | 4217703  | 1.558  | 1.492m  |
| 17)                         | MA 4,4'-DDT     | 6.451 | 7.156 | 74158361 | 208.1E6  | 82.511 | 76.473  |
| -----                       |                 |       |       |          |          |        |         |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD112320\  
Data File : PD060271.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 23 Nov 2020 20:54  
Operator : DD\AJ  
Sample : L4749-02MS  
Misc :  
ALS Vial : 50 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 24 00:38:33 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD110320CLP.M  
Quant Title : GC Extractables  
QLast Update : Wed Nov 04 04:05:33 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

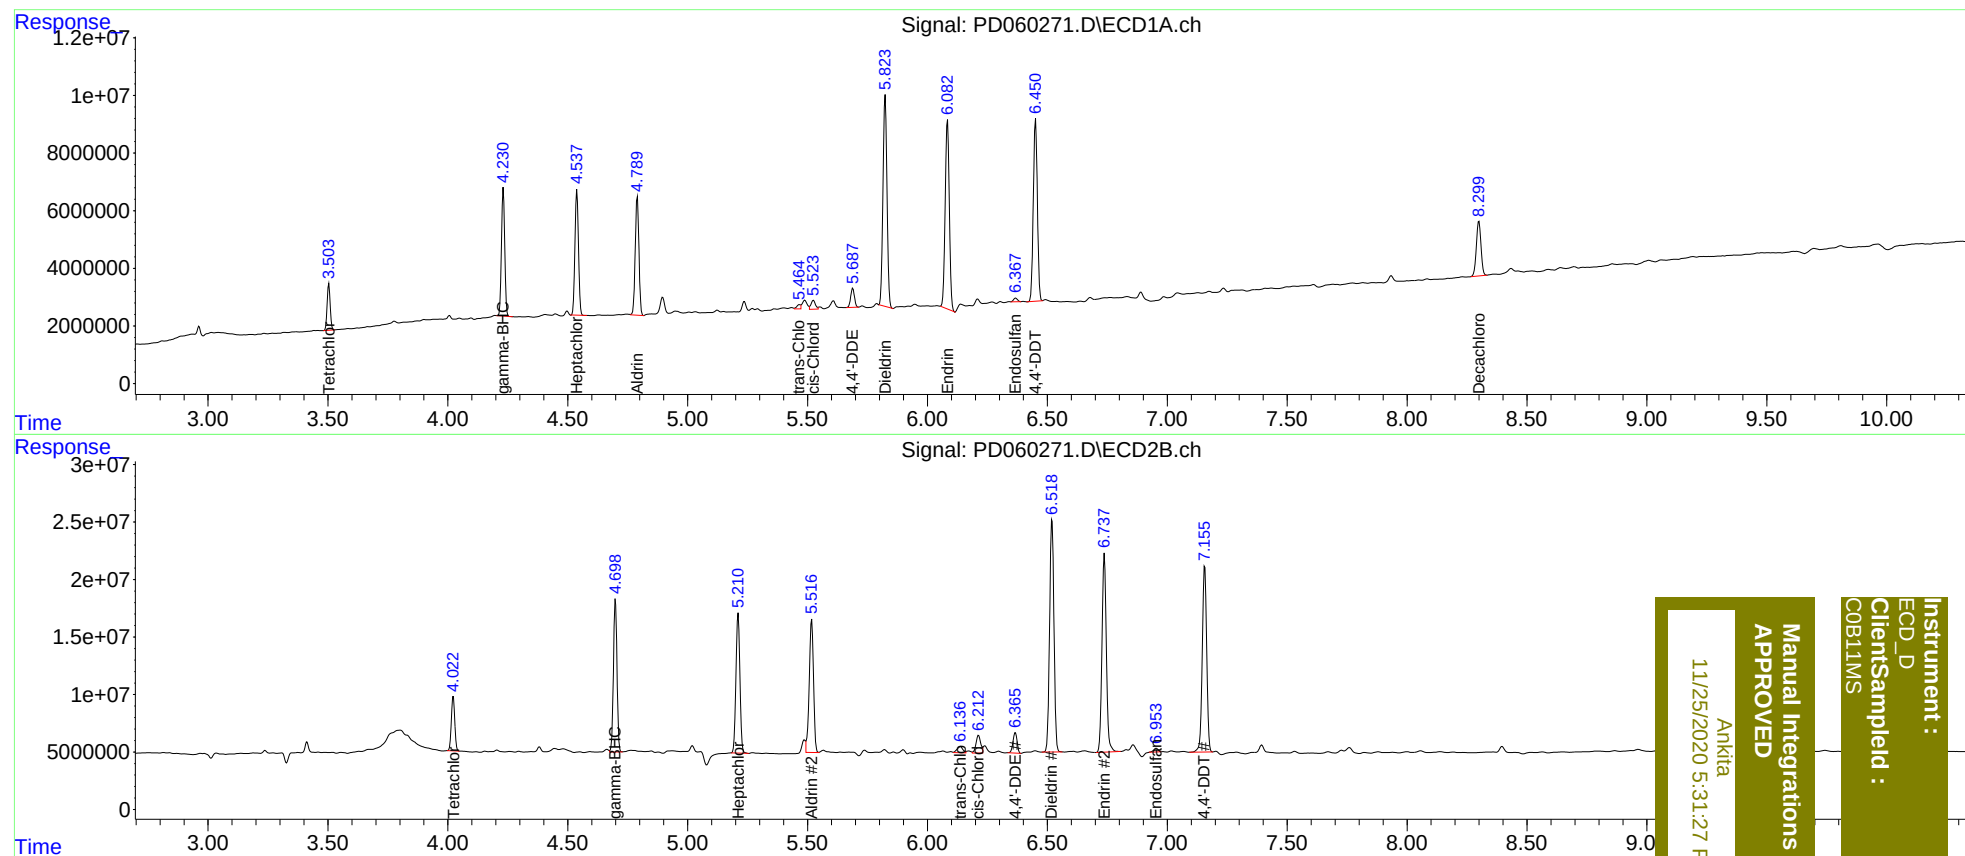

Manual Integrations  
APPROVED

Ankita

11/25/2020 5:31:27 PM

Instrument :  
ECD\_D  
ClientSampled :  
COB11MS