

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
 Data File : PD060225.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 09:55
 Operator : DD\AJ
 Sample : L4751-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B90

Manual Integrations
 APPROVED

Ankita
 11/27/2020 12:51:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 03:52:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.505	4.023	8712813	24639736	10.167	8.266
2) SA Decachlor...	8.302	9.110	11690893	30825787	14.070	12.531
Target Compounds						
10) B trans-Chl...	5.468	6.140	3807559	13741512	3.585m	4.000m
11) B cis-Chlor...	5.525	6.213	6478305	52900430	6.124m	15.408m#
12) B 4,4'-DDE	5.686	6.362	1266113	9366275	1.239m	2.897m#
17) MA 4,4'-DDT	6.453	7.155	3181900	4033674	3.540m	1.482m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
Data File : PD060225.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 09:55
Operator : DD\AJ
Sample : L4751-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 03:52:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

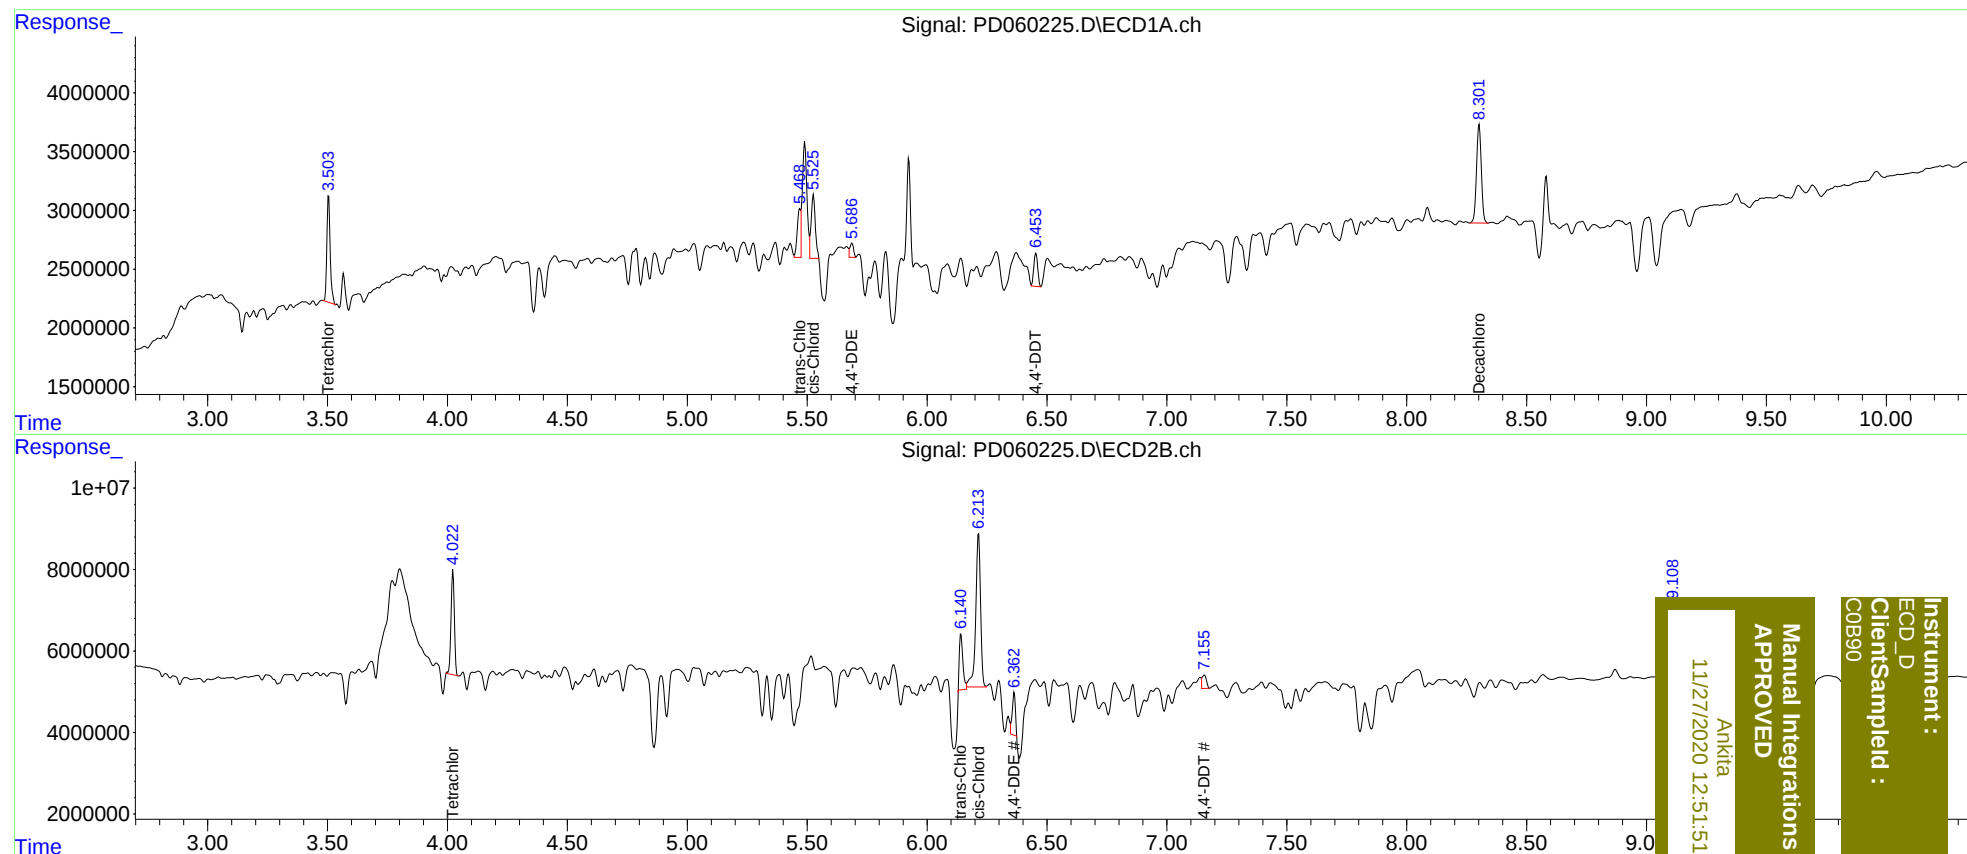

Manual Integrations
APPROVED

Ankita
11/27/2020 12:51:51 PM

Instrument :
ECD_D
Client Sampled :
C0890