

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
 Data File : PD060260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 18:06
 Operator : DD\AJ
 Sample : L4793-12
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B31

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:31:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 00:34:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.504	4.023	6803129	21619972	7.939	7.253
27) SA Decachlor...	8.298	9.108	12050910	25348821	14.504	10.304 #
Target Compounds						
10) B trans-Chl...	5.471	6.139	2139688	18987679	2.015m	5.527m#
11) B cis-Chlor...	5.523	6.213	2142100	22338187	2.025m	6.506m#
12) B 4,4'-DDE	5.689	6.362	1812469	8526998	1.773	2.637m#
17) MA 4,4'-DDT	6.449	7.155	3714917	5183252	4.133m	1.905m#
19) B Endosulfa...	6.739	7.278	596994	3300955	0.683	1.145 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
Data File : PD060260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 18:06
Operator : DD\AJ
Sample : L4793-12
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 00:34:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

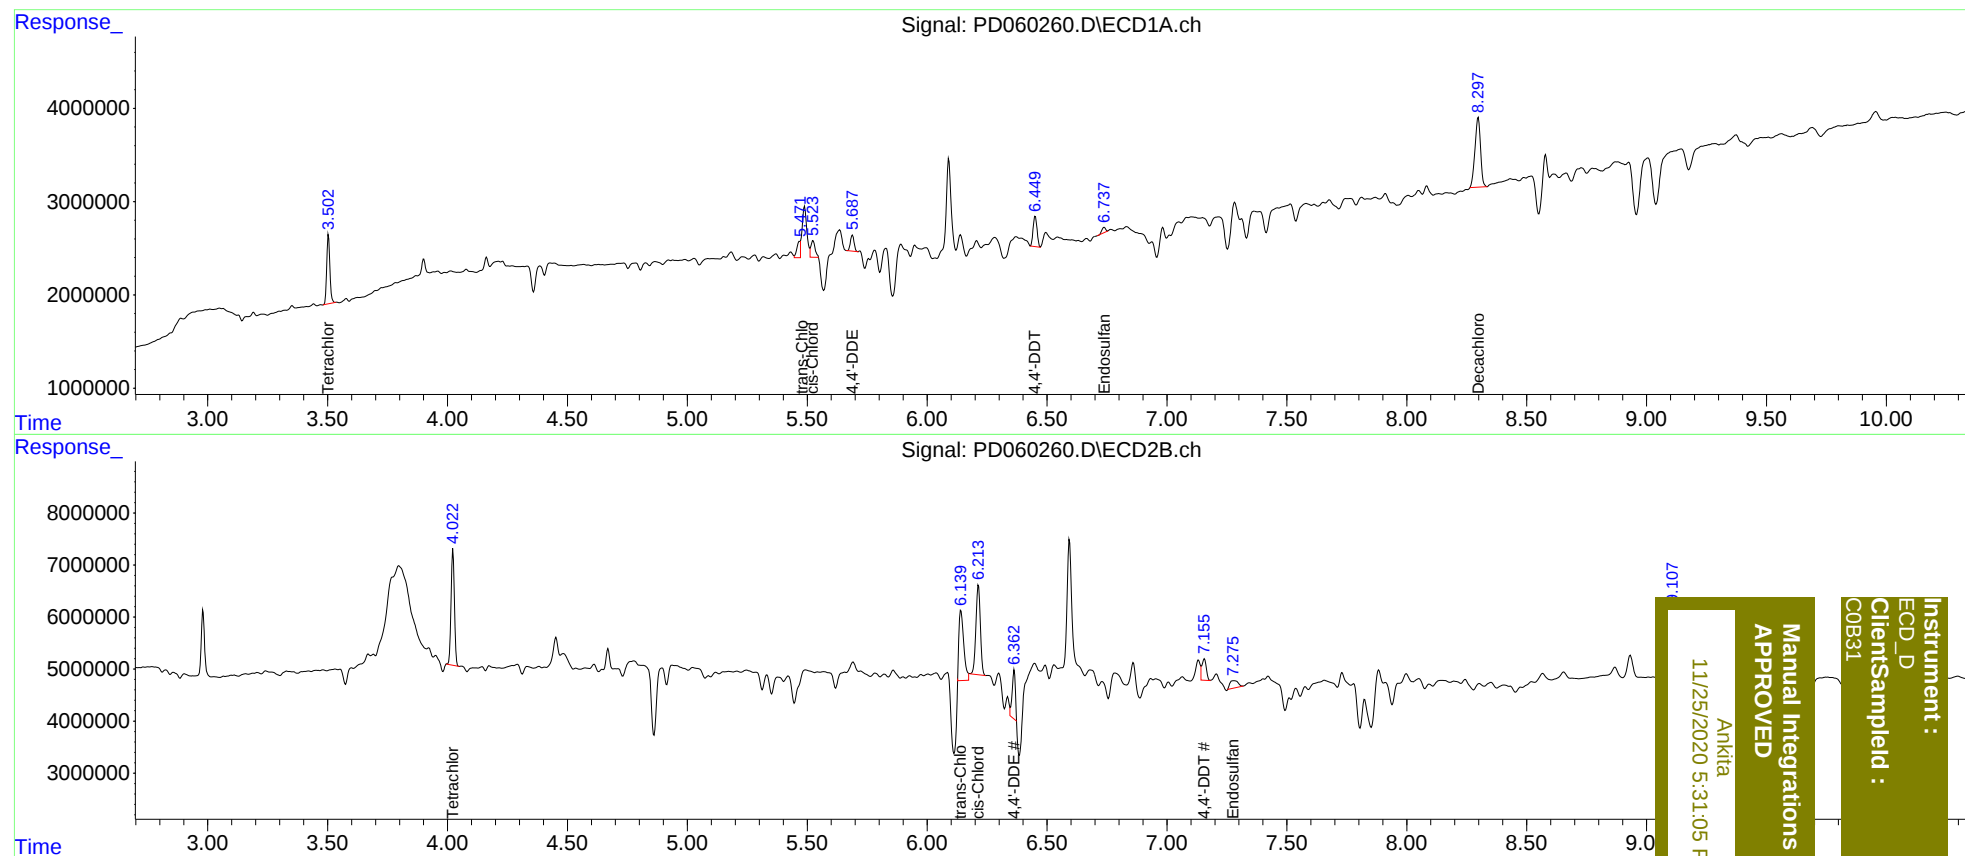

Instrument :
ECD_D
Client Sampled :
C0831

Manual Integrations
APPROVED
Ankita
11/25/2020 5:31:05 PM