

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
 Data File : PD060261.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 18:20
 Operator : DD\AJ
 Sample : L4793-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B38

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:31:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 00:34:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.023	9749583	32045962	11.377	10.750
27)	SA Decachlor...	8.300	9.109	16729620	40766108	20.135	16.571
Target Compounds							
8)	B Heptachlo...	5.237	5.903	2663202	4624076	2.521	1.404m#
10)	B trans-Chl...	5.471	6.139	1379367	5263344	1.299m	1.532m
11)	B cis-Chlor...	5.523	6.213	1730273	17234436	1.636m	5.020m#
12)	B 4,4'-DDE	5.689	6.363	1500395	5947597	1.468	1.839m#
17)	MA 4,4'-DDT	6.450	7.156	2027488	4501979	2.256m	1.654m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
Data File : PD060261.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 18:20
Operator : DD\AJ
Sample : L4793-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 00:34:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

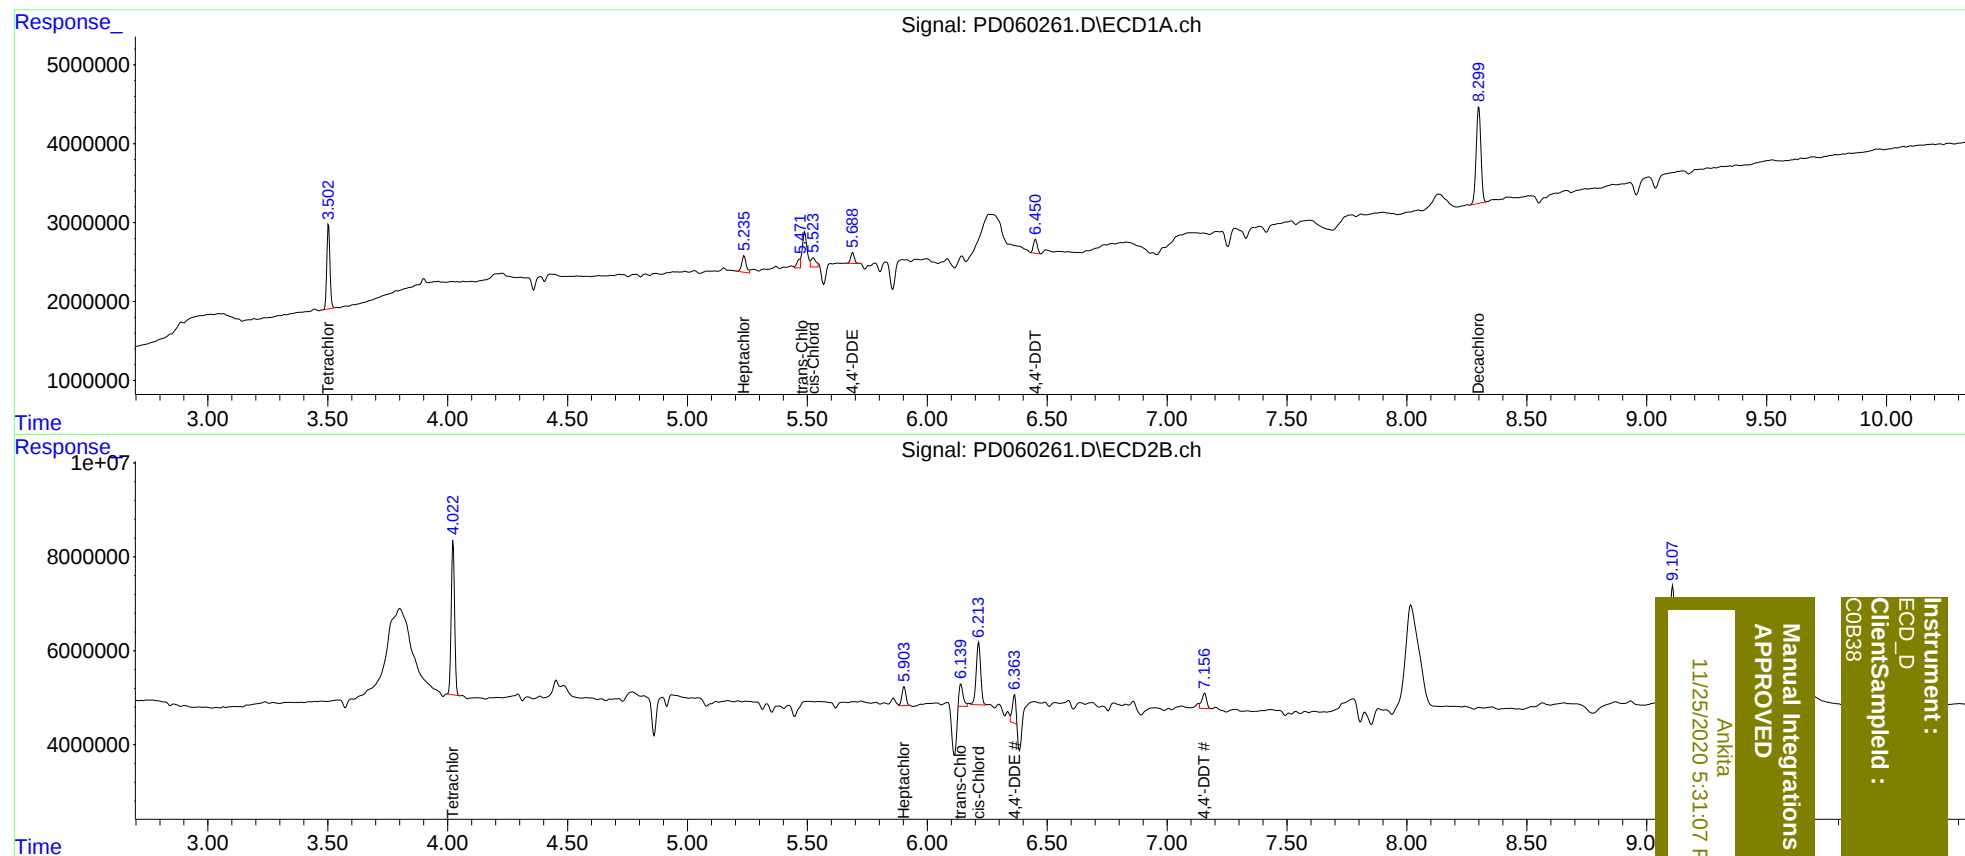

11/25/2020 5:31:07 PM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sample :
COB38