

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
 Data File : PD060263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2020 18:48
 Operator : DD\AJ
 Sample : L4793-15
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0B42

Manual Integrations
 APPROVED

Ankita
 11/25/2020 5:31:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 24 00:35:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 04 04:05:33 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.504	4.024	7599547	24927893	8.868	8.363
27) SA Decachlor...	8.301	9.109	10847610	26518442	13.055	10.780
Target Compounds						
8) B Heptachlo...	5.238	5.923	1548023	3492422	1.465	1.060m#
10) B trans-Chl...	5.466	6.137	7976200	47099036	7.510m	13.709m#
11) B cis-Chlor...	5.523	6.213	12418800	116.3E6	11.739m	33.865m#
12) B 4,4'-DDE	5.688	6.364	1151952	12374593	1.127m	3.827 #
17) MA 4,4'-DDT	6.451	7.155	1932839	2726677	2.151m	1.002m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112320\
Data File : PD060263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2020 18:48
Operator : DD\AJ
Sample : L4793-15
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 24 00:35:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD110320CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 04 04:05:33 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

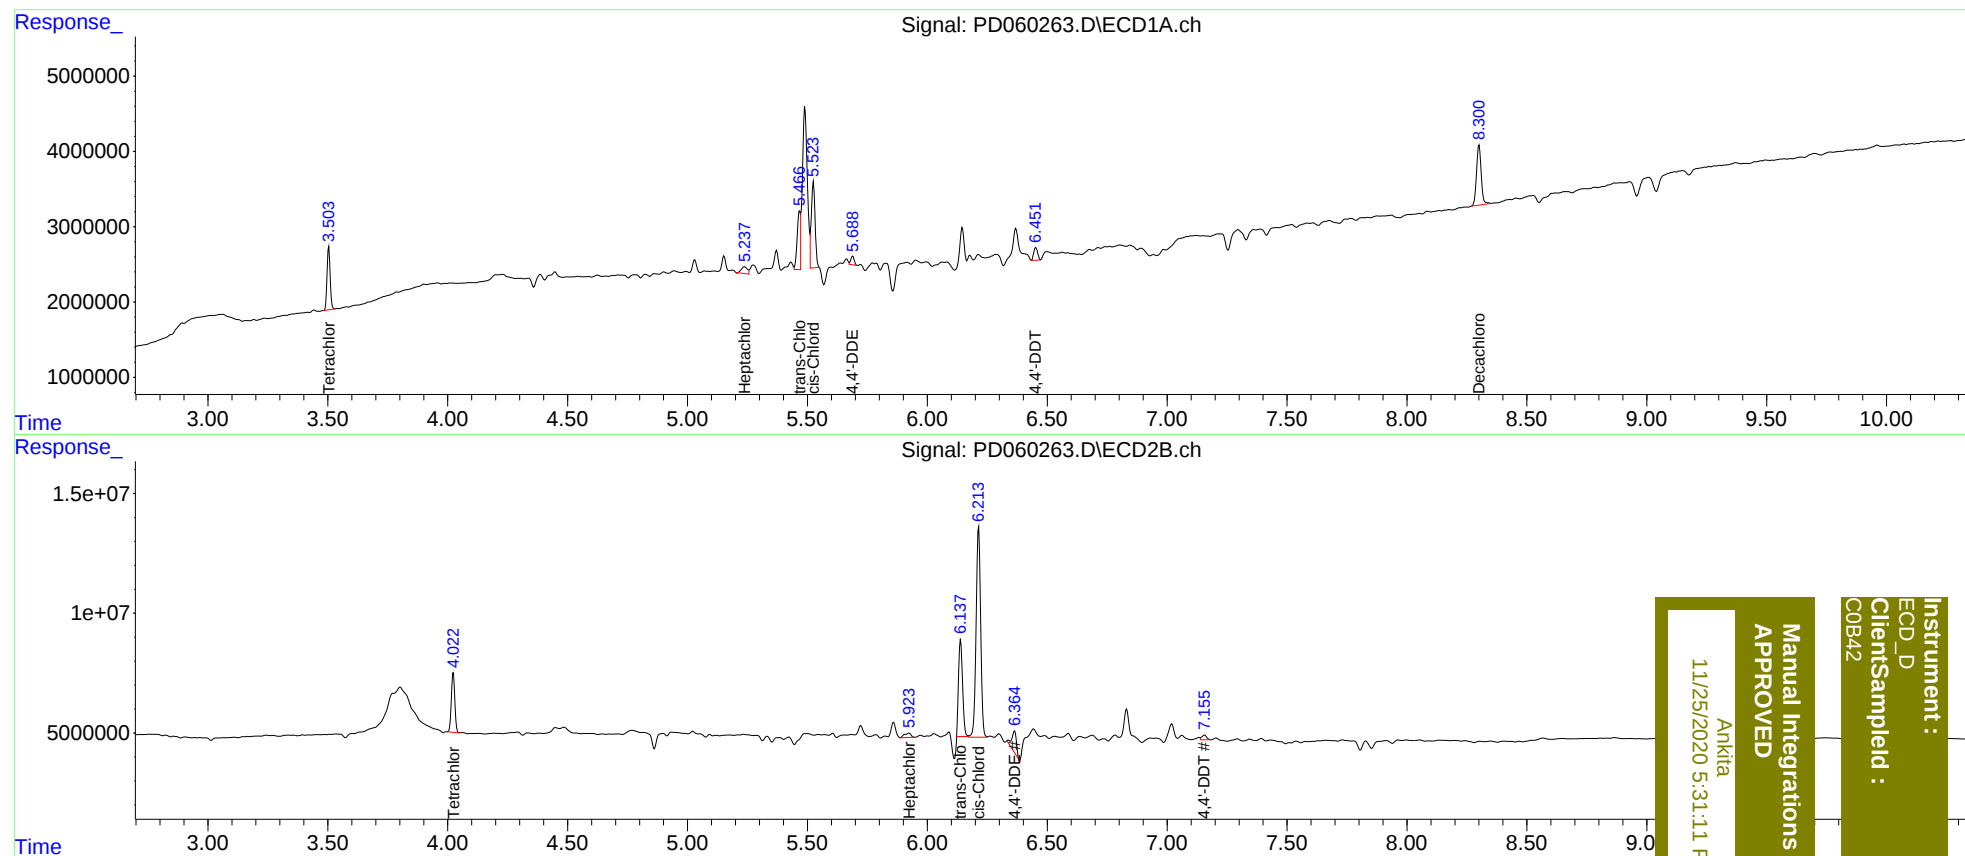

Manual Integrations
APPROVED

Ankita
11/25/2020 5:31:11 PM

Instrument :
ECD_D
ClientSampled :
C0B42