

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
 Data File : PD073226.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 19:35
 Operator : AR\AJ
 Sample : N5659-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQT8

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/25/2022
 Supervised By : Ankita Jodhani 11/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 01:12:20 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	2.698	3.459	47553591	1236.7E6	19.831	18.931
27) SA Decachlor...	7.824	8.907	76359653	496.8E6	33.464	33.574
Target Compounds						
5) MB Aldrin	4.138	5.159	1865647	21538025	0.554m	0.536
10) B trans-Chl...	4.891	5.858	1449889	61681102	0.470m	1.953m#
13) MA Dieldrin	5.280	6.253	24932792	222.8E6	8.139	7.393

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
Data File : PD073226.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 19:35
Operator : AR\AJ
Sample : N5659-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 01:12:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

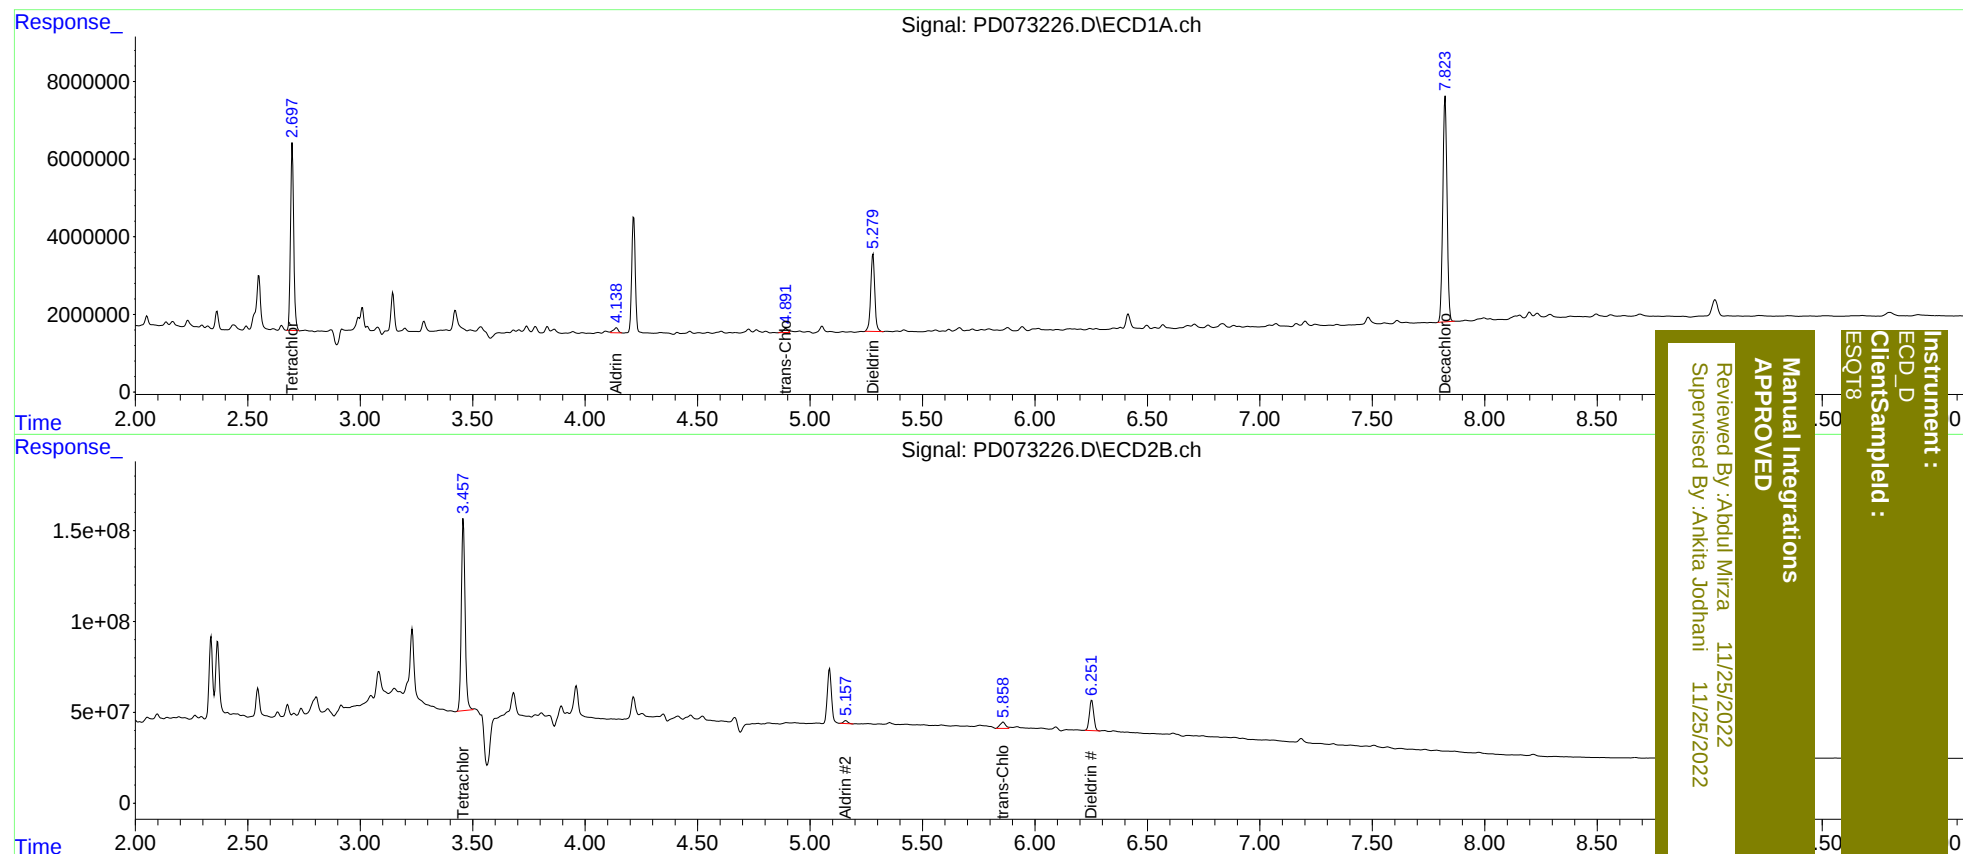

Instrument :
ECD_D
ClientSampled :
ESQ18

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/25/2022
Supervised By :Ankita Jodhani 11/25/2022