

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
 Data File : PD073228.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 20:01
 Operator : AR\AJ
 Sample : N5659-05MSD
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQT8MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/28/2022
 Supervised By : Ankita Jodhani 11/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 01:13:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	43885988	1158.2E6	18.301	17.730
27)	SA Decachlor...	7.823	8.907	75202861	494.6E6	32.957	33.420
Target Compounds							
2)	A alpha-BHC	3.200	3.923	189.7E6	3722.1E6	51.847	42.682
3)	MA gamma-BHC...	3.530	4.256	172.6E6	2916.1E6	52.000	42.977
4)	MA Heptachlor	3.862	4.821	166.4E6	1942.9E6	49.799	42.309
5)	MB Aldrin	4.141	5.160	175.9E6	1767.5E6	52.209	44.010
6)	B beta-BHC	3.831	4.469	66160494	1112.6E6	41.208	41.640m
7)	B delta-BHC	4.061	4.714	172.8E6	2185.5E6	47.541	40.167
8)	B Heptachlo...	4.645	5.592	147.3E6	1445.0E6	47.397	42.750
9)	A Endosulfan I	5.014	5.976	133.2E6	1332.2E6	47.117	45.798
10)	B trans-Chl...	4.893	5.845	153.1E6	1428.3E6	49.662	45.213
11)	B cis-Chlor...	4.957	5.921	148.8E6	1403.2E6	47.524	44.199
12)	B 4,4'-DDE	5.145	6.094	299.7E6	2715.4E6	100.175	90.446
13)	MA Dieldrin	5.280	6.253	345.4E6	3088.3E6	112.734	102.454
14)	MA Endrin	5.556	6.484	279.9E6	2398.4E6	103.261	97.230
15)	B Endosulfa...	5.854	6.714	262.8E6	2302.9E6	97.573	95.326
16)	A 4,4'-DDD	5.703	6.618	244.0E6	2193.1E6	101.294	95.693
17)	MA 4,4'-DDT	5.951	6.926	255.4E6	2233.0E6	114.176	103.970
18)	B Endrin al...	6.036	6.845	186.4E6	1641.2E6	86.321	86.632
19)	B Endosulfa...	6.259	7.078	240.6E6	1971.7E6	95.888	94.817
20)	A Methoxychlor	6.535	7.406	636.4E6	4582.0E6	508.094	491.078
21)	B Endrin ke...	6.769	7.568	295.0E6	2191.4E6	101.049	98.146

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
Data File : PD073228.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 20:01
Operator : AR\AJ
Sample : N5659-05MSD
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 01:13:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD11722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

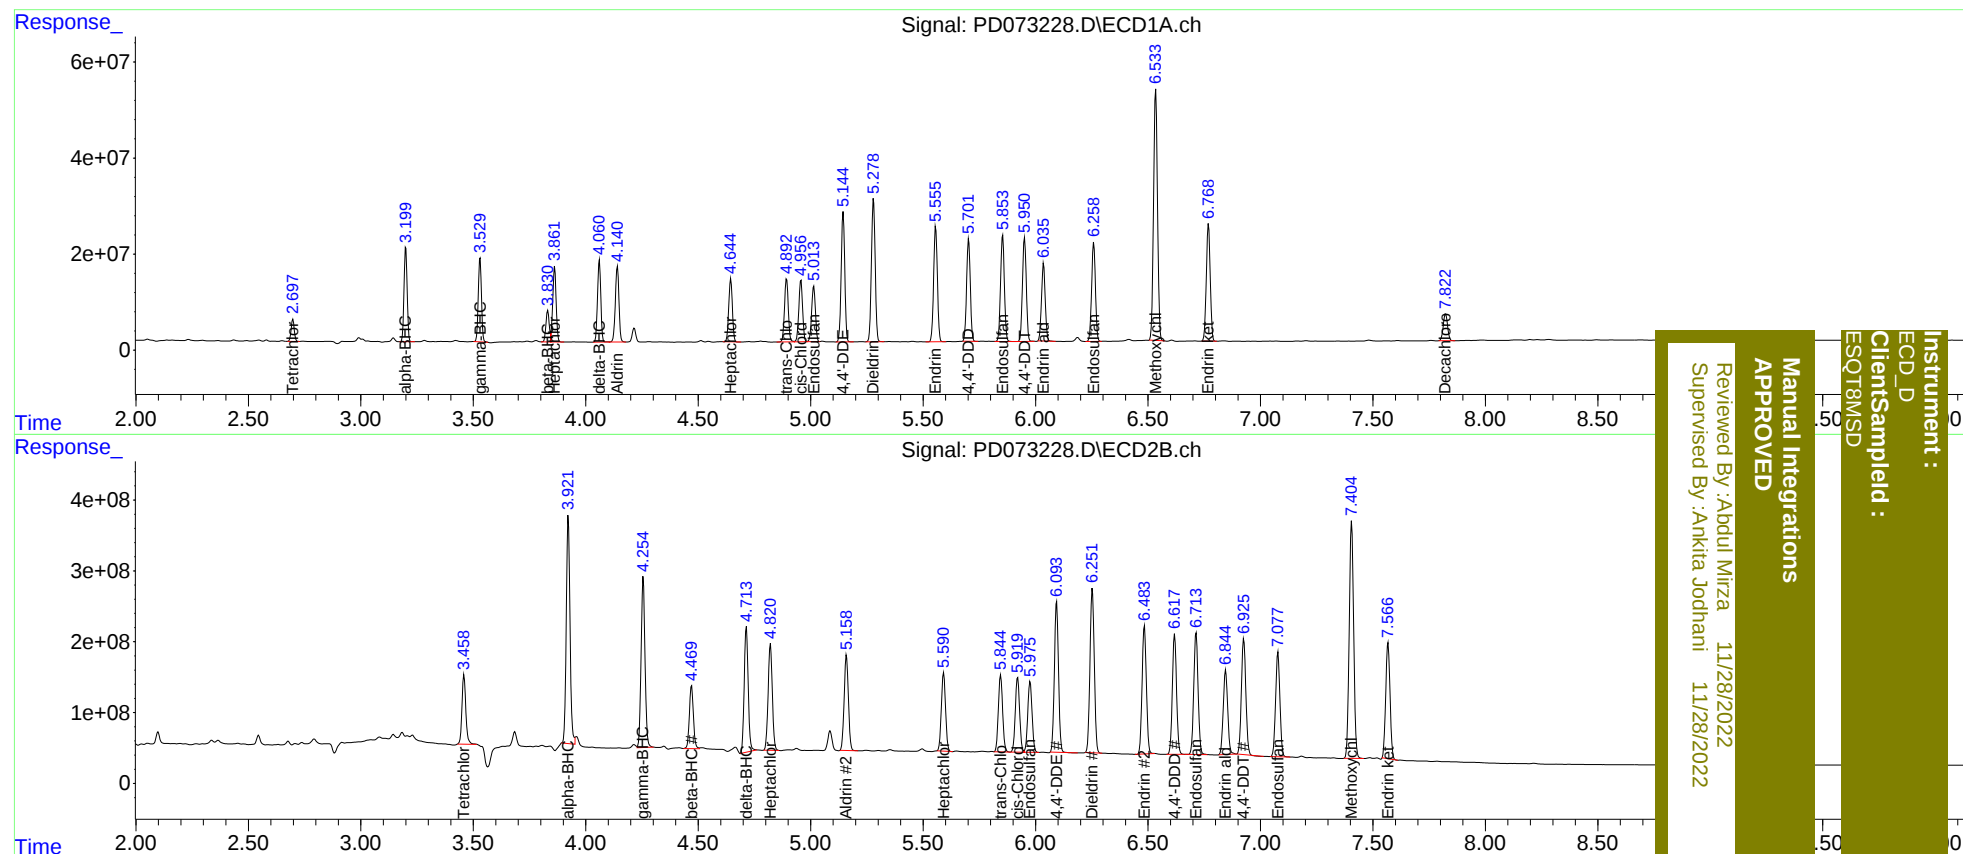

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/28/2022
Supervised By: Ankita Jodhani 11/28/2022

Instrument :
ECD_D
ClientSampled :
ESQ8MSD