

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
 Data File : PD073215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 17:08
 Operator : AR\AJ
 Sample : PB149253BS
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS253

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/28/2022
 Supervised By : Ankita Jodhani 11/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 01:09:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	42838807	1157.2E6	17.865	17.714
2)	SA Decachlor...	7.824	8.907	90582444	599.1E6	39.696	40.484
Target Compounds							
2)	A alpha-BHC	3.200	3.922	15355861	420.7E6	4.196	4.824
3)	MA gamma-BHC...	3.530	4.256	15111874	355.1E6	4.554	5.233
4)	MA Heptachlor	3.862	4.821	14964607	233.5E6	4.479	5.085
5)	MB Aldrin	4.141	5.160	15487705	212.6E6	4.596	5.294
6)	B beta-BHC	3.832	4.470	7541507	132.4E6	4.697	4.956m
7)	B delta-BHC	4.061	4.715	14900697	269.9E6	4.100	4.960
8)	B Heptachlo...	4.645	5.592	14627535	175.4E6	4.708	5.188
9)	A Endosulfan I	5.014	5.977	13651760	155.1E6	4.831	5.332
10)	B trans-Chl...	4.894	5.846	14635419	160.0E6	4.749	5.066
11)	B cis-Chlor...	4.957	5.921	14757720	161.2E6	4.713	5.077
12)	B 4,4'-DDE	5.145	6.095	25652910	296.0E6	8.575	9.860
13)	MA Dieldrin	5.280	6.253	28071340	318.1E6	9.163	10.553
14)	MA Endrin	5.557	6.485	24346864	253.3E6	8.981	10.271
15)	B Endosulfa...	5.855	6.715	25370573	257.3E6	9.421	10.650
16)	A 4,4'-DDD	5.703	6.619	22474926	244.0E6	9.328	10.645
17)	MA 4,4'-DDT	5.952	6.926	20069266	218.7E6	8.972	10.185
18)	B Endrin al...	6.037	6.846	21290083	203.7E6	9.857	10.751
19)	B Endosulfa...	6.260	7.078	23939088	215.3E6	9.541	10.354
20)	A Methoxychlor	6.536	7.406	61164592	494.6E6	48.835	53.013
21)	B Endrin ke...	6.770	7.568	29837941	248.8E6	10.222	11.144

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
Data File : PD073215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 17:08
Operator : AR\AJ
Sample : PB149253BS
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 01:09:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD11722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

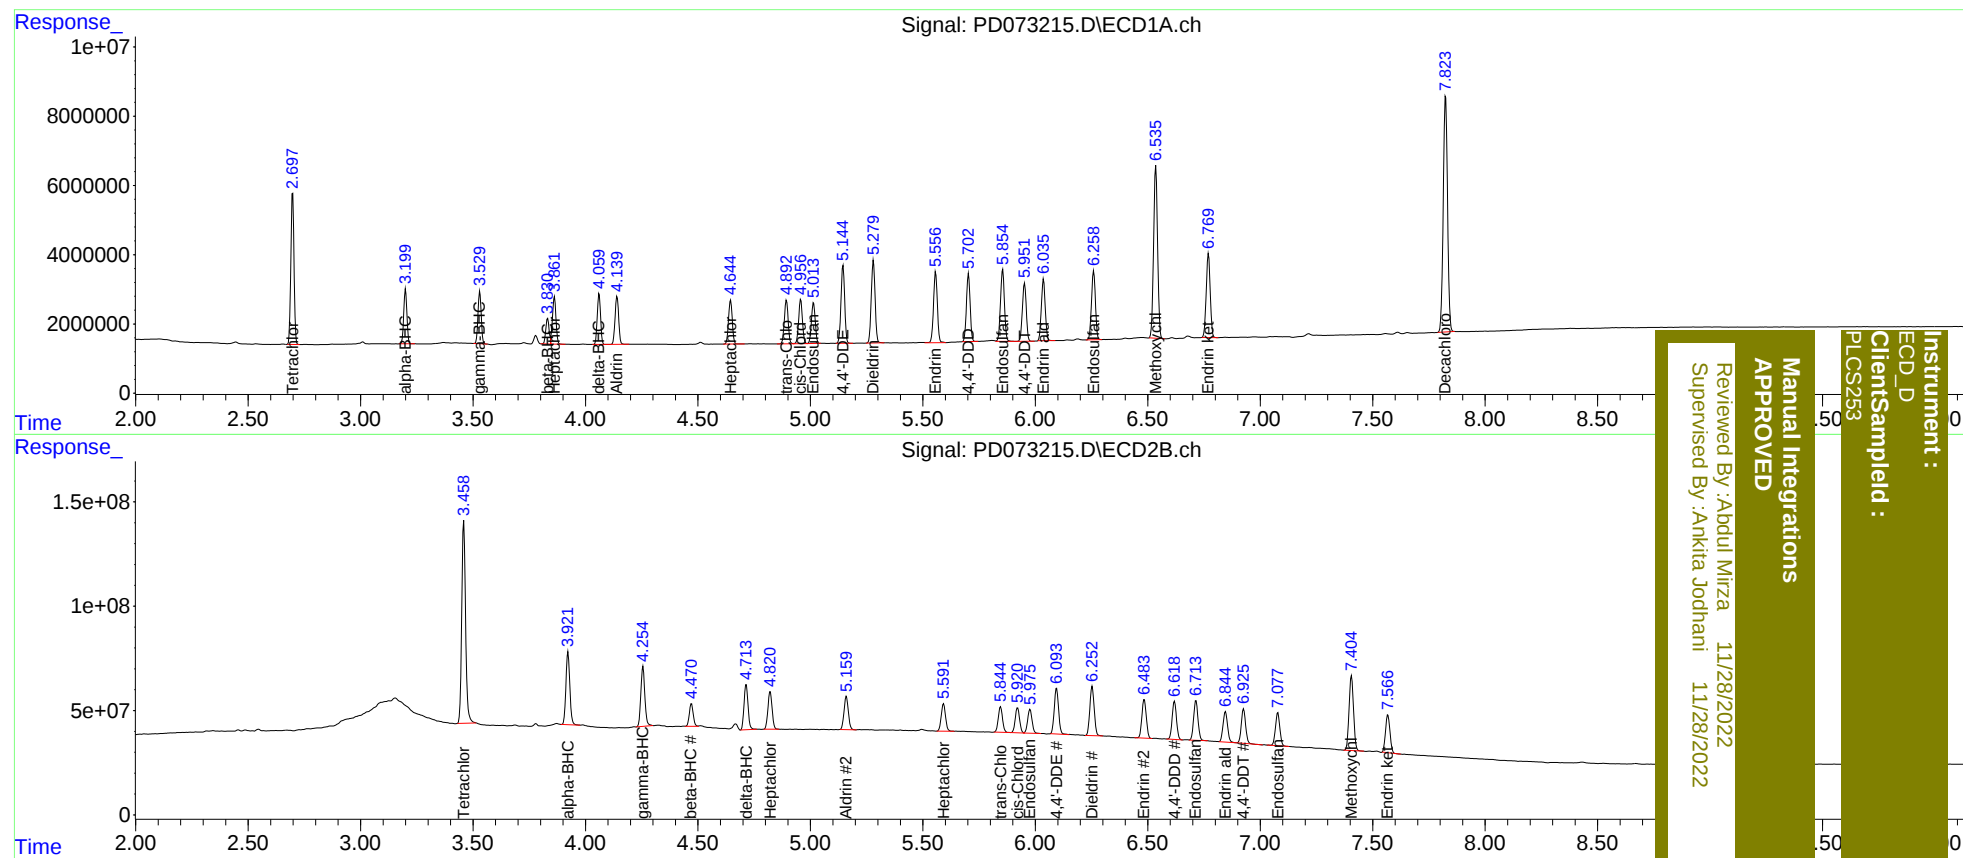

Instrument :
ECD_D
ClientSampled :
PLCS253

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/28/2022
Supervised By :Ankita Jodhani 11/28/2022