

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
 Data File : PD073218.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 17:48
 Operator : AR\AJ
 Sample : N5683-03MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQW0MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/28/2022
 Supervised By : Ankita Jodhani 11/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 01:09:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.461	35095700	1215.8E6	14.636	18.612 #
27)	SA Decachlor...	7.824	8.908	43794184	289.9E6	19.192	19.592
Target Compounds							
2)	A alpha-BHC	3.201	3.923	127.8E6	2749.7E6	34.926	31.532
3)	MA gamma-BHC...	3.531	4.256	130.6E6	2332.4E6	39.338	34.375
4)	MA Heptachlor	3.862	4.822	132.3E6	1631.6E6	39.594	35.530
5)	MB Aldrin	4.141	5.160	133.8E6	1425.0E6	39.701	35.483
6)	B beta-BHC	3.832	4.470	61790985	998.1E6	38.486	37.357m
7)	B delta-BHC	4.061	4.714	9381116	174.7E6	2.581	3.210
8)	B Heptachlo...	4.646	5.593	132.4E6	1328.9E6	42.614	39.313
9)	A Endosulfan I	5.015	5.977	123.0E6	1211.6E6	43.510	41.652
10)	B trans-Chl...	4.894	5.846	131.7E6	1243.3E6	42.715	39.357
11)	B cis-Chlor...	4.957	5.921	127.8E6	1235.0E6	40.813	38.901
12)	B 4,4'-DDE	5.145	6.096	252.8E6	2352.6E6	84.500	78.360
13)	MA Dieldrin	5.281	6.254	282.0E6	2631.1E6	92.038	87.288
14)	MA Endrin	5.557	6.486	243.2E6	2105.1E6	89.701	85.342
15)	B Endosulfa...	5.856	6.715	234.9E6	2090.7E6	87.221	86.543
16)	A 4,4'-DDD	5.704	6.620	207.8E6	1874.2E6	86.236	81.777
17)	MA 4,4'-DDT	5.952	6.928	197.4E6	1828.7E6	88.234	85.146
18)	B Endrin al...	6.037	6.846	168.3E6	1490.1E6	77.914	78.655
19)	B Endosulfa...	6.260	7.079	139.7E6	1185.3E6	55.689	57.000
20)	A Methoxychlor	6.535	7.406	558.9E6	4040.3E6	446.278	433.025
21)	B Endrin ke...	6.770	7.569	269.0E6	2019.2E6	92.144	90.435

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
Data File : PD073218.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 17:48
Operator : AR\AJ
Sample : N5683-03MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 01:09:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

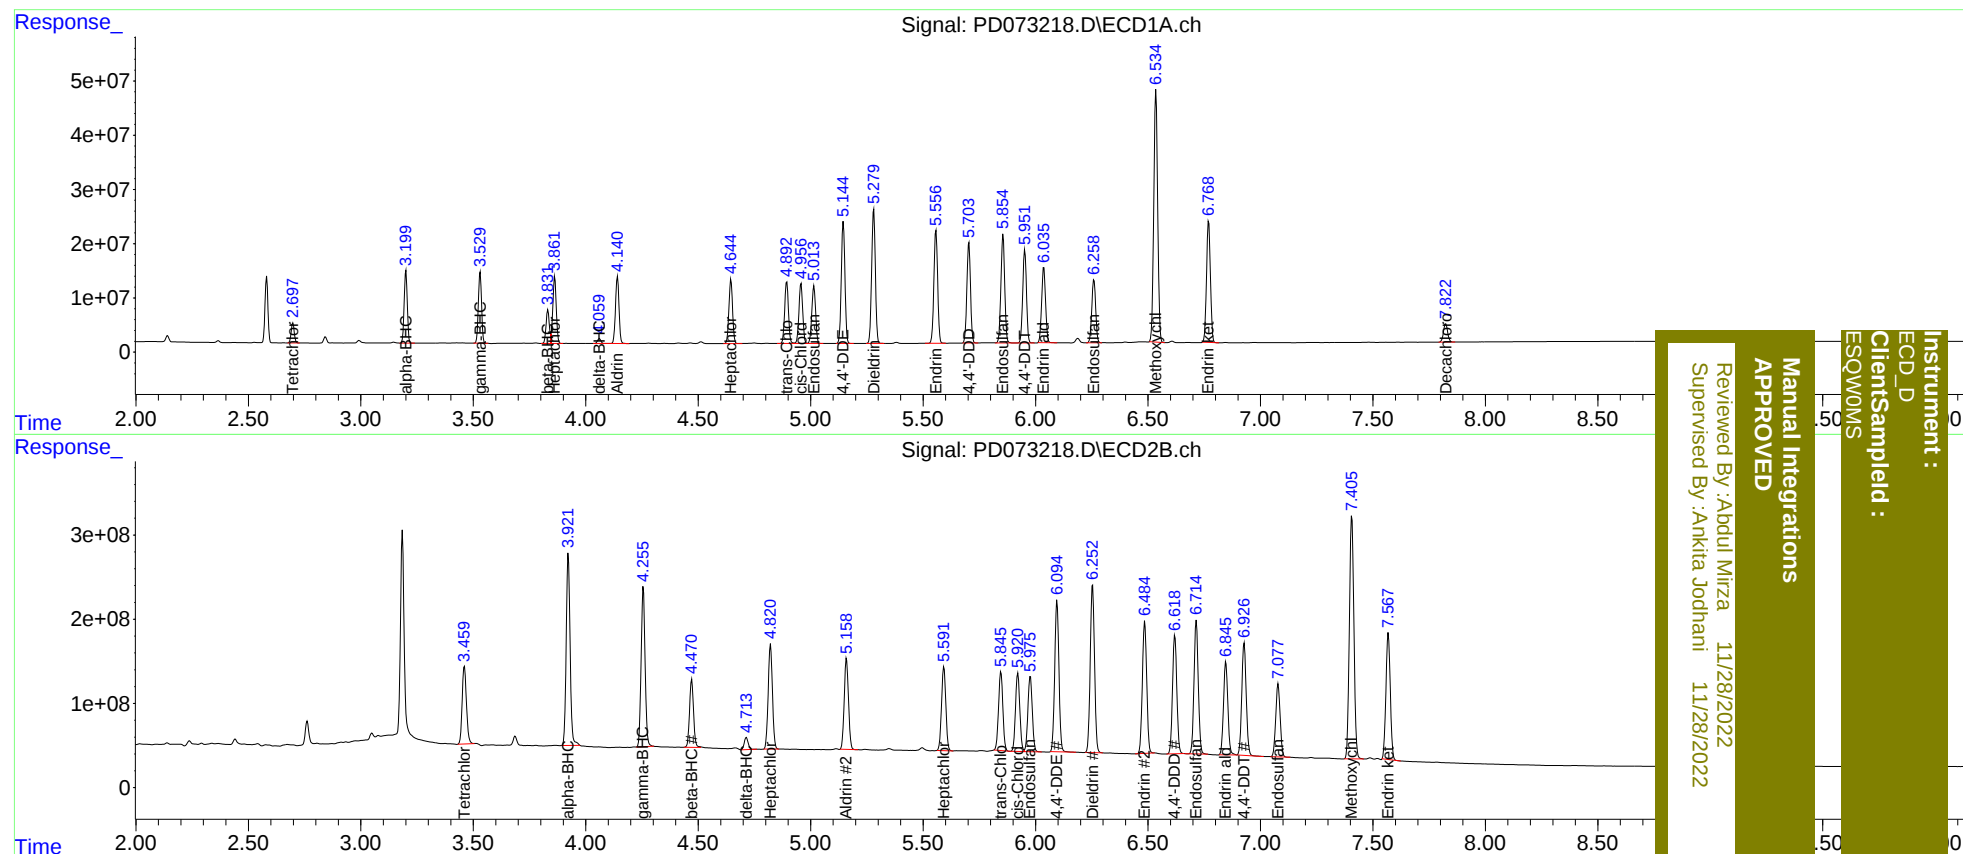

Reviewed By: Abdul Mirza 11/28/2022
Supervised By: Ankita Jodhani 11/28/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
ESQWOMS