

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
 Data File : PD073219.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 18:02
 Operator : AR\AJ
 Sample : N5683-04MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQW0MSD

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/25/2022
 Supervised By : Ankita Jodhani 11/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 01:10:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.461	36193756	1270.2E6	15.094	19.444 #
27)	SA Decachlor...	7.824	8.907	44156976	291.3E6	19.351	19.686
Target Compounds							
2)	A alpha-BHC	3.201	3.922	128.9E6	2795.0E6	35.230	32.051
3)	MA gamma-BHC...	3.531	4.256	131.4E6	2367.3E6	39.585	34.889
4)	MA Heptachlor	3.863	4.822	133.7E6	1645.1E6	40.007	35.824
5)	MB Aldrin	4.141	5.160	134.6E6	1436.8E6	39.945	35.776
6)	B beta-BHC	3.832	4.470	62413750	1000.1E6	38.874	37.432m
7)	B delta-BHC	4.061	4.715	9537862	175.2E6	2.624	3.220
8)	B Heptachlo...	4.646	5.592	132.8E6	1331.5E6	42.728	39.392
9)	A Endosulfan I	5.014	5.977	123.3E6	1214.3E6	43.647	41.745
10)	B trans-Chl...	4.894	5.846	131.7E6	1228.8E6	42.717	38.899
11)	B cis-Chlor...	4.958	5.921	128.0E6	1234.2E6	40.864	38.876
12)	B 4,4'-DDE	5.145	6.095	252.8E6	2362.2E6	84.507	78.680
13)	MA Dieldrin	5.280	6.254	281.7E6	2623.6E6	91.972	87.038
14)	MA Endrin	5.557	6.485	243.2E6	2118.7E6	89.695	85.891
15)	B Endosulfa...	5.855	6.715	234.9E6	2082.9E6	87.224	86.219
16)	A 4,4'-DDD	5.703	6.619	207.8E6	1871.8E6	86.250	81.672
17)	MA 4,4'-DDT	5.952	6.927	196.5E6	1814.6E6	87.828	84.493
18)	B Endrin al...	6.037	6.846	165.9E6	1482.7E6	76.826	78.264
19)	B Endosulfa...	6.259	7.078	140.3E6	1184.4E6	55.929	56.954
20)	A Methoxychlor	6.535	7.406	555.2E6	4020.9E6	443.273	430.945
21)	B Endrin ke...	6.770	7.568	269.2E6	2021.2E6	92.211	90.525

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
Data File : PD073219.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 18:02
Operator : AR\AJ
Sample : N5683-04MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 01:10:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

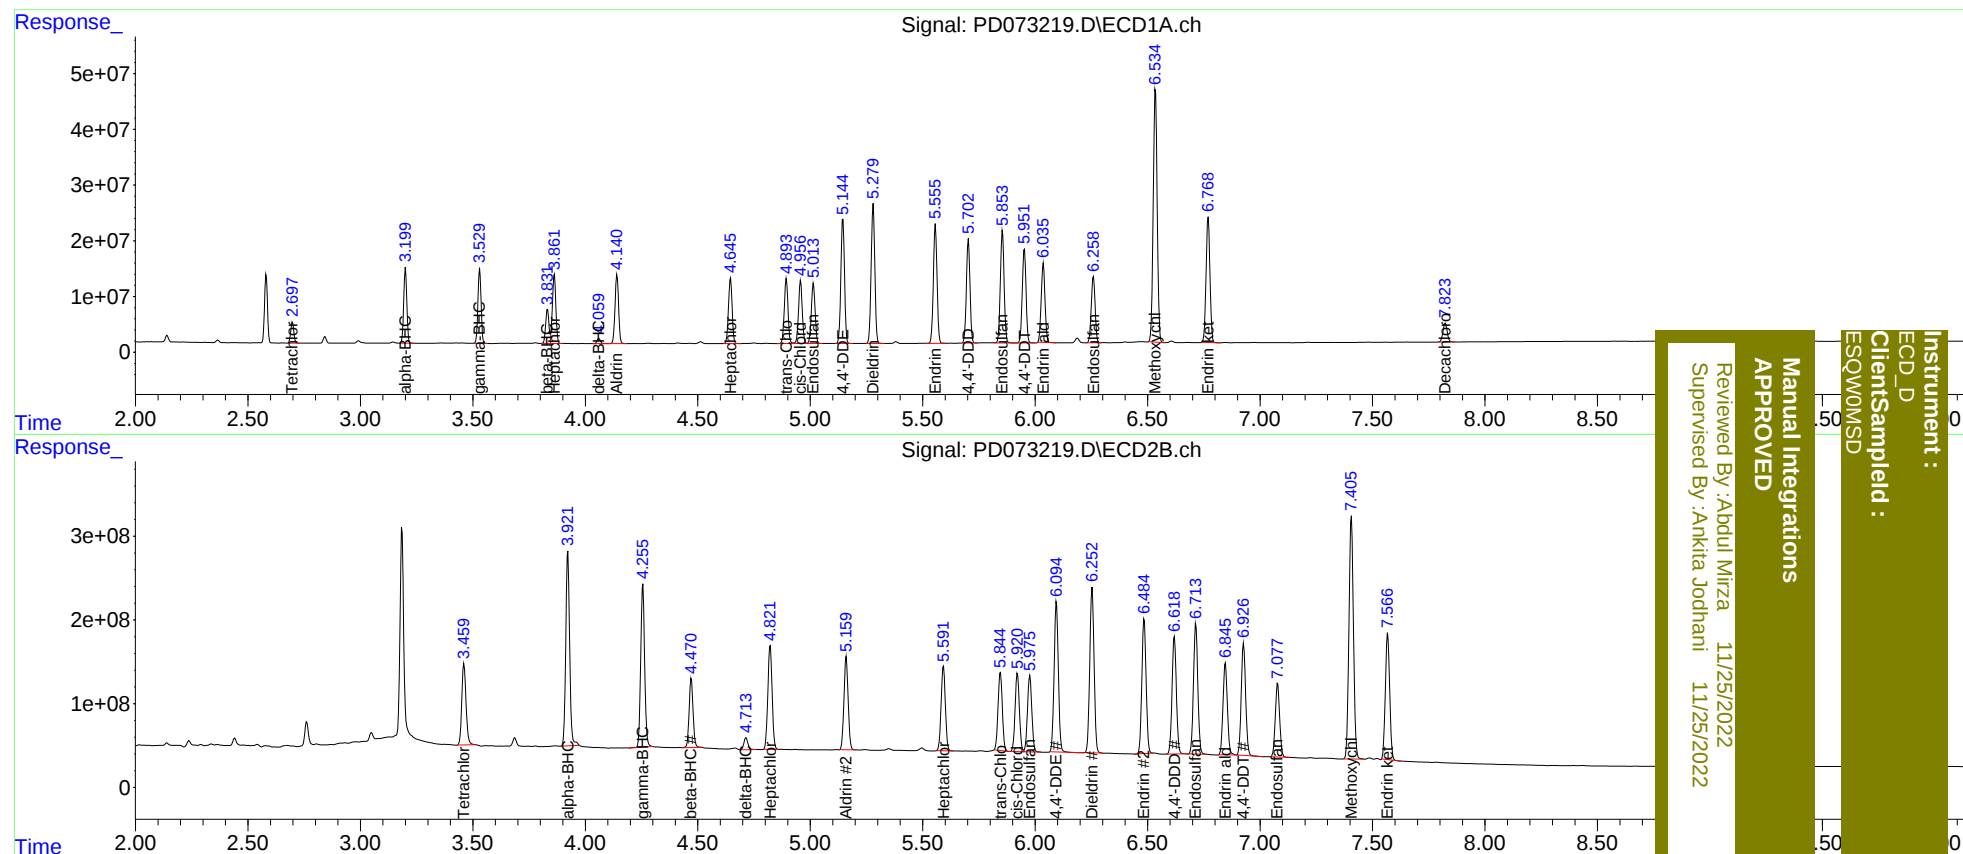

Reviewed By: Abdul Mirza 11/25/2022
Supervised By: Ankita Jodhani 11/25/2022

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
ESQW0MSD