

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
 Data File : PD073224.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 19:08
 Operator : AR\AJ
 Sample : PB149263BS
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS263

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/28/2022
 Supervised By : Ankita Jodhani 11/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 01:11:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	42939518	1175.6E6	17.907	17.996
27)	SA Decachlor...	7.824	8.908	87017753	566.6E6	38.134	38.289
Target Compounds							
2)	A alpha-BHC	3.200	3.922	13743774	381.4E6	3.755	4.373
3)	MA gamma-BHC...	3.530	4.255	13489608	325.4E6	4.065	4.796
4)	MA Heptachlor	3.862	4.821	13445931	212.0E6	4.025	4.617
5)	MB Aldrin	4.141	5.159	13883796	188.4E6	4.120	4.691
6)	B beta-BHC	3.832	4.469	6712856	117.4E6	4.181	4.394m
7)	B delta-BHC	4.061	4.714	13250642	242.5E6	3.646	4.456
8)	B Heptachlo...	4.645	5.592	13089341	156.2E6	4.213	4.622
9)	A Endosulfan I	5.014	5.976	12182274	134.3E6	4.311	4.616
10)	B trans-Chl...	4.893	5.845	12994773	141.0E6	4.216	4.464
11)	B cis-Chlor...	4.956	5.920	13092822	139.7E6	4.181	4.400
12)	B 4,4'-DDE	5.145	6.094	22491540	260.6E6	7.518	8.680
13)	MA Dieldrin	5.280	6.252	24692417	281.0E6	8.060	9.322
14)	MA Endrin	5.556	6.484	21042618	218.9E6	7.762	8.872
15)	B Endosulfa...	5.854	6.714	22374963	229.0E6	8.309	9.480
16)	A 4,4'-DDD	5.703	6.619	19600348	216.5E6	8.135	9.446
17)	MA 4,4'-DDT	5.951	6.927	17887521	192.7E6	7.996	8.974
18)	B Endrin al...	6.036	6.846	18554572	179.9E6	8.591	9.498
19)	B Endosulfa...	6.259	7.078	21102386	191.6E6	8.410	9.215
20)	A Methoxychlor	6.534	7.406	53858591	430.9E6	43.002	46.180
21)	B Endrin ke...	6.769	7.568	26296403	224.8E6	9.008	10.068

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
Data File : PD073224.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 19:08
Operator : AR\AJ
Sample : PB149263BS
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 01:11:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

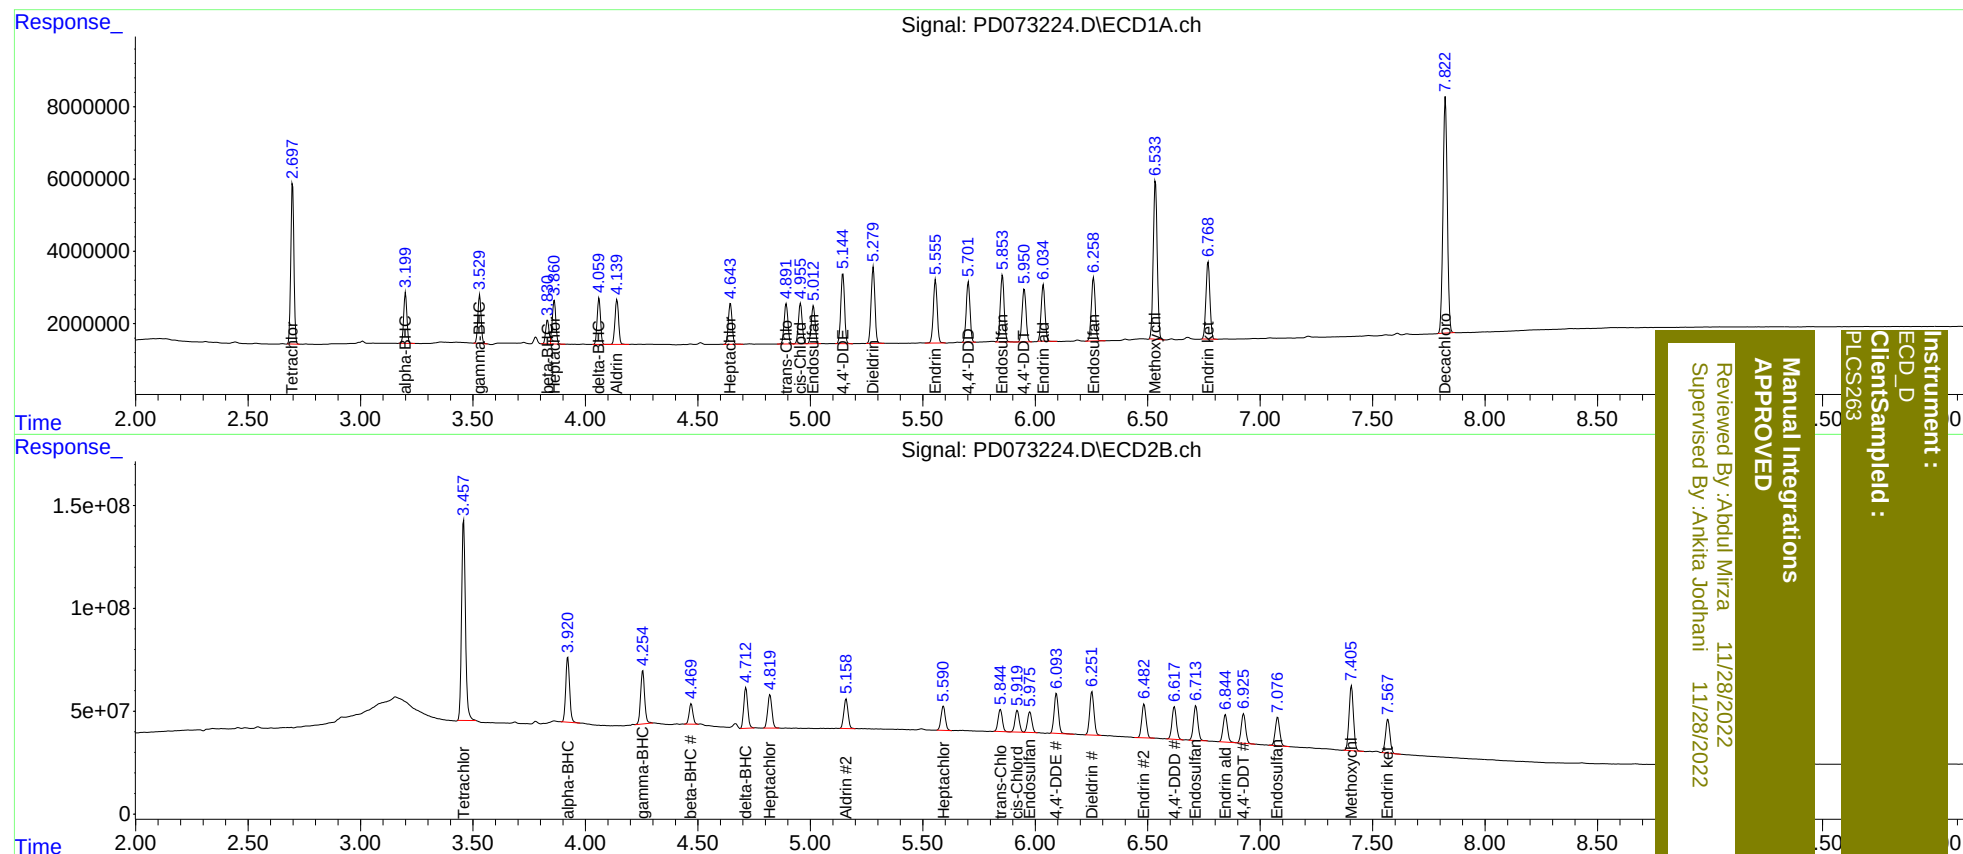

Instrument :
ECD_D
Client Sampled :
PLCS263

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/28/2022
Supervised By : Ankita Jodhani 11/28/2022