

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
 Data File : PD073227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Nov 2022 19:48
 Operator : AR\AJ
 Sample : N5659-04MS
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ESQT8MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/28/2022
 Supervised By :Ankita Jodhani 11/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 01:12:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 17 06:19:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	2.698	3.459	42706414	1090.6E6	17.810	16.695
27)	SA Decachlor...	7.824	8.908	74466130	487.5E6	32.634	32.939
Target Compounds							
2)	A alpha-BHC	3.201	3.923	185.0E6	3579.7E6	50.553	41.049
3)	MA gamma-BHC...	3.531	4.256	168.4E6	2813.6E6	50.751	41.466
4)	MA Heptachlor	3.862	4.822	163.1E6	1893.9E6	48.816	41.243
5)	MB Aldrin	4.141	5.161	172.2E6	1725.3E6	51.091	42.960
6)	B beta-BHC	3.832	4.470	64165779	1072.2E6	39.965	40.127m
7)	B delta-BHC	4.061	4.715	168.6E6	2130.8E6	46.376	39.162
8)	B Heptachlo...	4.645	5.592	144.5E6	1402.9E6	46.498	41.504
9)	A Endosulfan I	5.014	5.977	130.8E6	1297.8E6	46.272	44.613
10)	B trans-Chl...	4.894	5.846	150.6E6	1393.1E6	48.852	44.098
11)	B cis-Chlor...	4.957	5.921	145.9E6	1372.1E6	46.611	43.221
12)	B 4,4'-DDE	5.145	6.095	294.0E6	2677.6E6	98.272	89.185
13)	MA Dieldrin	5.280	6.253	339.6E6	3033.5E6	110.846	100.636
14)	MA Endrin	5.557	6.485	276.6E6	2347.6E6	102.015	95.171
15)	B Endosulfa...	5.855	6.715	258.3E6	2261.2E6	95.926	93.603
16)	A 4,4'-DDD	5.703	6.619	240.0E6	2147.9E6	99.631	93.721
17)	MA 4,4'-DDT	5.952	6.927	251.7E6	2208.9E6	112.522	102.851
18)	B Endrin al...	6.036	6.846	184.0E6	1607.1E6	85.174	84.832
19)	B Endosulfa...	6.259	7.079	236.7E6	1934.5E6	94.331	93.026
20)	A Methoxychlor	6.534	7.407	634.1E6	4546.9E6	506.241	487.319
21)	B Endrin ke...	6.769	7.568	289.7E6	2168.4E6	99.234	97.116

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112422\
Data File : PD073227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Nov 2022 19:48
Operator : AR\AJ
Sample : N5659-04MS
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 01:12:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD111722CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 17 06:19:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

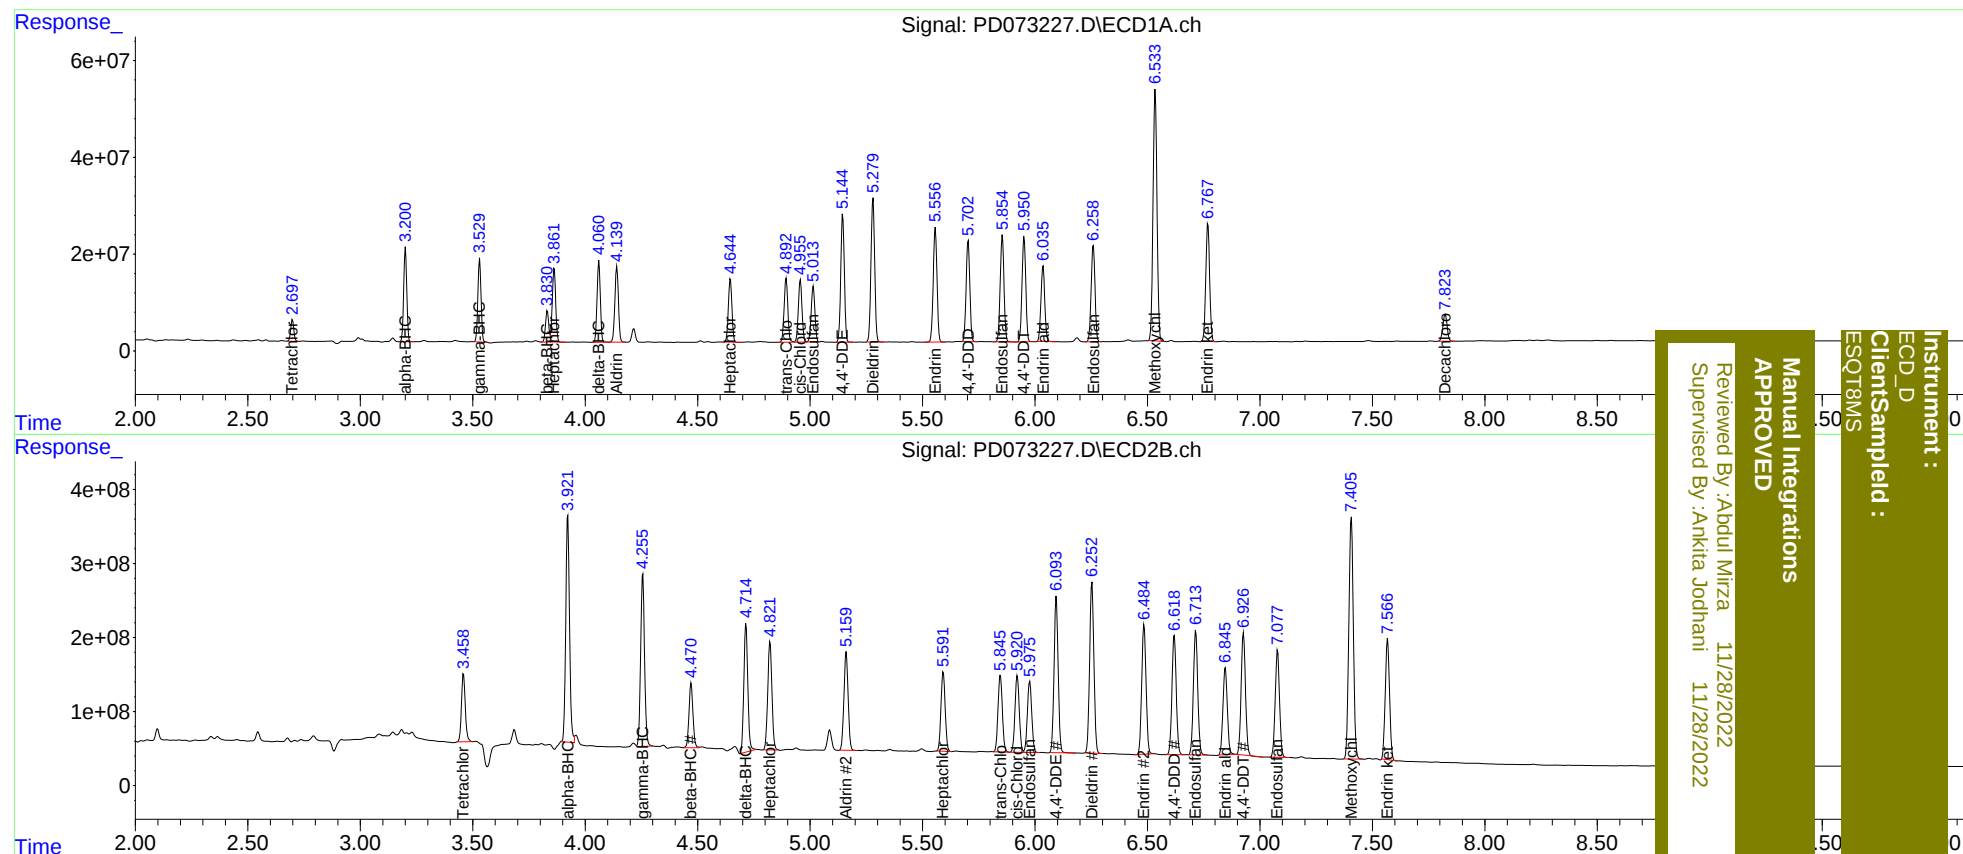

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 11/28/2022
Supervised By: Ankita Jodhani 11/28/2022

Instrument :
ECD_D
Client Sampled :
ESQ18MS