

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060282.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 09:16
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 26 01:30:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Nov 26 01:04:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
27)	SA Decachlor...	8.305	0.000	650846	0	0.496	N.D. #
Target Compounds							
6)	B beta-BHC	0.000	4.820f	0	2411885	N.D.	1.152
9)	A Endosulfan I	0.000	6.215f	0	483194	N.D.	0.127
10)	B trans-Chl...	0.000	6.092f	0	78152005	N.D.	18.753
11)	B cis-Chlor...	0.000	6.215	0	483194	N.D.	0.118
15)	B Endosulfa...	6.403f	6.908f	563836	2361561	0.450	0.733 #
16)	A 4,4'-DDD	0.000	6.815f	0	1373458	N.D.	0.423
17)	MA 4,4'-DDT	6.403f	0.000	563836	0	0.432	N.D. #
23)	Toxaphene-2	5.917	0.000	848011	0	66.827	N.D. #
24)	Toxaphene-3	6.300	0.000	5128191	0	340.892	N.D. #
25)	Toxaphene-4	6.403	0.000	563836	0	16.527	N.D. #
26)	Toxaphene-5	7.157	0.000	7511377	0	206.476	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060282.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 09:16
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 26 01:30:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Thu Nov 26 01:04:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

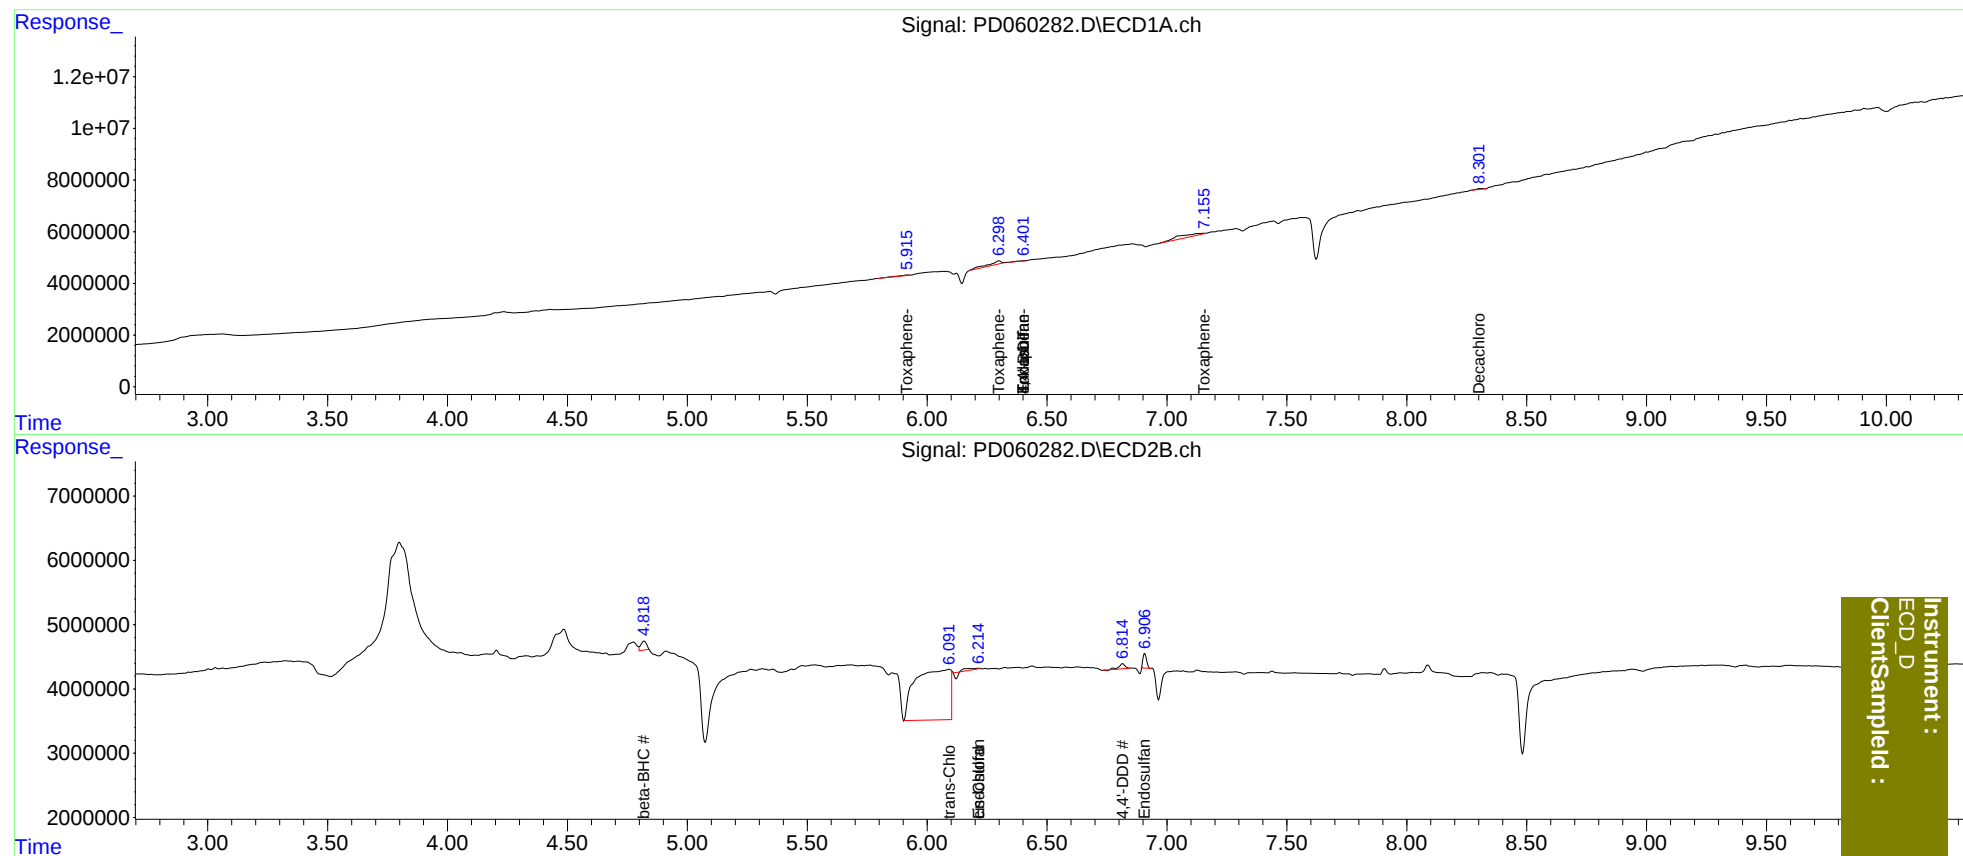


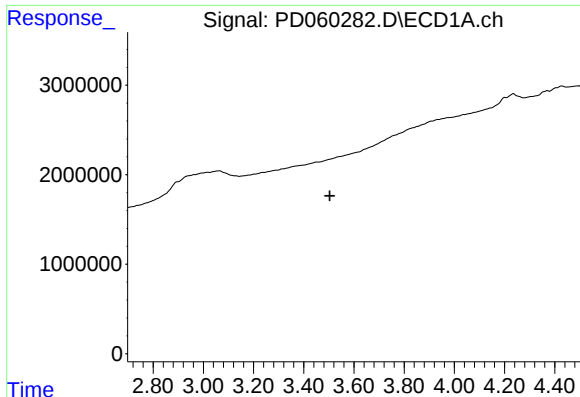

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

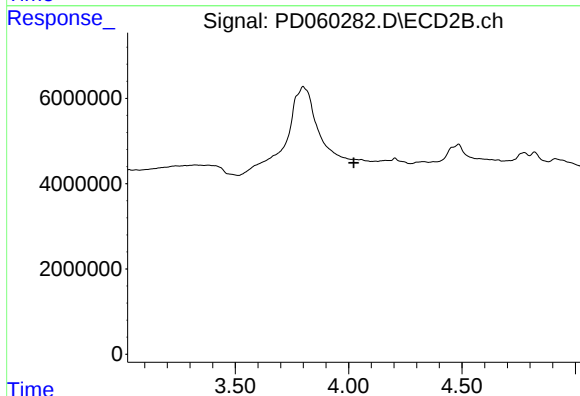


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.023 min
Response: 0
Conc: N.D.

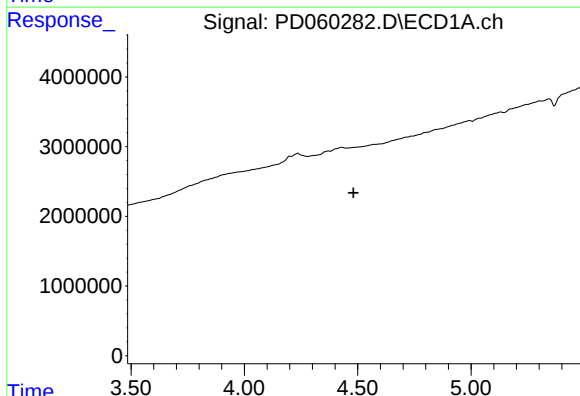


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.482 min
Response: 0
Conc: N.D.

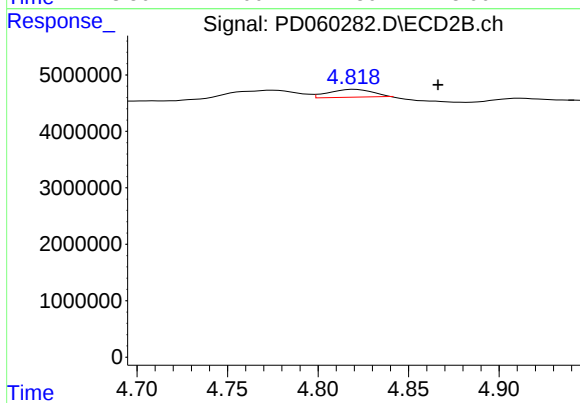

#6 beta-BHC


R.T.: 4.820 min
Delta R.T.: -0.046 min
Response: 2411885
Conc: 1.15 ng/ml

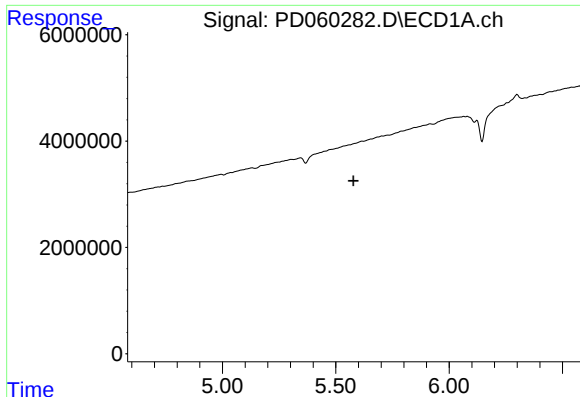

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.578 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

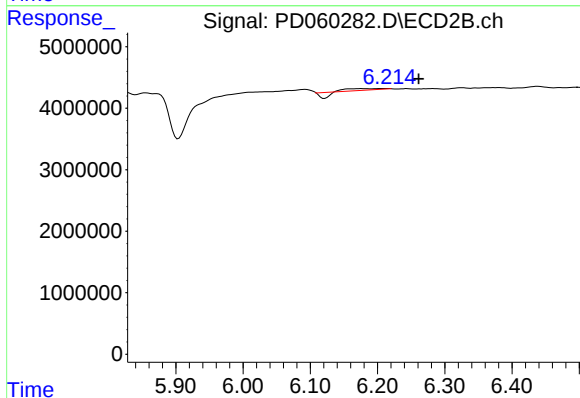


#9 Endosulfan I

R.T.: 6.215 min
Delta R.T.: -0.046 min
Response: 483194
Conc: 0.13 ng/ml

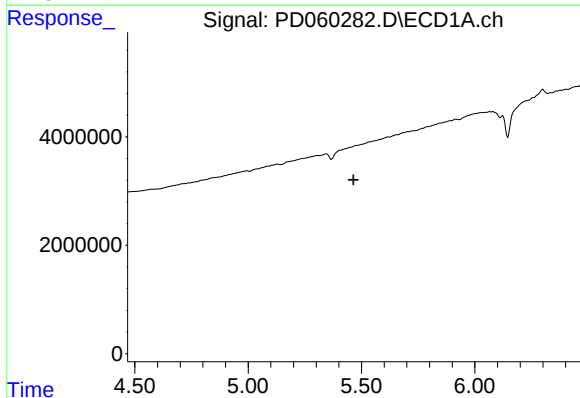


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.465 min
Response: 0
Conc: N.D.

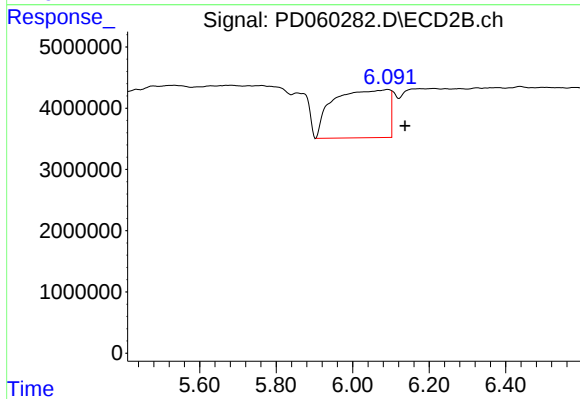

#10 trans-Chlordane


R.T.: 6.092 min
Delta R.T.: -0.045 min
Response: 78152005
Conc: 18.75 ng/ml

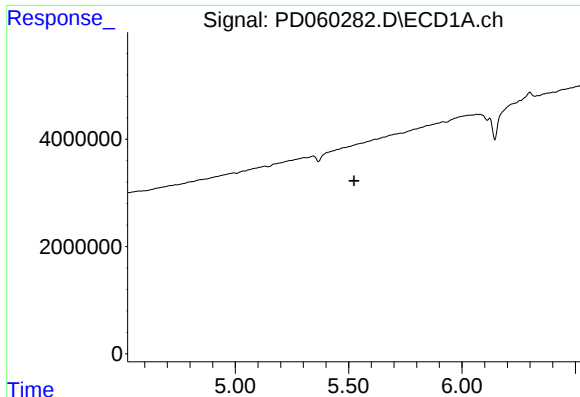

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

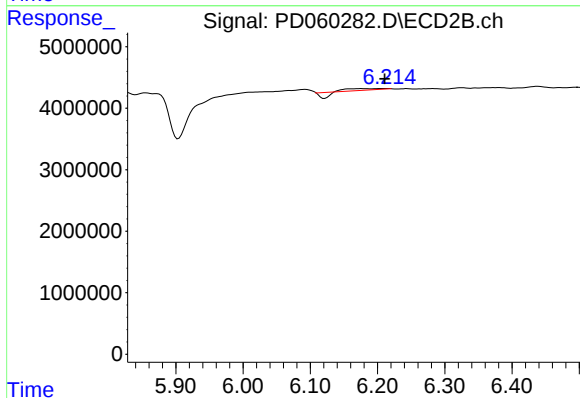


#11 cis-Chlordane

R.T.: 6.215 min
Delta R.T.: 0.004 min
Response: 483194
Conc: 0.12 ng/ml

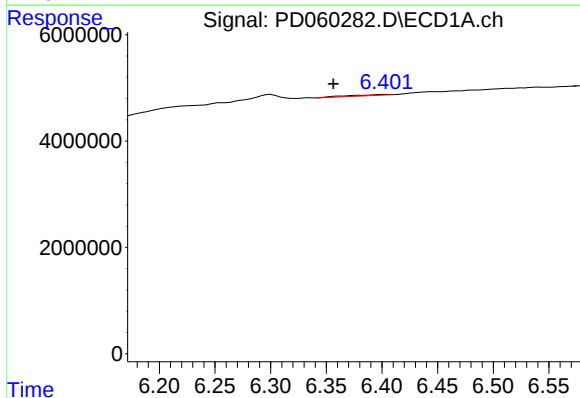


#15 Endosulfan II

R.T.: 6.403 min
Delta R.T.: 0.047 min
Response: 563836
Conc: 0.45 ng/ml

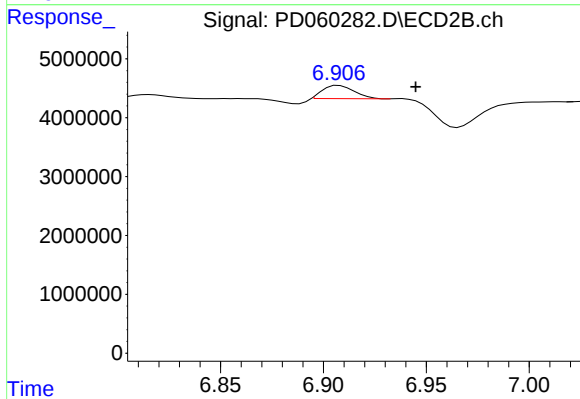

#15 Endosulfan II


R.T.: 6.908 min
Delta R.T.: -0.037 min
Response: 2361561
Conc: 0.73 ng/ml

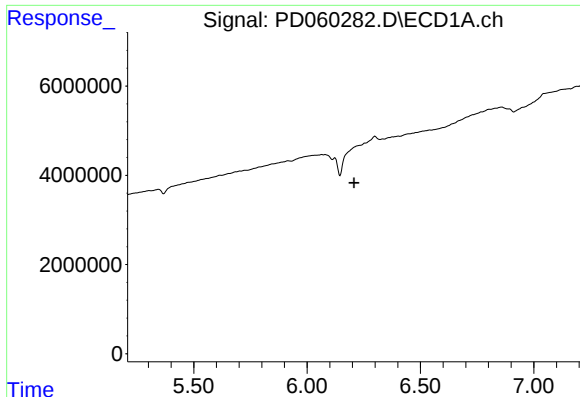

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

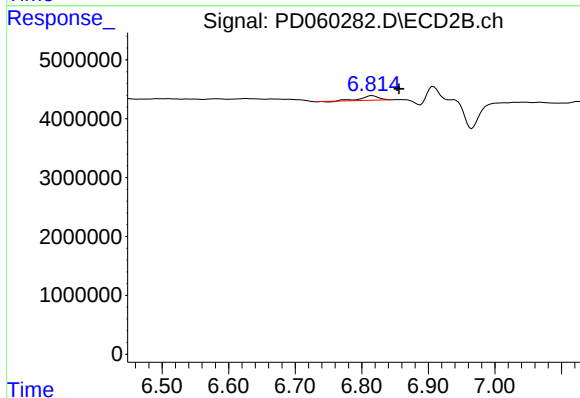


#16 4,4'-DDD

R.T.: 6.815 min
Delta R.T.: -0.041 min
Response: 1373458
Conc: 0.42 ng/ml

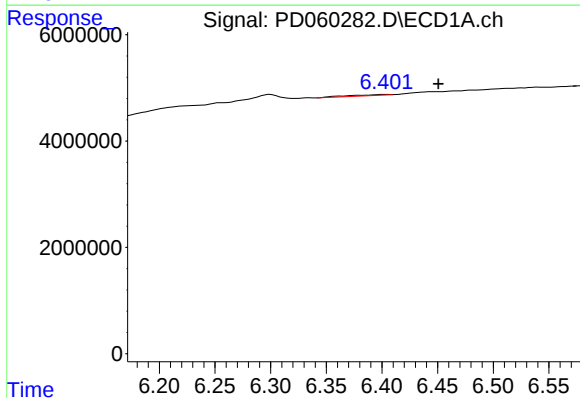


#17 4,4'-DDT

R.T.: 6.403 min
Delta R.T.: -0.048 min
Response: 563836
Conc: 0.43 ng/ml

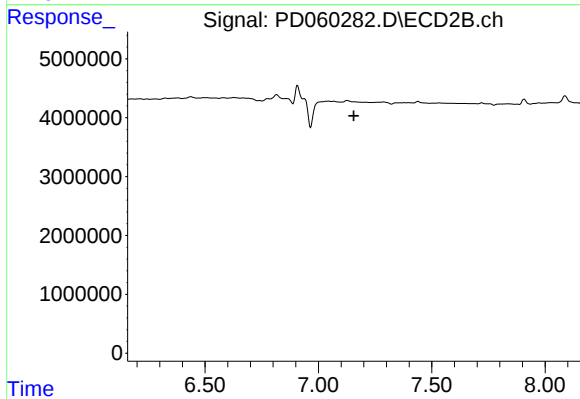

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.156 min
Response: 0
Conc: N.D.

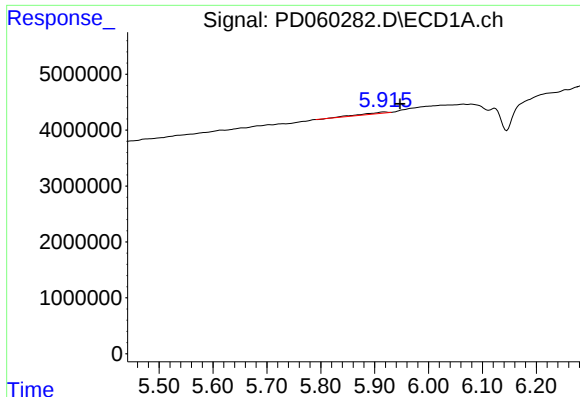

#23 Toxaphene-2


R.T.: 5.917 min
Delta R.T.: -0.030 min
Response: 848011
Conc: 66.83 ng/ml

Instrument :
ECD_D
ClientSampleId :

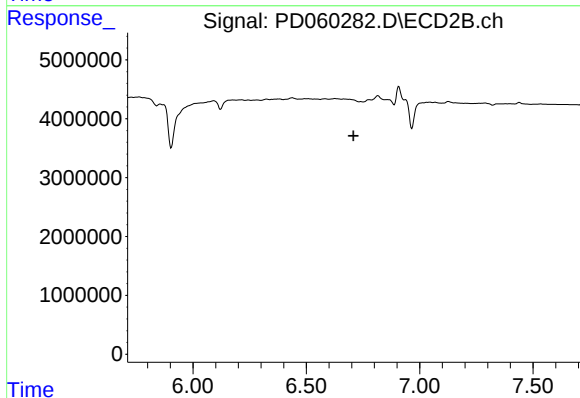


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 6.708 min
Response: 0
Conc: N.D.

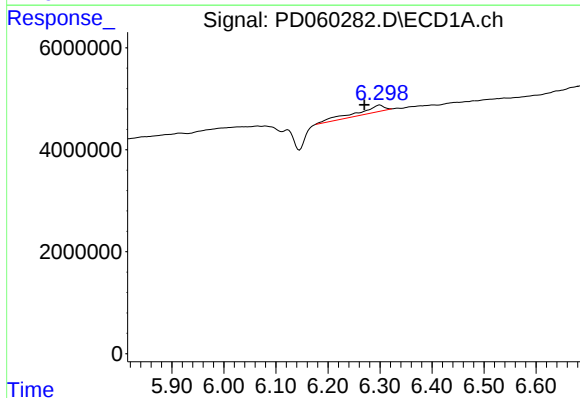


#24 Toxaphene-3

R.T.: 6.300 min
Delta R.T.: 0.030 min
Response: 5128191
Conc: 340.89 ng/ml

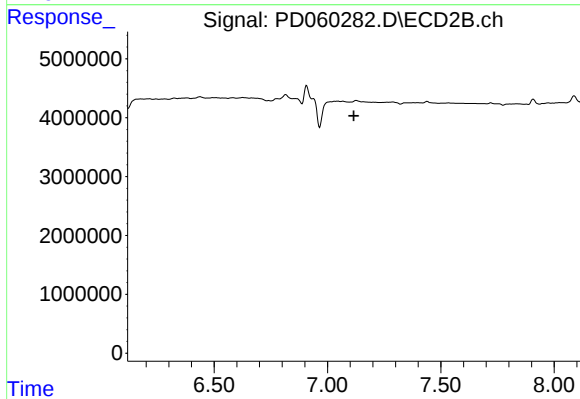

#24 Toxaphene-3


R.T.: 0.000 min
Exp R.T. : 7.116 min
Response: 0
Conc: N.D.

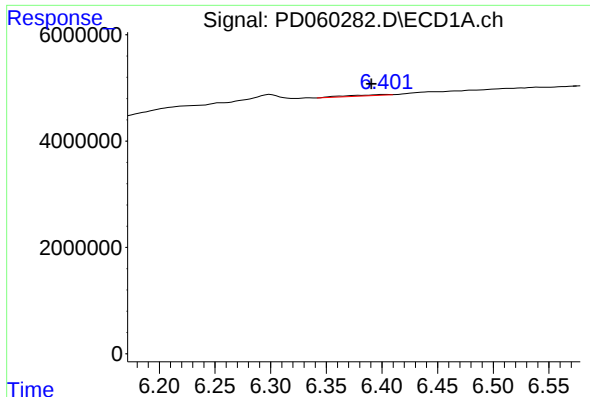

#25 Toxaphene-4


R.T.: 6.403 min
Delta R.T.: 0.012 min
Response: 563836
Conc: 16.53 ng/ml

Instrument :
ECD_D
ClientSampleId :

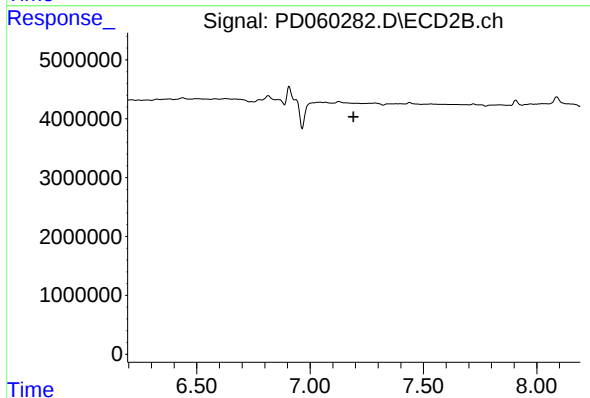


#25 Toxaphene-4

R.T.: 0.000 min
Exp R.T. : 7.192 min
Response: 0
Conc: N.D.

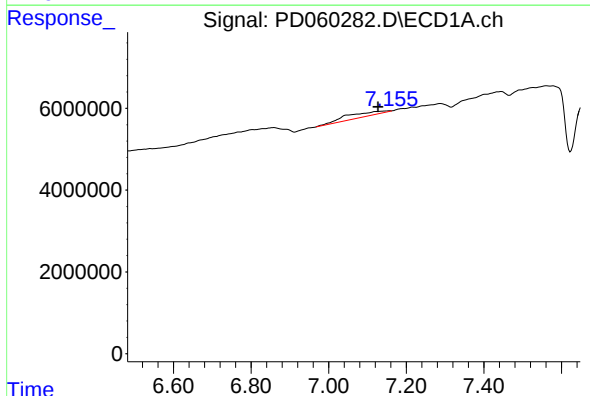


#26 Toxaphene-5

R.T.: 7.157 min
Delta R.T.: 0.030 min
Response: 7511377
Conc: 206.48 ng/ml

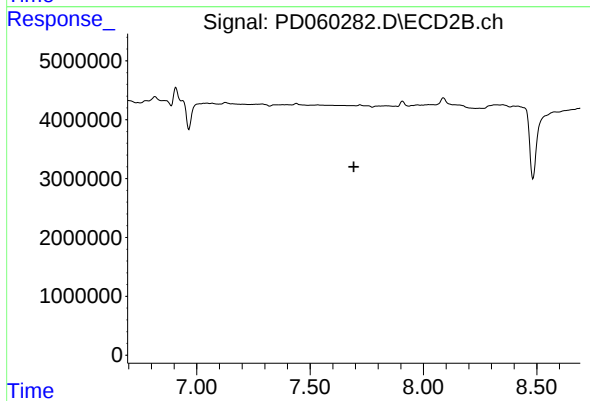

#26 Toxaphene-5


R.T.: 0.000 min
Exp R.T. : 7.692 min
Response: 0
Conc: N.D.

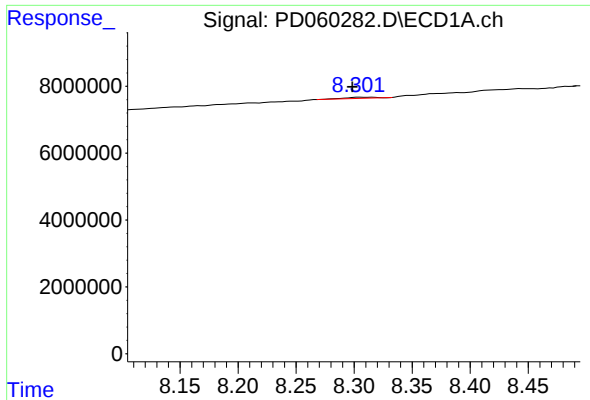

#27 Decachlorobiphenyl

R.T.: 8.305 min
Delta R.T.: 0.006 min
Response: 650846
Conc: 0.50 ng/ml

Instrument :
ECD_D
ClientSampleId :

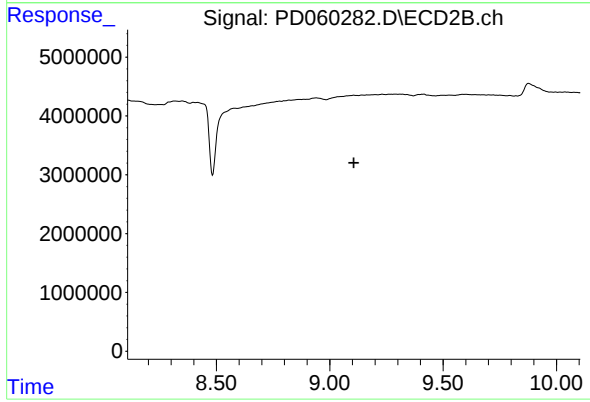

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.107 min
Response: 0
Conc: N.D.