

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060290.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 11:09
 Operator : DD\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 12:48:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 25 12:47:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.503	4.023	5579973	18453804	4.983	5.048
27)	SA Decachlor...	8.297	9.106	13280446	29846318	9.845	10.561
Target Compounds							
2)	A alpha-BHC	3.944	4.413	8715509	26743445	5.005	4.947
3)	MA gamma-BHC...	4.231	4.699	8289870	23749010	5.052	4.805
4)	MA Heptachlor	4.537	5.210	8022027	23528784	4.973	4.922
9)	A Endosulfan I	5.578	6.261	7339274	19075718	5.138	4.961
13)	MA Dieldrin	5.823	6.519	16475234	41119899	10.145	9.753
14)	MA Endrin	6.082	6.737	14167892	34535196	10.359	9.790
16)	A 4,4'-DDD	6.207	6.856	13442298	31918315	10.182	9.695
17)	MA 4,4'-DDT	6.450	7.156	12851218	32348833	9.630	9.655
20)	A Methoxychlor	6.998	7.612	33014008	89667877	52.004	52.680


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060290.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 11:09
Operator : DD\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 12:48:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 25 12:47:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

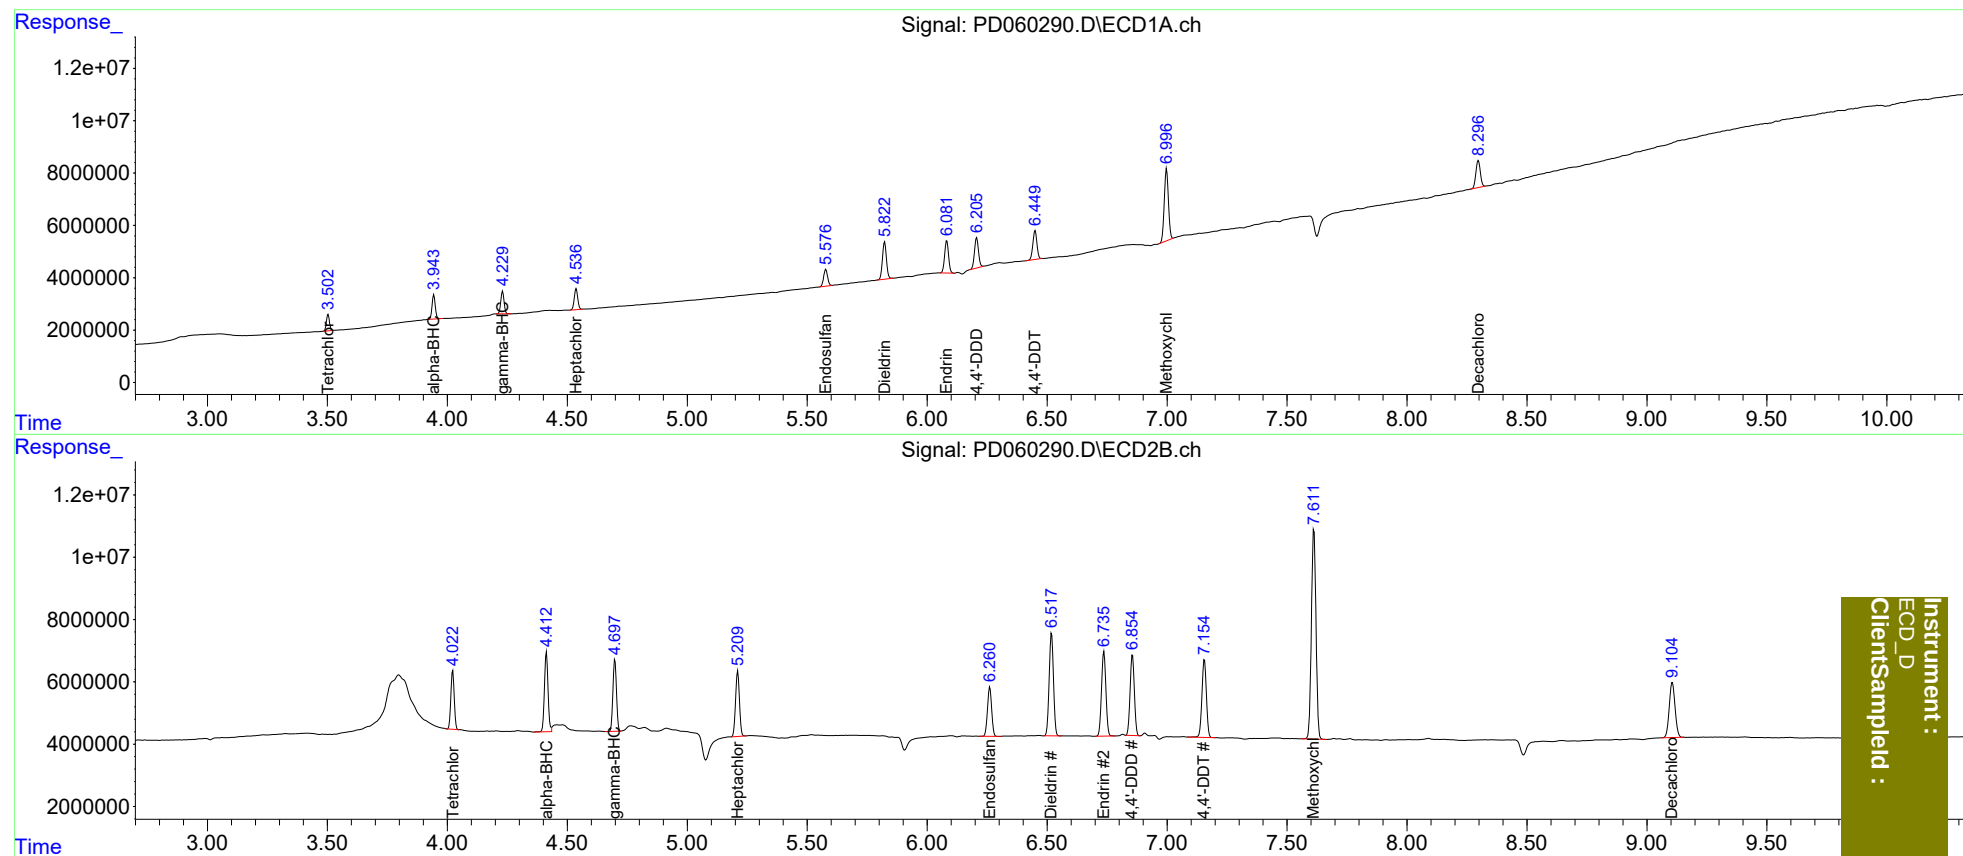


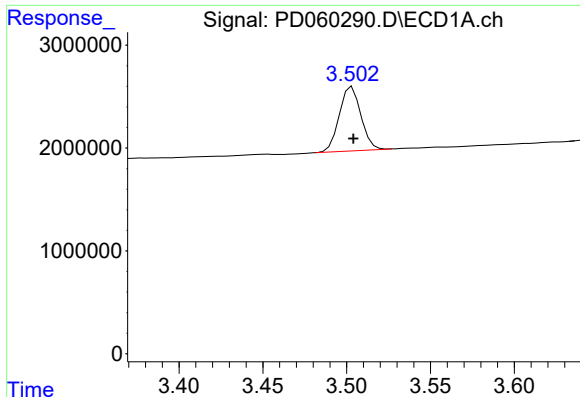

#1 Tetrachloro-m-xylene


R.T.: 3.503 min
Delta R.T.: 0.000 min
Response: 5579973
Conc: 4.98 ng/ml

Instrument :
ECD_D
ClientSampleId :

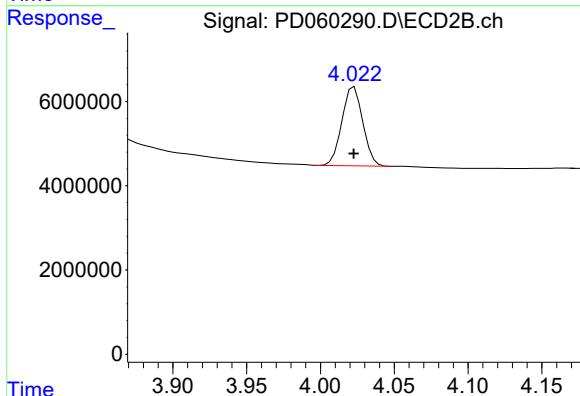


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 18453804
Conc: 5.05 ng/ml

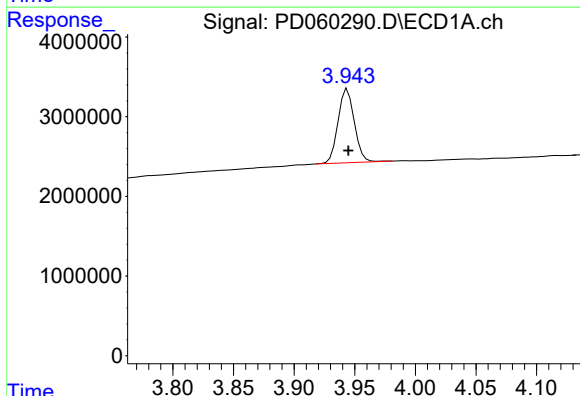


#2 alpha-BHC

R.T.: 3.944 min
Delta R.T.: 0.000 min
Response: 8715509
Conc: 5.01 ng/ml

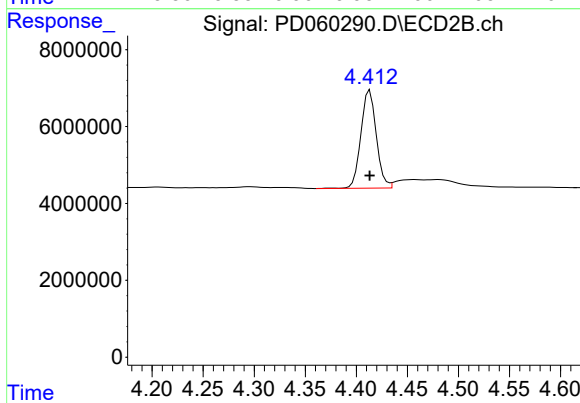

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 26743445
Conc: 4.95 ng/ml

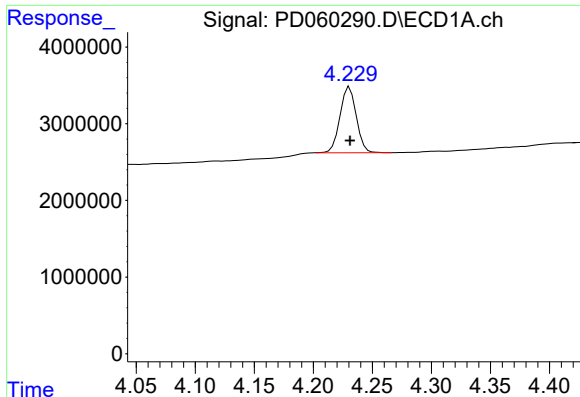

#3 gamma-BHC (Lindane)


R.T.: 4.231 min
Delta R.T.: 0.000 min
Response: 8289870
Conc: 5.05 ng/ml

Instrument :
ECD_D
ClientSampleId :

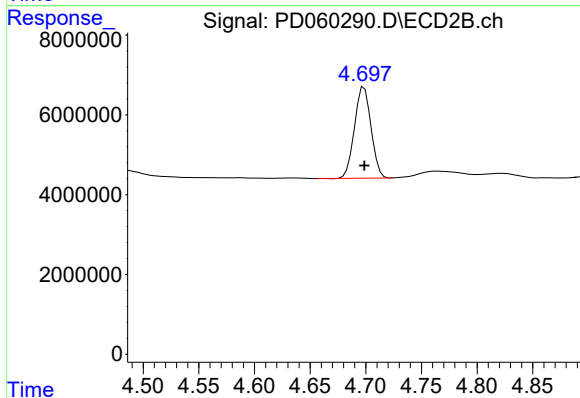


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 23749010
Conc: 4.81 ng/ml

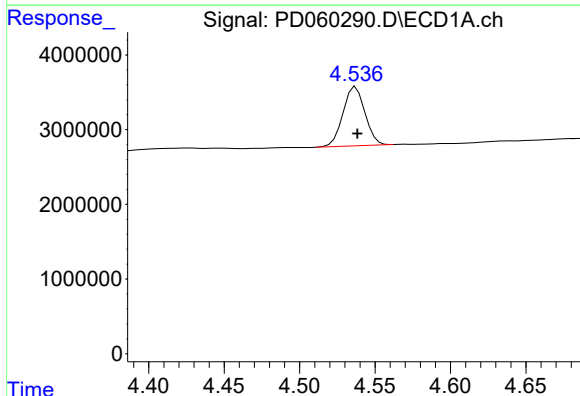


#4 Heptachlor

R.T.: 4.537 min
Delta R.T.: 0.000 min
Response: 8022027
Conc: 4.97 ng/ml

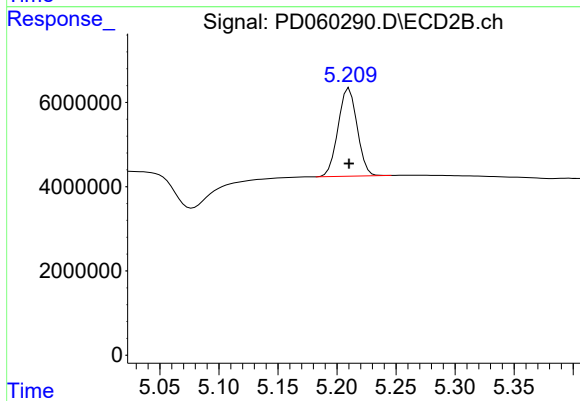

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 23528784
Conc: 4.92 ng/ml

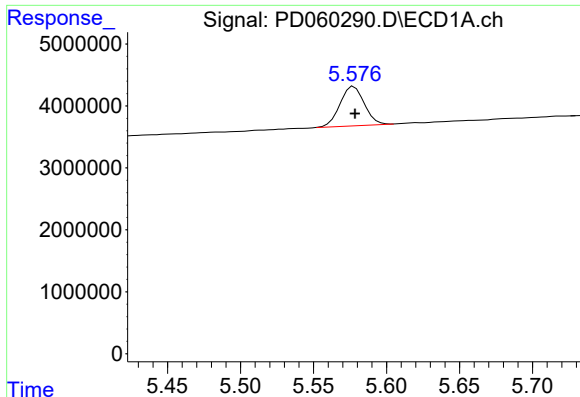

#9 Endosulfan I


R.T.: 5.578 min
Delta R.T.: 0.000 min
Response: 7339274
Conc: 5.14 ng/ml

Instrument :
ECD_D
ClientSampleId :

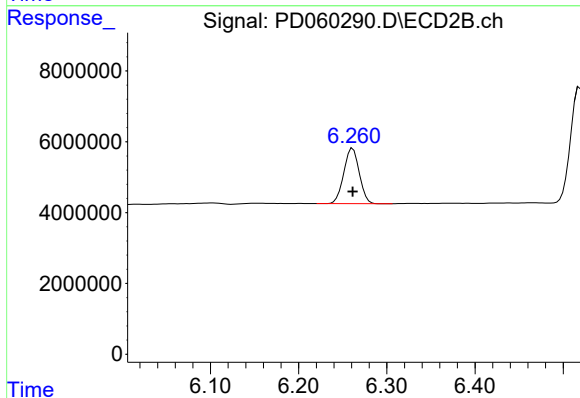


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 19075718
Conc: 4.96 ng/ml

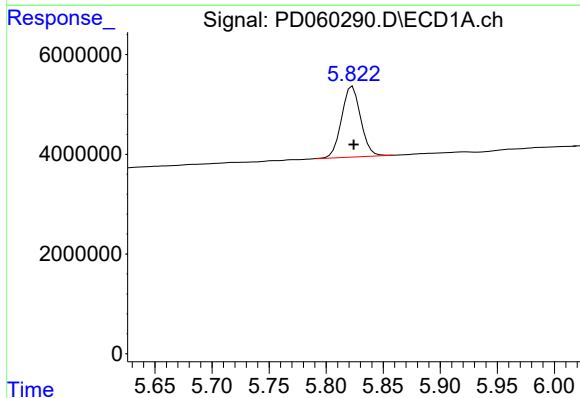


#13 Dieldrin

R.T.: 5.823 min
Delta R.T.: -0.001 min
Response: 16475234
Conc: 10.14 ng/ml

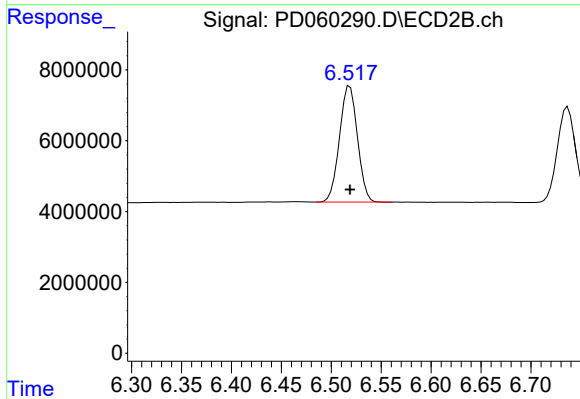

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 41119899
Conc: 9.75 ng/ml

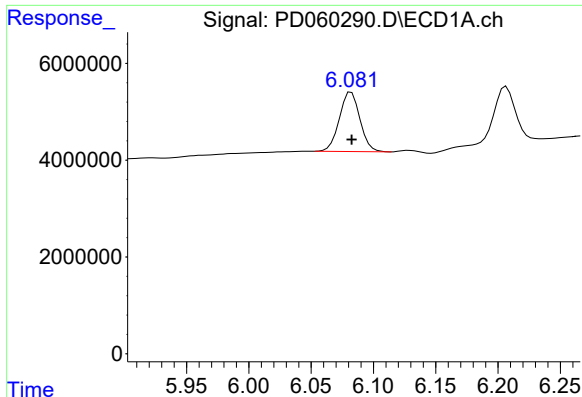

#14 Endrin


R.T.: 6.082 min
Delta R.T.: 0.000 min
Response: 14167892
Conc: 10.36 ng/ml

Instrument :
ECD_D
ClientSampleId :

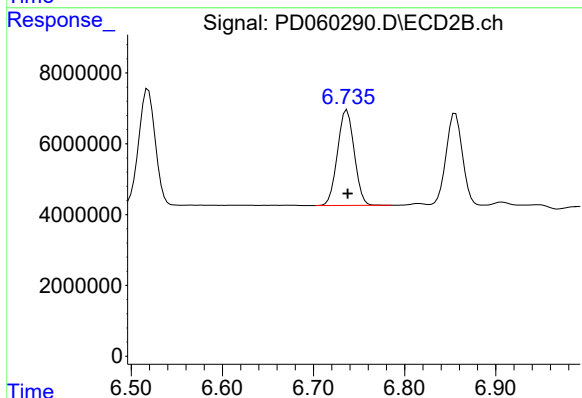


#14 Endrin

R.T.: 6.737 min
Delta R.T.: 0.000 min
Response: 34535196
Conc: 9.79 ng/ml

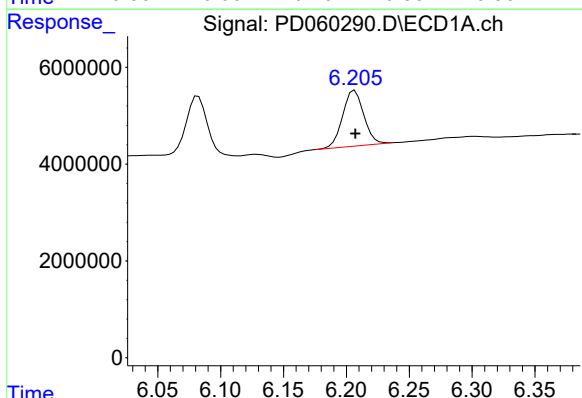


#16 4,4'-DDD

R.T.: 6.207 min
Delta R.T.: 0.000 min
Response: 13442298
Conc: 10.18 ng/ml

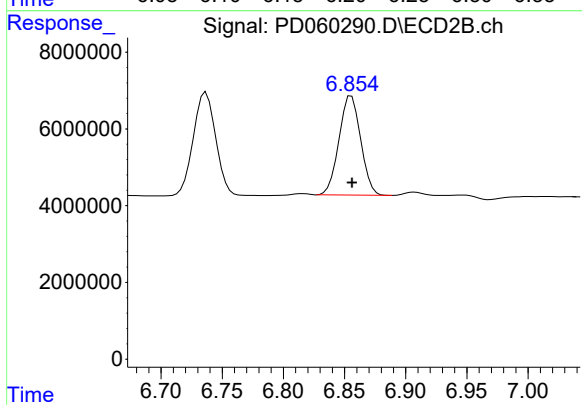

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 31918315
Conc: 9.70 ng/ml

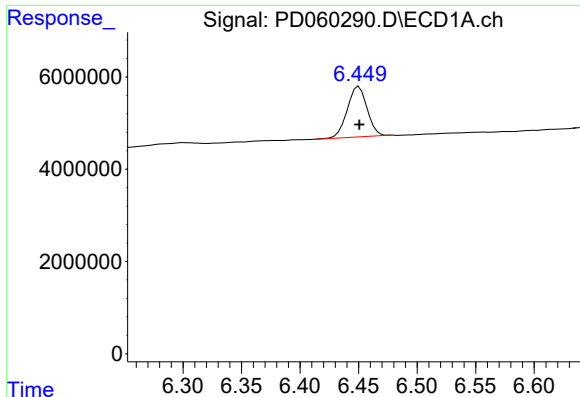

#17 4,4'-DDT


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 12851218
Conc: 9.63 ng/ml

Instrument :
ECD_D
ClientSampleId :

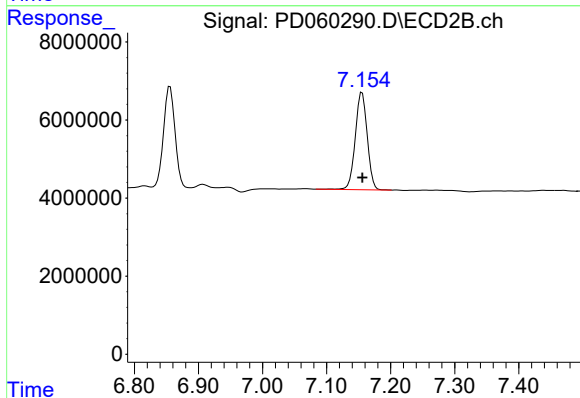


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 32348833
Conc: 9.66 ng/ml

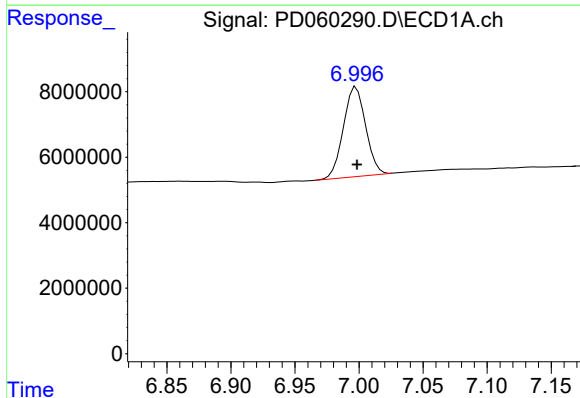


#20 Methoxychlor

R.T.: 6.998 min
Delta R.T.: 0.000 min
Response: 33014008
Conc: 52.00 ng/ml

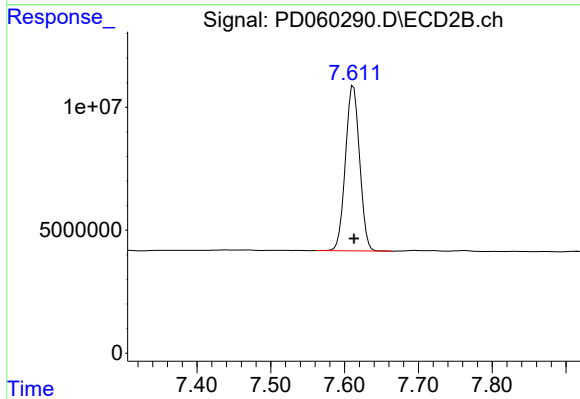

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: -0.001 min
Response: 89667877
Conc: 52.68 ng/ml

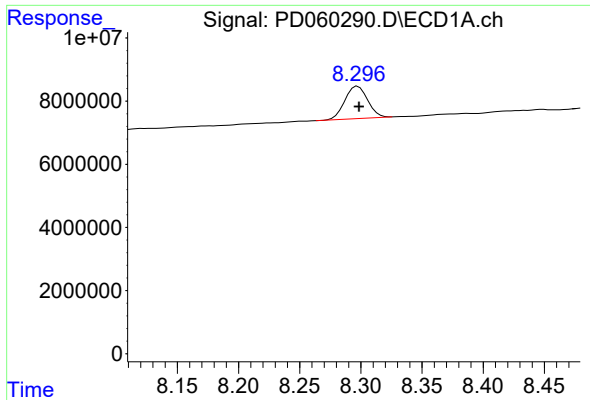

#27 Decachlorobiphenyl

R.T.: 8.297 min
Delta R.T.: -0.001 min
Response: 13280446
Conc: 9.85 ng/ml

Instrument :
ECD_D
ClientSampleId :

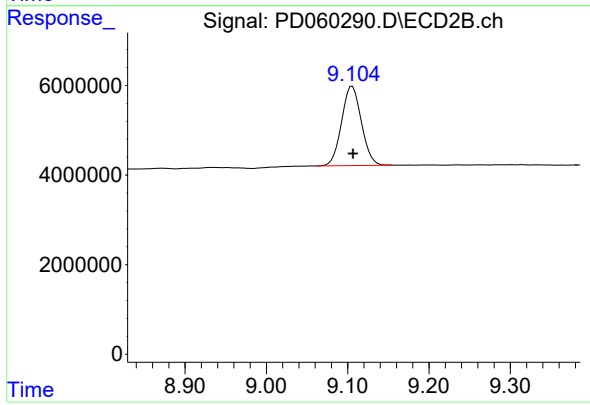

#27 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: -0.001 min
Response: 29846318
Conc: 10.56 ng/ml