

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 12:04
 Operator : DD\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 12:47:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 25 12:47:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.023	22397476	73110432	20.000	20.000
27)	SA Decachlor...	8.299	9.107	53956511	113.0E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.945	4.413	34824562	108.1E6	20.000	20.000
3)	MA gamma-BHC...	4.231	4.699	32816885	98841338	20.000	20.000
4)	MA Heptachlor	4.538	5.210	32265337	95598438	20.000	20.000
9)	A Endosulfan I	5.578	6.261	28571349	76904875	20.000	20.000
13)	MA Dieldrin	5.824	6.519	64961714	168.6E6	40.000	40.000
14)	MA Endrin	6.083	6.737	54709628	141.1E6	40.000	40.000
16)	A 4,4'-DDD	6.207	6.856	52807971	131.7E6	40.000	40.000
17)	MA 4,4'-DDT	6.451	7.156	53382416	134.0E6	40.000	40.000
20)	A Methoxychlor	6.999	7.613	127.0E6	340.4E6	200.000	200.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 12:04
Operator : DD\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 12:47:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 25 12:47:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

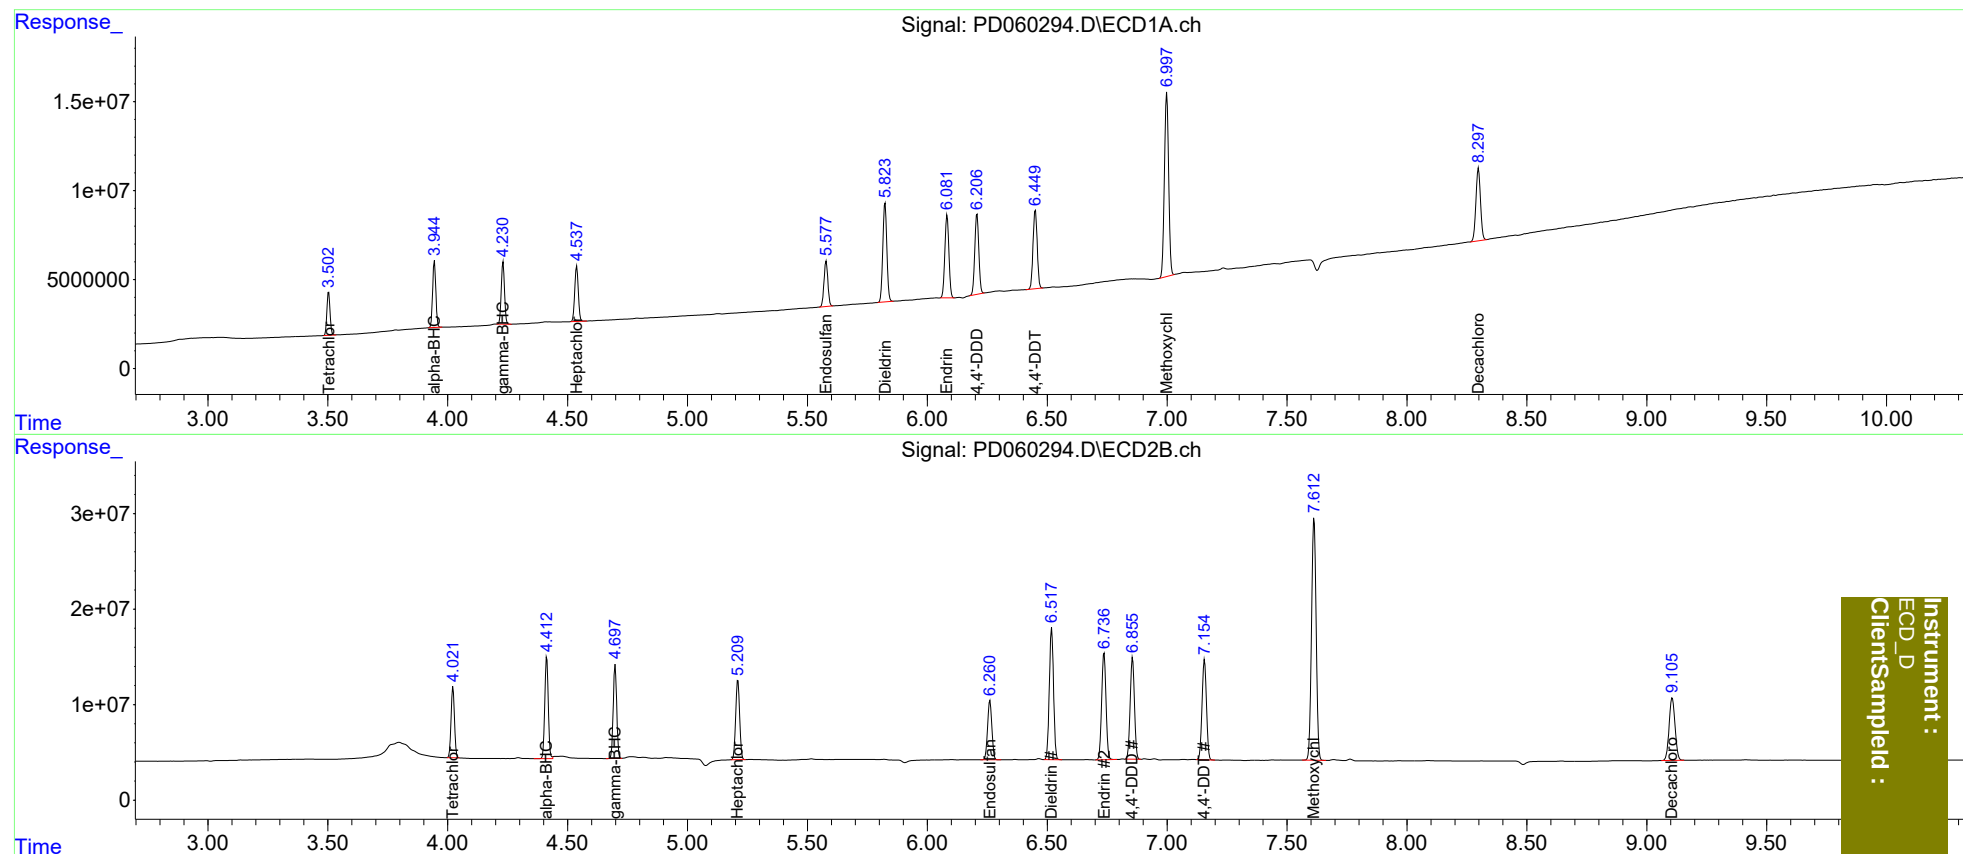


Instrument :
ECD_D
ClientSampled :

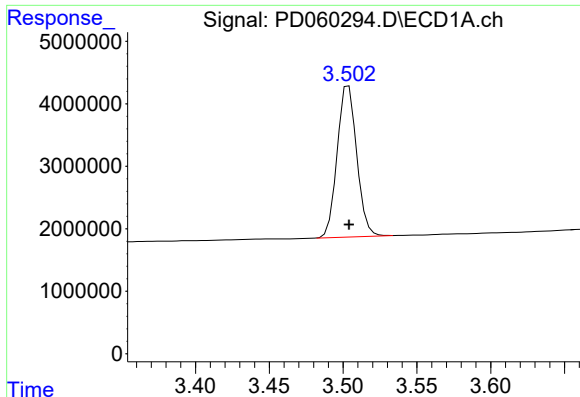

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 22397476
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

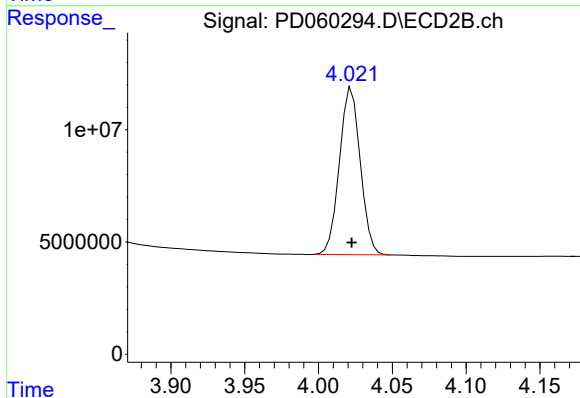


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 73110432
Conc: 20.00 ng/ml

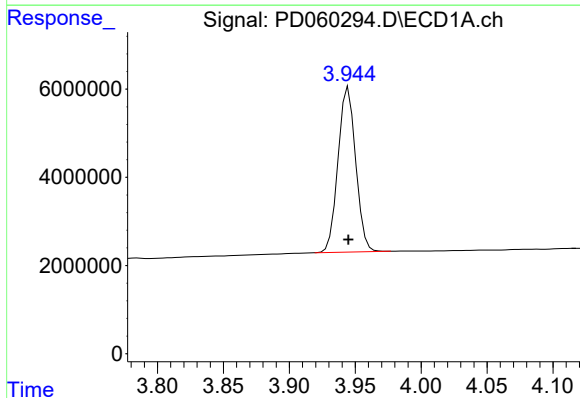


#2 alpha-BHC

R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 34824562
Conc: 20.00 ng/ml

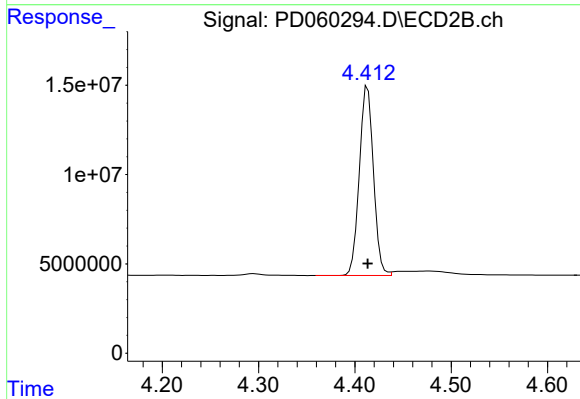

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 108113449
Conc: 20.00 ng/ml

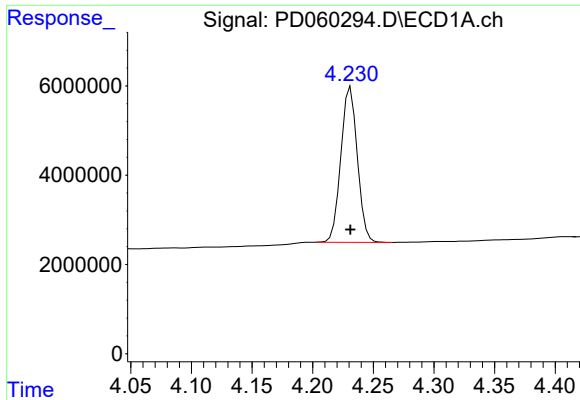

#3 gamma-BHC (Lindane)


R.T.: 4.231 min
Delta R.T.: 0.000 min
Response: 32816885
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

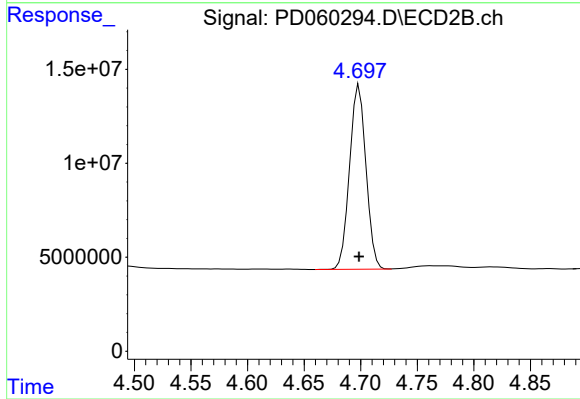


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 98841338
Conc: 20.00 ng/ml

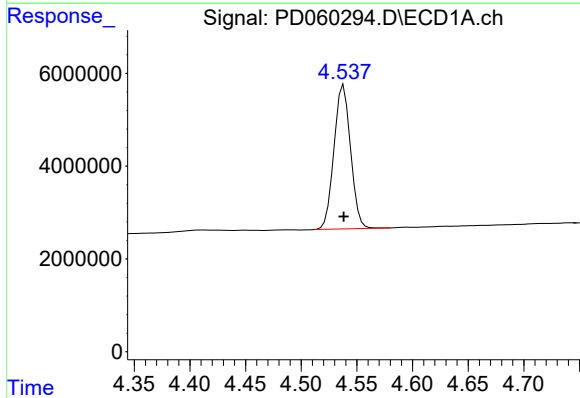


#4 Heptachlor

R.T.: 4.538 min
Delta R.T.: 0.000 min
Response: 32265337
Conc: 20.00 ng/ml

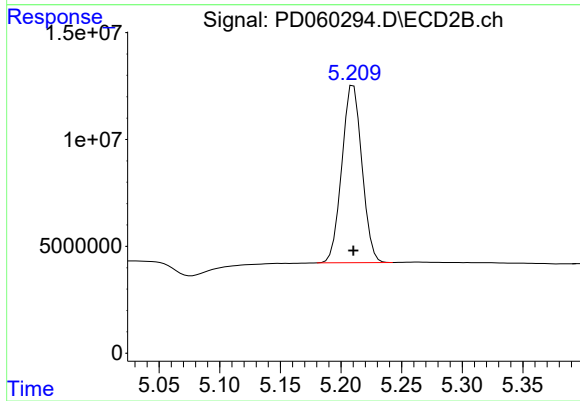

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 95598438
Conc: 20.00 ng/ml

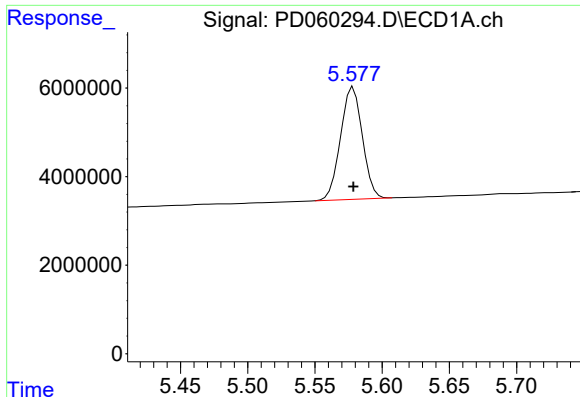

#9 Endosulfan I


R.T.: 5.578 min
Delta R.T.: 0.000 min
Response: 28571349
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

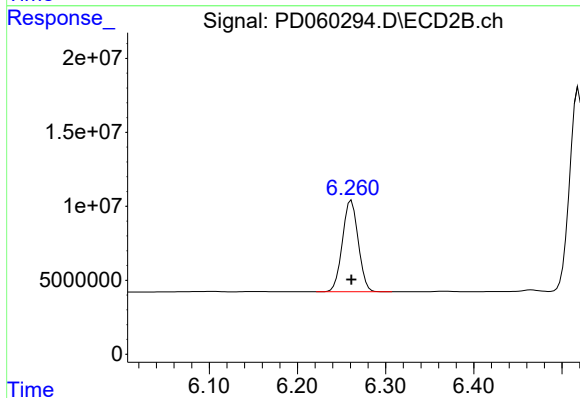


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 76904875
Conc: 20.00 ng/ml

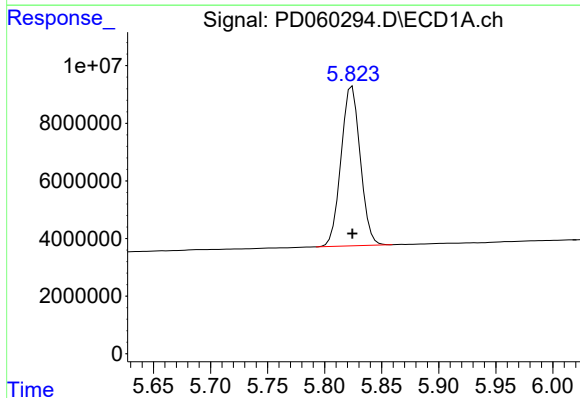


#13 Dieldrin

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 64961714
Conc: 40.00 ng/ml

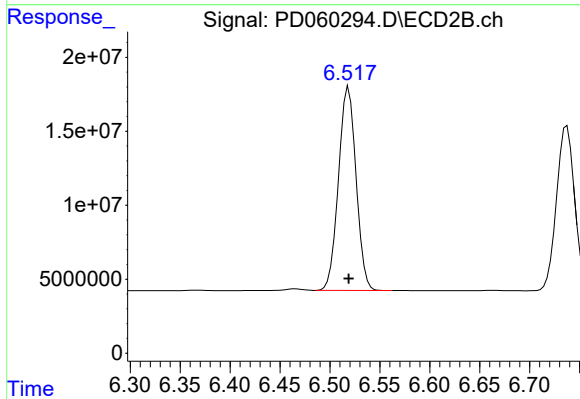

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 168645336
Conc: 40.00 ng/ml

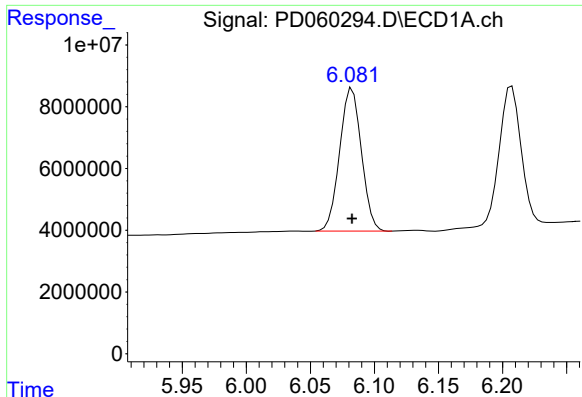

#14 Endrin


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 54709628
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

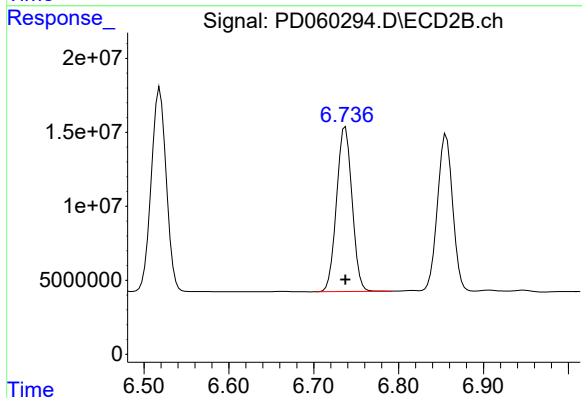


#14 Endrin

R.T.: 6.737 min
Delta R.T.: 0.000 min
Response: 141098494
Conc: 40.00 ng/ml

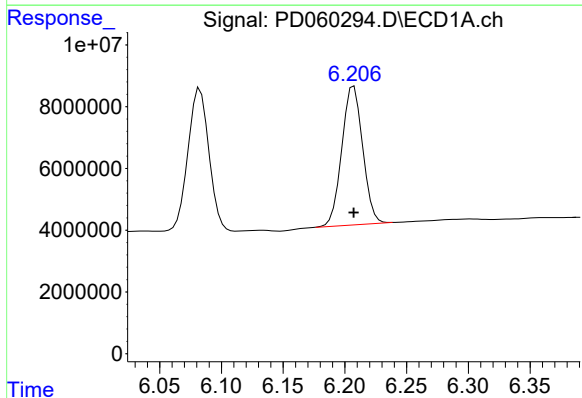


#16 4,4'-DDD

R.T.: 6.207 min
Delta R.T.: 0.000 min
Response: 52807971
Conc: 40.00 ng/ml

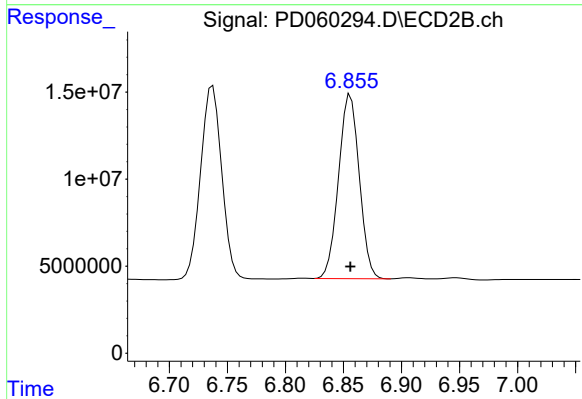

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 131685849
Conc: 40.00 ng/ml

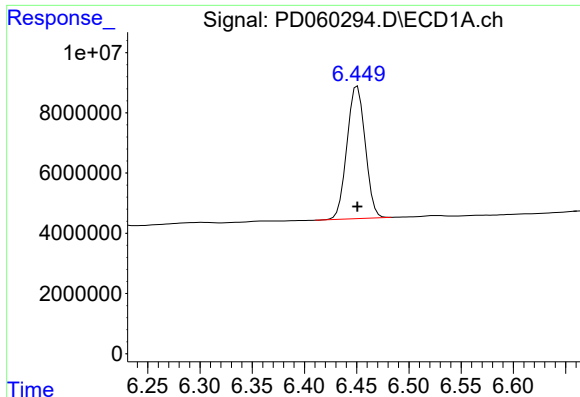

#17 4,4'-DDT


R.T.: 6.451 min
Delta R.T.: 0.000 min
Response: 53382416
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

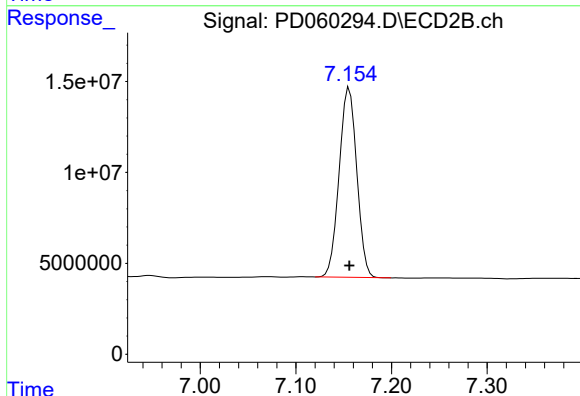


#17 4,4'-DDT

R.T.: 7.156 min
Delta R.T.: 0.000 min
Response: 134017463
Conc: 40.00 ng/ml

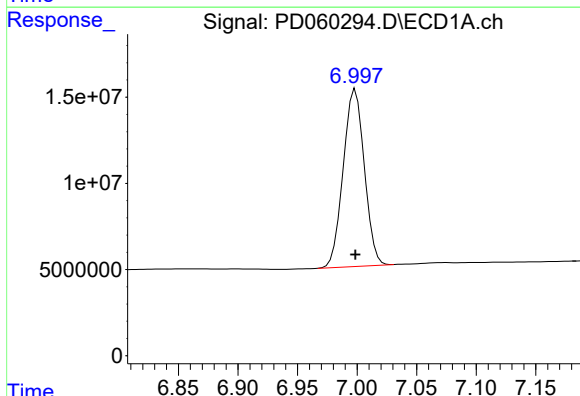


#20 Methoxychlor

R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 126966761
Conc: 200.00 ng/ml

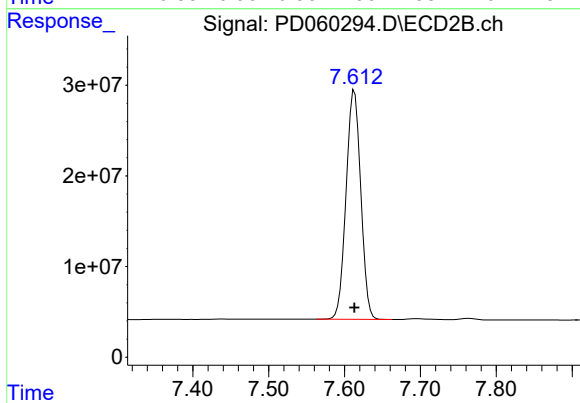

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 340426004
Conc: 200.00 ng/ml

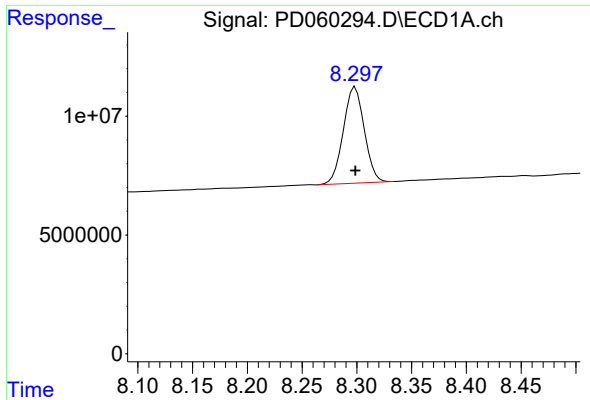

#27 Decachlorobiphenyl

R.T.: 8.299 min
Delta R.T.: 0.000 min
Response: 53956511
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

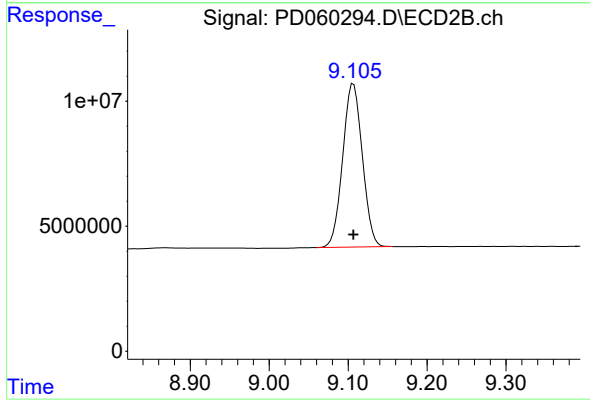

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 113047476
Conc: 40.00 ng/ml