

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 12:33
 Operator : DD\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 12:48:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 25 12:47:07 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.022	43358862	142.5E6	38.718	38.984
27)	SA Decachlor...	8.298	9.107	103.5E6	215.7E6	76.727	76.327
Target Compounds							
2)	A alpha-BHC	3.945	4.413	68600342	218.8E6	39.398	40.469
3)	MA gamma-BHC...	4.232	4.699	64037741	197.0E6	39.027	39.867
4)	MA Heptachlor	4.538	5.210	62671054	187.7E6	38.847	39.263
9)	A Endosulfan I	5.579	6.261	54292383	150.7E6	38.005	39.186
13)	MA Dieldrin	5.824	6.518	125.1E6	333.3E6	77.052	79.054
14)	MA Endrin	6.083	6.737	105.2E6	280.3E6	76.941	79.459
16)	A 4,4'-DDD	6.207	6.856	102.1E6	260.6E6	77.332	79.157
17)	MA 4,4'-DDT	6.450	7.155	104.7E6	269.9E6	78.488	80.544
20)	A Methoxychlor	6.998	7.612	238.4E6	646.7E6	375.487	379.942

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 12:33
Operator : DD\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 12:48:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 25 12:47:07 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

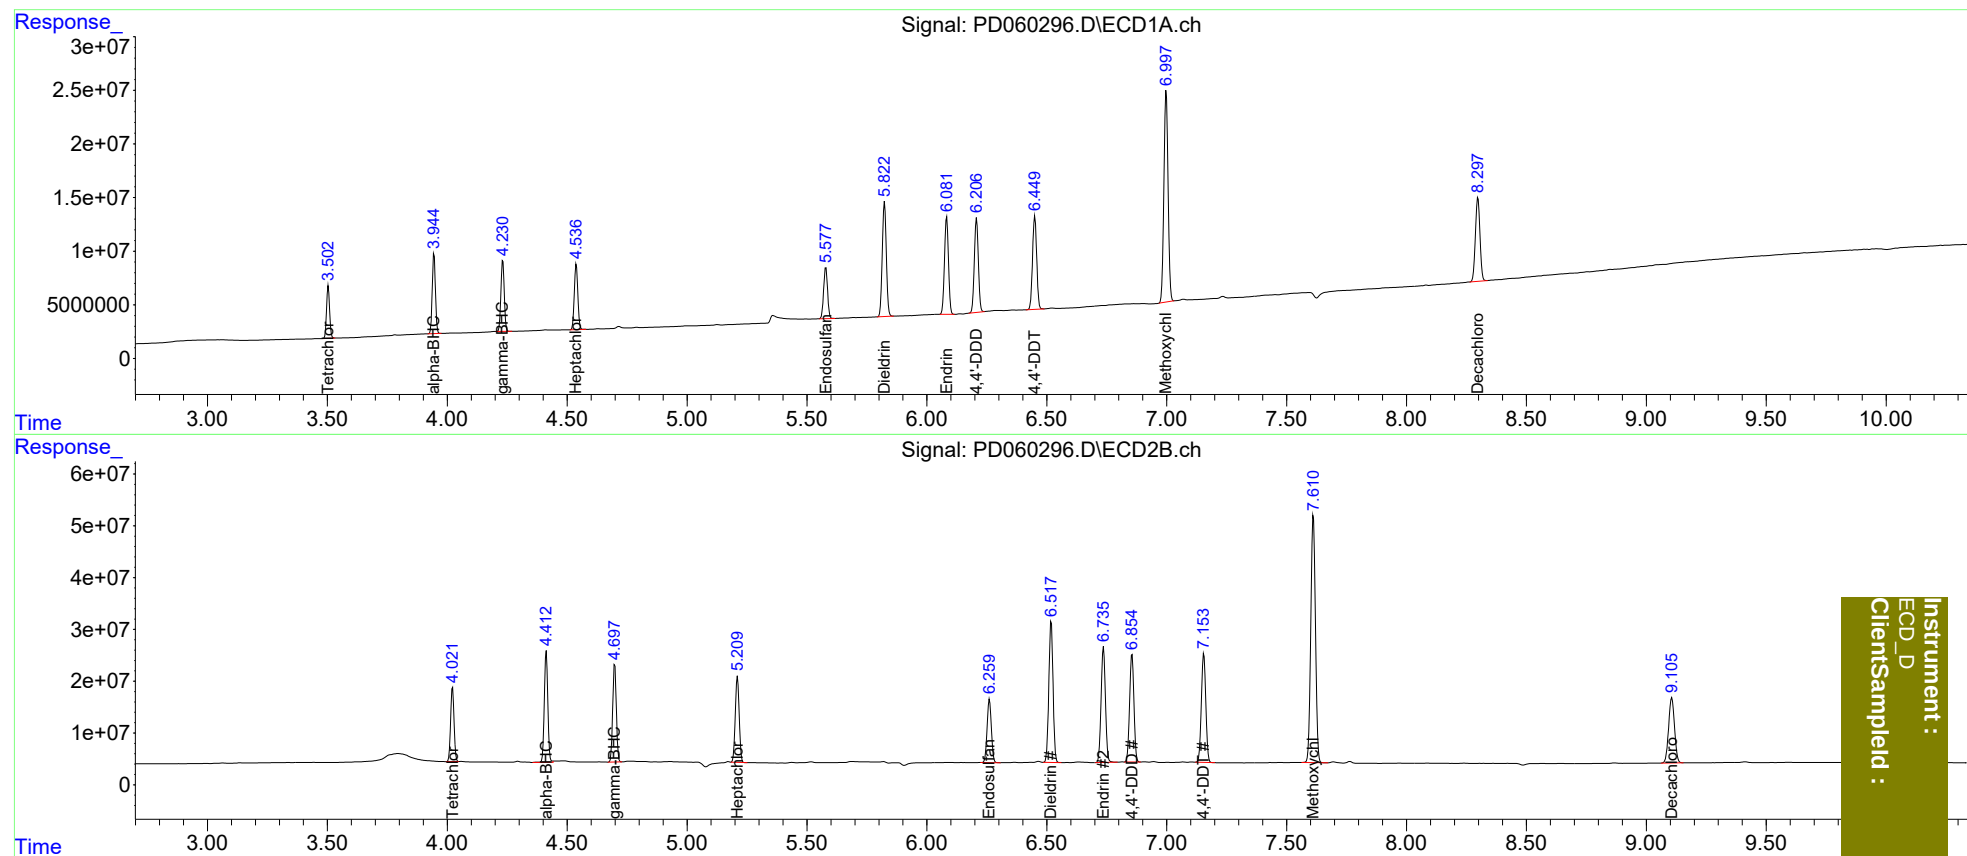


Instrument :
ECD_D
ClientSampled :

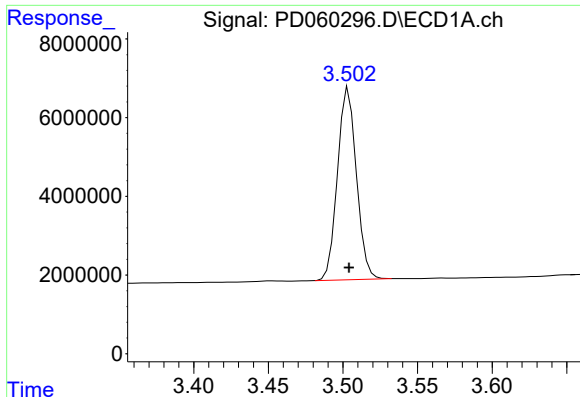

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 43358862
Conc: 38.72 ng/ml

Instrument :
ECD_D
ClientSampleId :

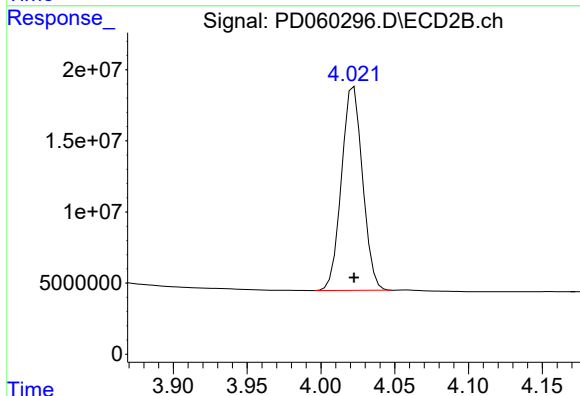


#1 Tetrachloro-m-xylene

R.T.: 4.022 min
Delta R.T.: 0.000 min
Response: 142506648
Conc: 38.98 ng/ml

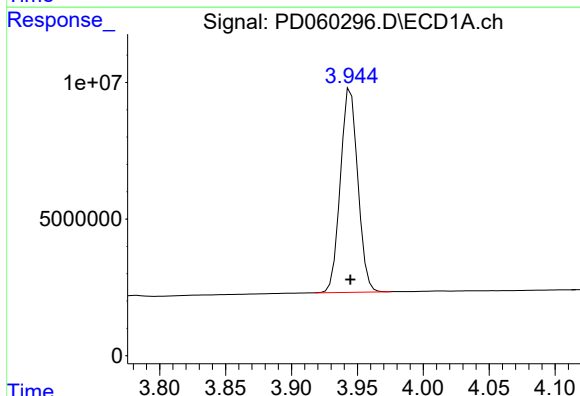


#2 alpha-BHC

R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 68600342
Conc: 39.40 ng/ml

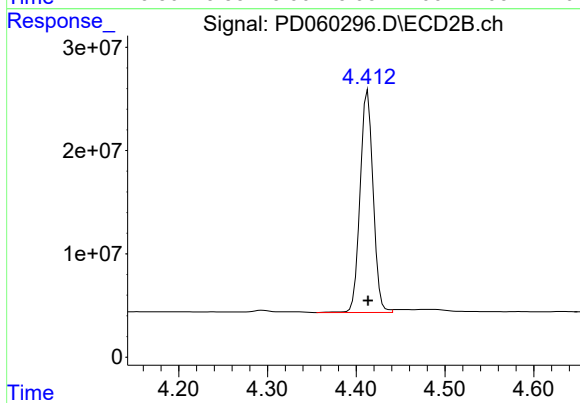

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 218761920
Conc: 40.47 ng/ml

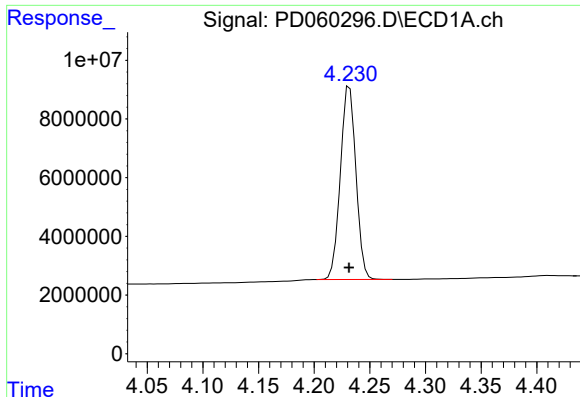

#3 gamma-BHC (Lindane)


R.T.: 4.232 min
Delta R.T.: 0.000 min
Response: 64037741
Conc: 39.03 ng/ml

Instrument :
ECD_D
ClientSampleId :

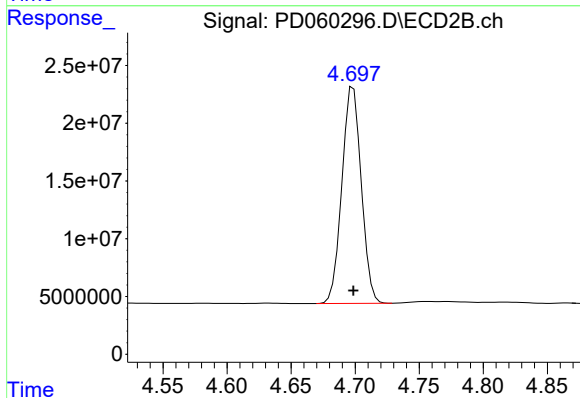


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 197025600
Conc: 39.87 ng/ml

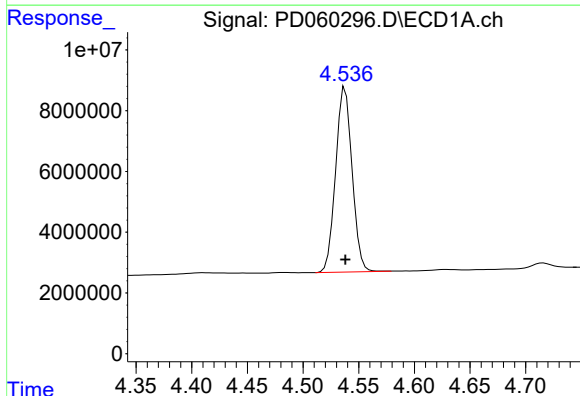


#4 Heptachlor

R.T.: 4.538 min
Delta R.T.: 0.000 min
Response: 62671054
Conc: 38.85 ng/ml

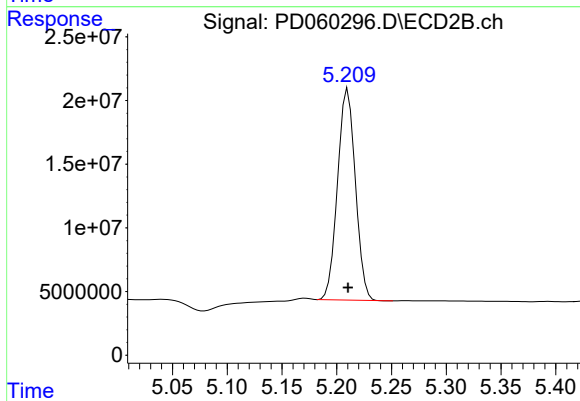

#4 Heptachlor


R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 187673710
Conc: 39.26 ng/ml

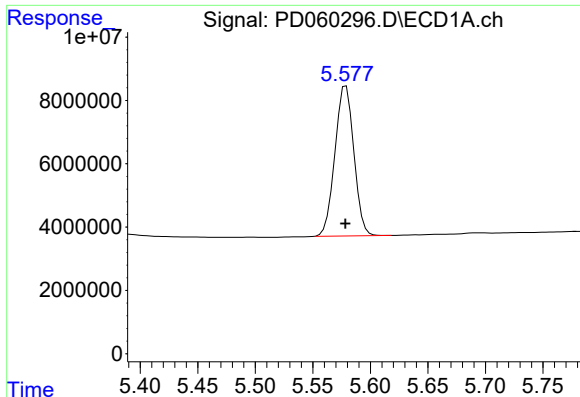

#9 Endosulfan I


R.T.: 5.579 min
Delta R.T.: 0.000 min
Response: 54292383
Conc: 38.00 ng/ml

Instrument :
ECD_D
ClientSampleId :

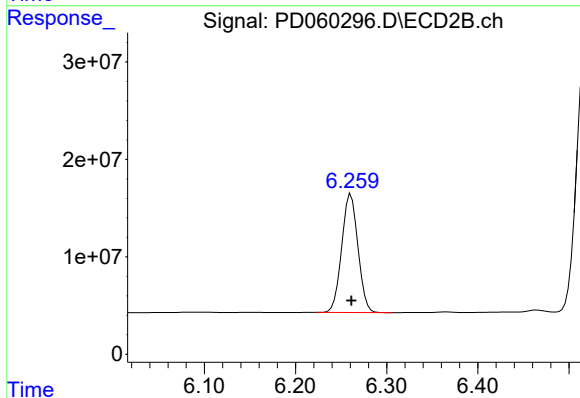


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 150678672
Conc: 39.19 ng/ml

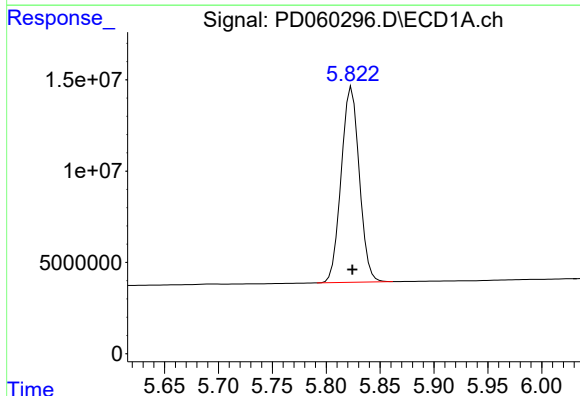


#13 Dieldrin

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 125135698
Conc: 77.05 ng/ml

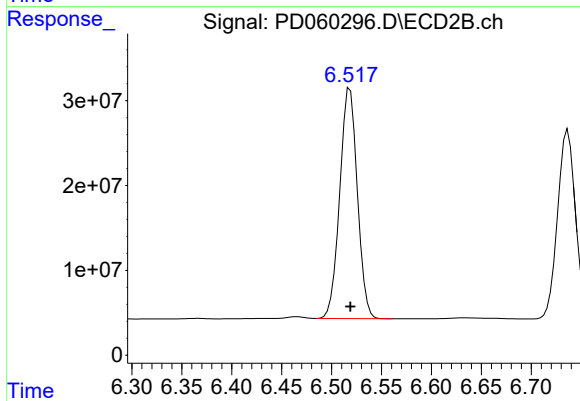

#13 Dieldrin


R.T.: 6.518 min
Delta R.T.: 0.000 min
Response: 333302014
Conc: 79.05 ng/ml

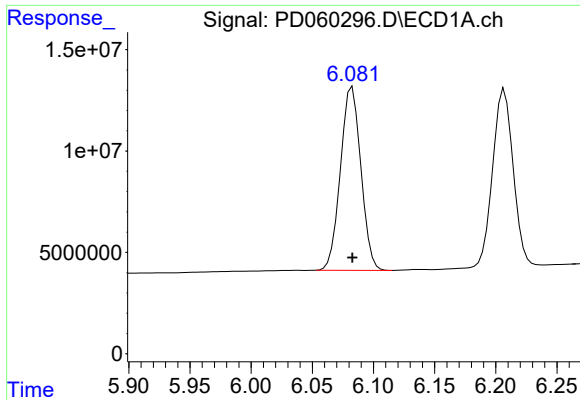

#14 Endrin


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 105235733
Conc: 76.94 ng/ml

Instrument :
ECD_D
ClientSampleId :

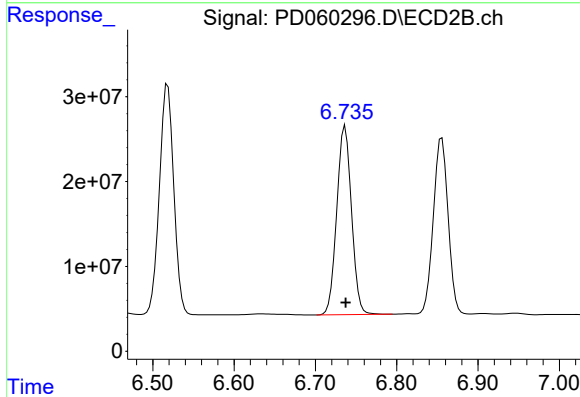


#14 Endrin

R.T.: 6.737 min
Delta R.T.: 0.000 min
Response: 280289476
Conc: 79.46 ng/ml

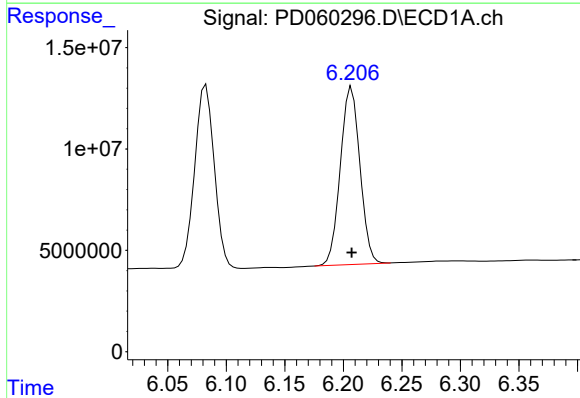


#16 4,4'-DDD

R.T.: 6.207 min
Delta R.T.: 0.000 min
Response: 102094045
Conc: 77.33 ng/ml

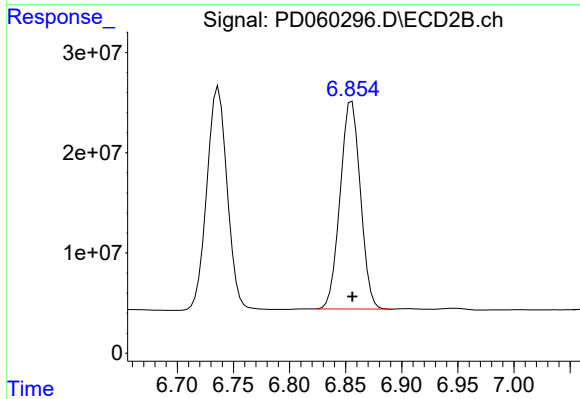

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 260595745
Conc: 79.16 ng/ml

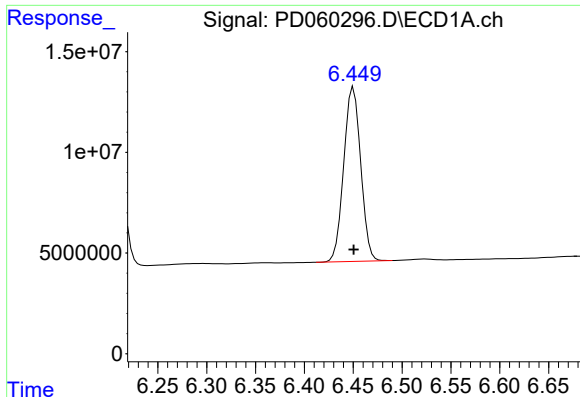

#17 4,4'-DDT


R.T.: 6.450 min
Delta R.T.: 0.000 min
Response: 104747052
Conc: 78.49 ng/ml

Instrument :
ECD_D
ClientSampleId :

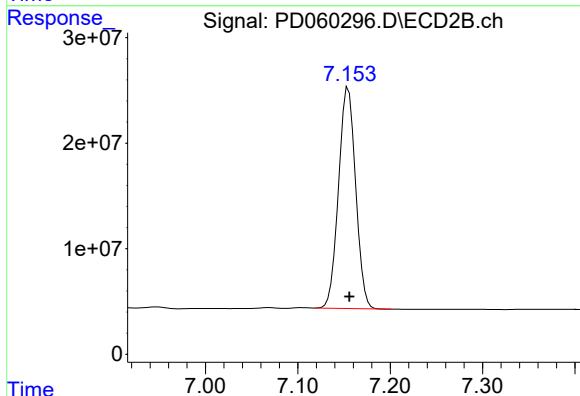


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: -0.001 min
Response: 269858105
Conc: 80.54 ng/ml

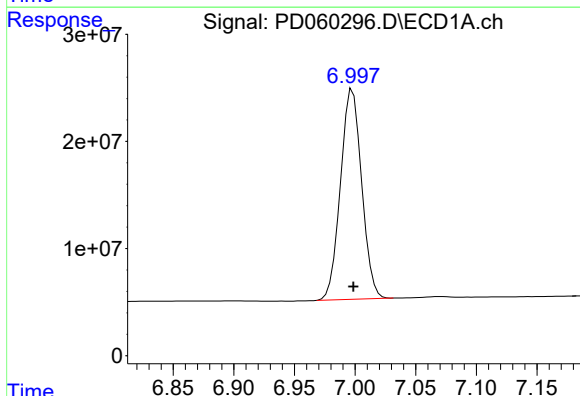


#20 Methoxychlor

R.T.: 6.998 min
Delta R.T.: 0.000 min
Response: 238371648
Conc: 375.49 ng/ml

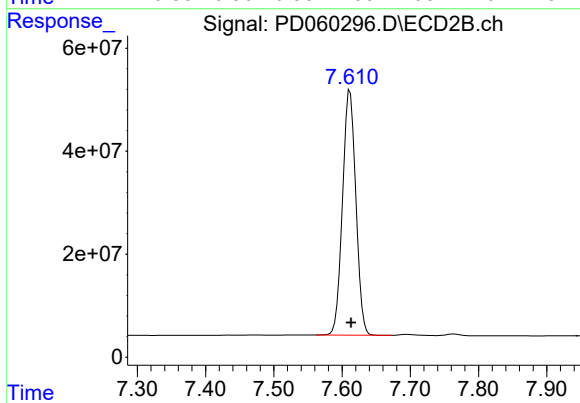

#20 Methoxychlor


R.T.: 7.612 min
Delta R.T.: -0.001 min
Response: 646710185
Conc: 379.94 ng/ml

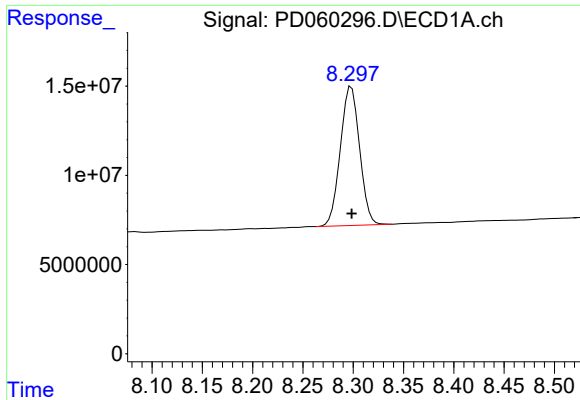

#27 Decachlorobiphenyl

R.T.: 8.298 min
Delta R.T.: 0.000 min
Response: 103498032
Conc: 76.73 ng/ml

Instrument :
ECD_D
ClientSampleId :

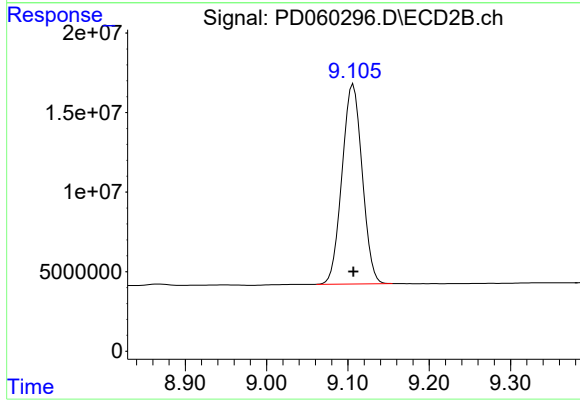

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 215715003
Conc: 76.33 ng/ml