

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 13:01
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:12:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 25 12:52:17 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.023	83949146	277.5E6	75.594	76.093
27)	SA Decachlor...	8.300	9.107	196.7E6	407.1E6	147.757	142.491
Target Compounds							
2)	A alpha-BHC	3.945	4.413	135.2E6	428.4E6	77.901	79.383
3)	MA gamma-BHC...	4.231	4.699	125.8E6	389.5E6	76.672	79.946
4)	MA Heptachlor	4.538	5.211	120.7E6	373.0E6	75.290	78.846
9)	A Endosulfan I	5.578	6.261	106.7E6	294.9E6	74.931	77.128
13)	MA Dieldrin	5.824	6.519	243.8E6	651.0E6	150.801	156.262
14)	MA Endrin	6.083	6.737	201.3E6	542.8E6	146.419	155.181
16)	A 4,4'-DDD	6.207	6.856	198.1E6	510.1E6	150.173	156.399
17)	MA 4,4'-DDT	6.451	7.155	205.2E6	527.9E6	156.382	159.489
20)	A Methoxychlor	6.998	7.613	438.8E6	1178.7E6	689.306	686.503

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 13:01
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:12:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 25 12:52:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

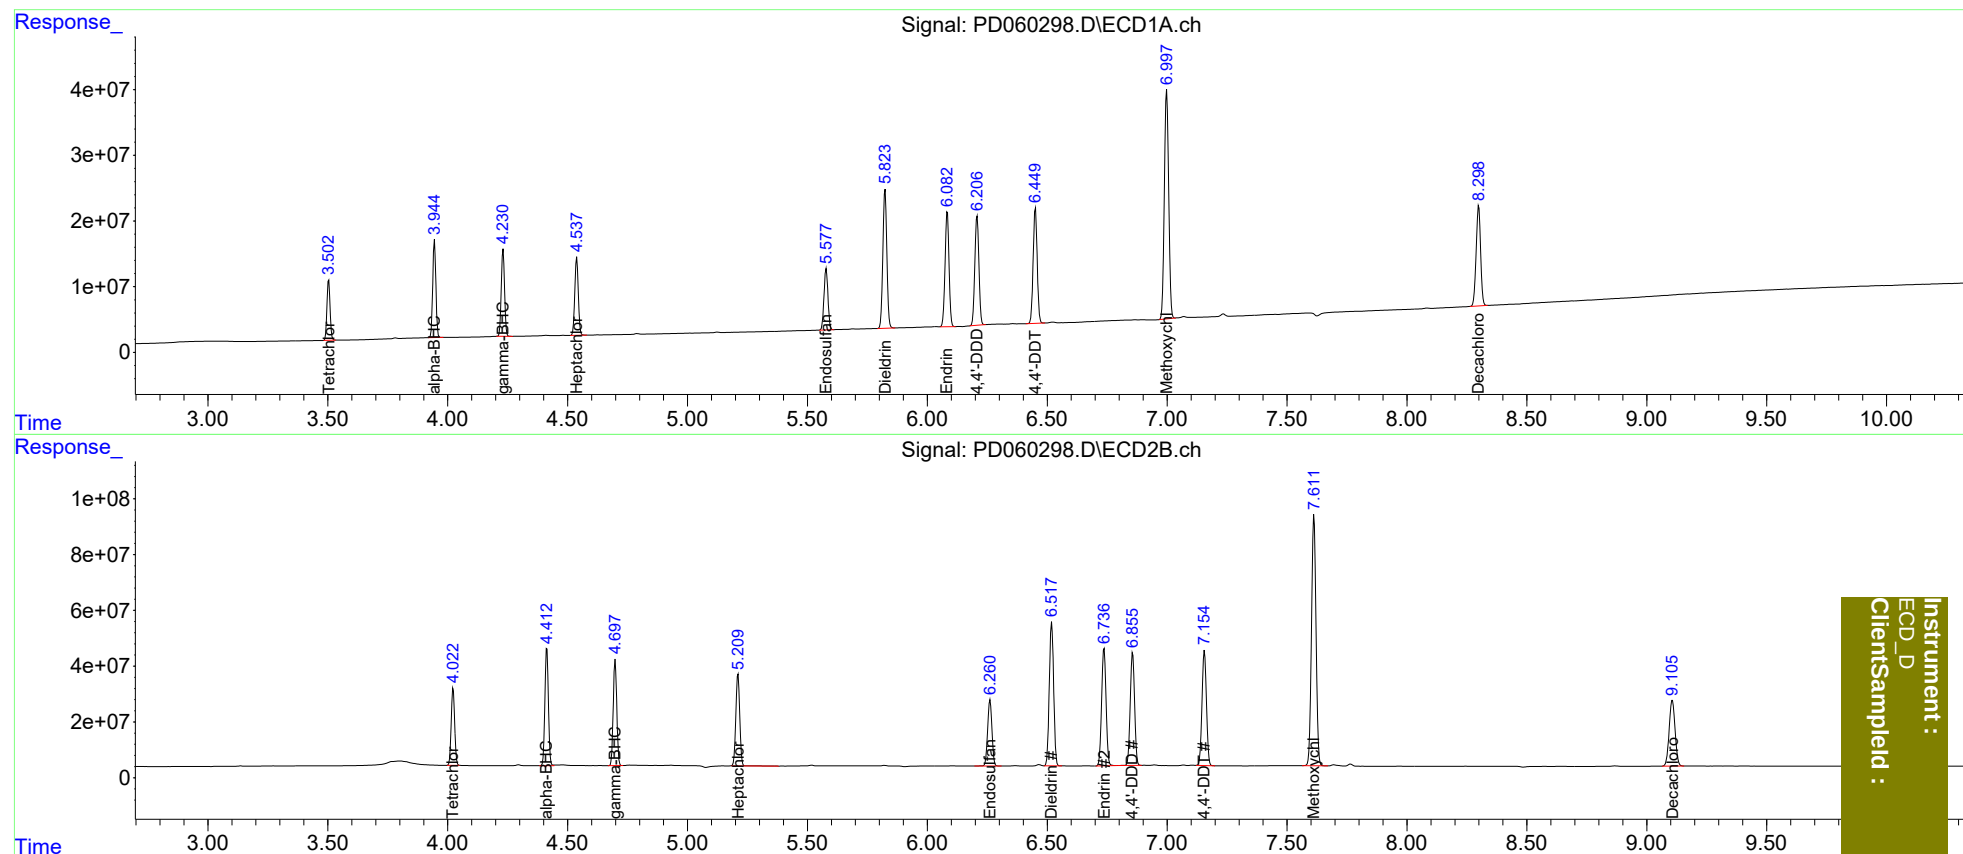


Instrument :
ECD_D
ClientSampled :

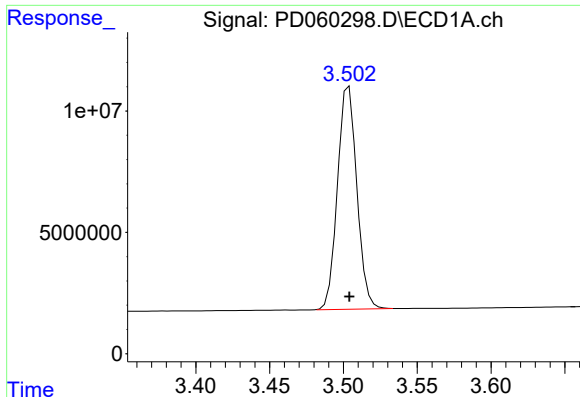

#1 Tetrachloro-m-xylene


R.T.: 3.504 min
Delta R.T.: 0.000 min
Response: 83949146
Conc: 75.59 ng/ml

Instrument :
ECD_D
ClientSampleId :

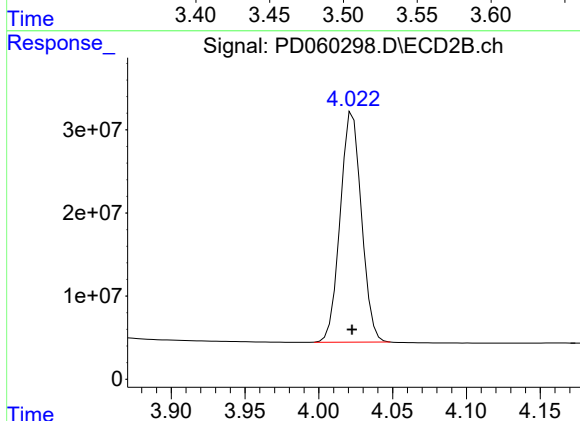


#1 Tetrachloro-m-xylene

R.T.: 4.023 min
Delta R.T.: 0.000 min
Response: 277461769
Conc: 76.09 ng/ml

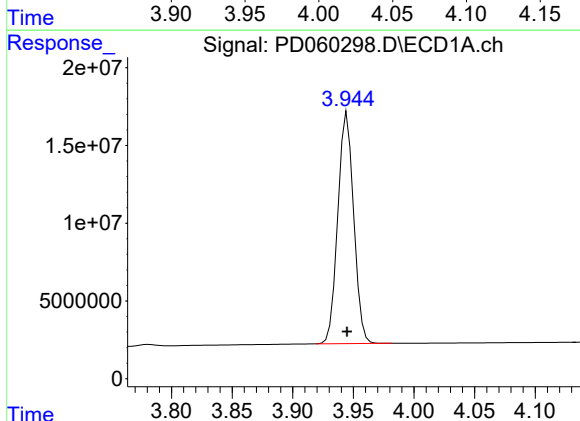


#2 alpha-BHC

R.T.: 3.945 min
Delta R.T.: 0.000 min
Response: 135182918
Conc: 77.90 ng/ml

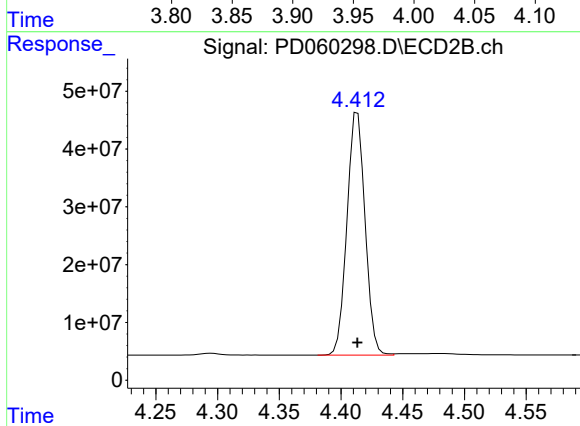

#2 alpha-BHC


R.T.: 4.413 min
Delta R.T.: 0.000 min
Response: 428420990
Conc: 79.38 ng/ml

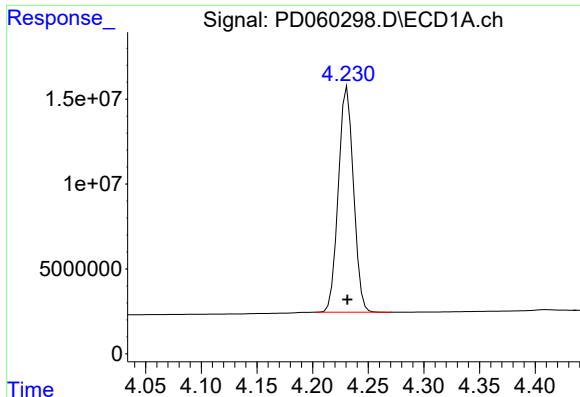

#3 gamma-BHC (Lindane)


R.T.: 4.231 min
Delta R.T.: 0.000 min
Response: 125783301
Conc: 76.67 ng/ml

Instrument :
ECD_D
ClientSampleId :

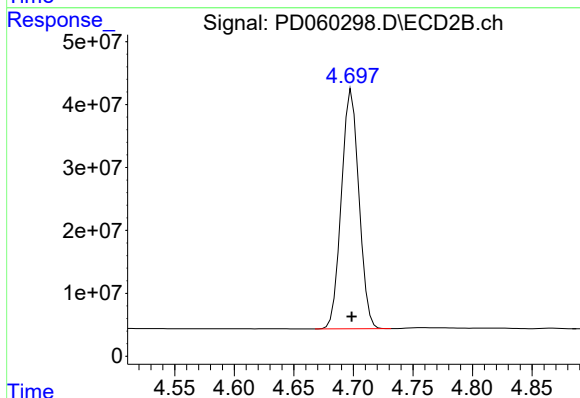


#3 gamma-BHC (Lindane)

R.T.: 4.699 min
Delta R.T.: 0.000 min
Response: 389520612
Conc: 79.95 ng/ml

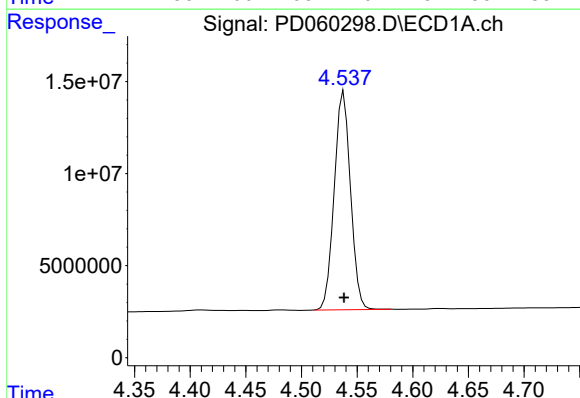


#4 Heptachlor

R.T.: 4.538 min
Delta R.T.: 0.000 min
Response: 120659384
Conc: 75.29 ng/ml

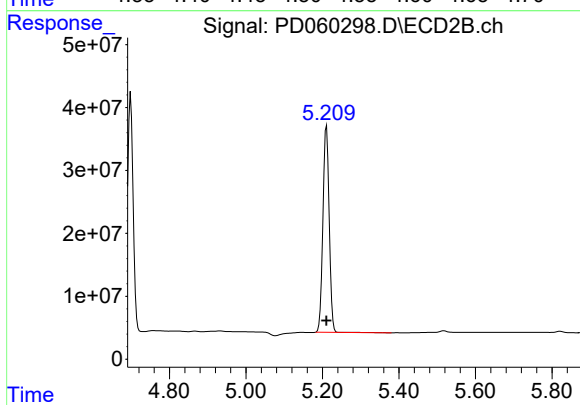

#4 Heptachlor


R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 373044068
Conc: 78.85 ng/ml

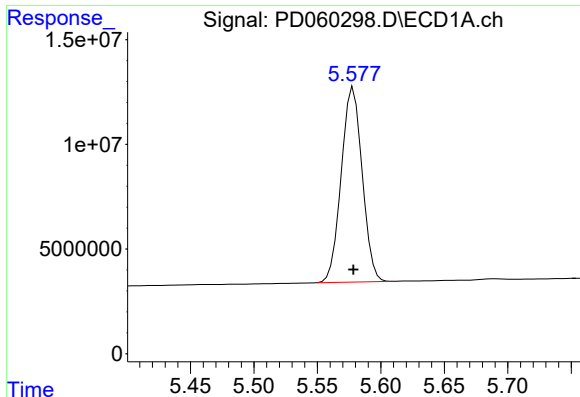

#9 Endosulfan I


R.T.: 5.578 min
Delta R.T.: 0.000 min
Response: 106665531
Conc: 74.93 ng/ml

Instrument :
ECD_D
ClientSampleId :

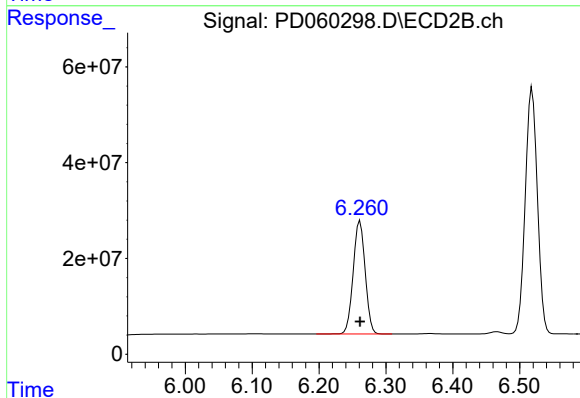


#9 Endosulfan I

R.T.: 6.261 min
Delta R.T.: 0.000 min
Response: 294879131
Conc: 77.13 ng/ml

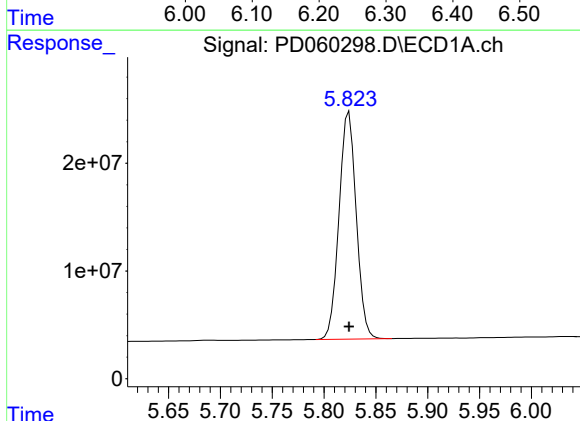


#13 Dieldrin

R.T.: 5.824 min
Delta R.T.: 0.000 min
Response: 243837254
Conc: 150.80 ng/ml

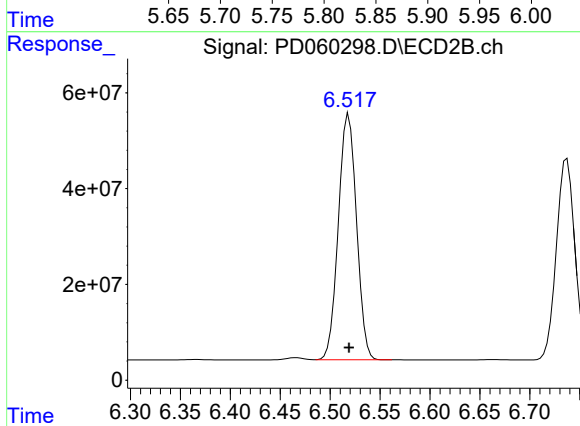

#13 Dieldrin


R.T.: 6.519 min
Delta R.T.: 0.000 min
Response: 650961913
Conc: 156.26 ng/ml

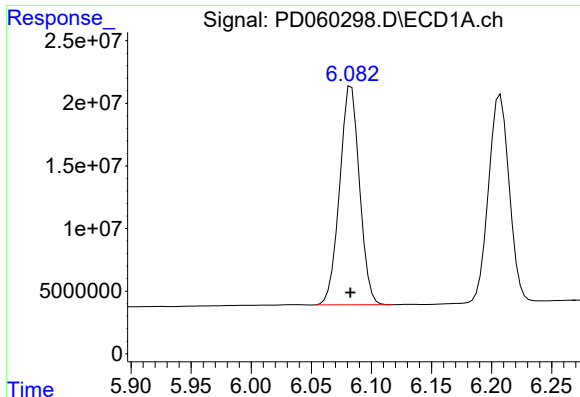

#14 Endrin


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 201297149
Conc: 146.42 ng/ml

Instrument :
ECD_D
ClientSampleId :

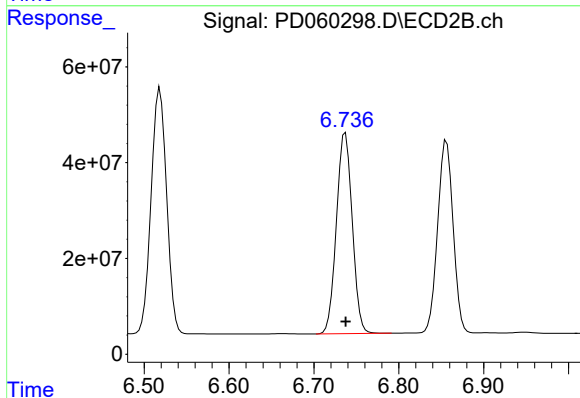


#14 Endrin

R.T.: 6.737 min
Delta R.T.: 0.000 min
Response: 542799378
Conc: 155.18 ng/ml

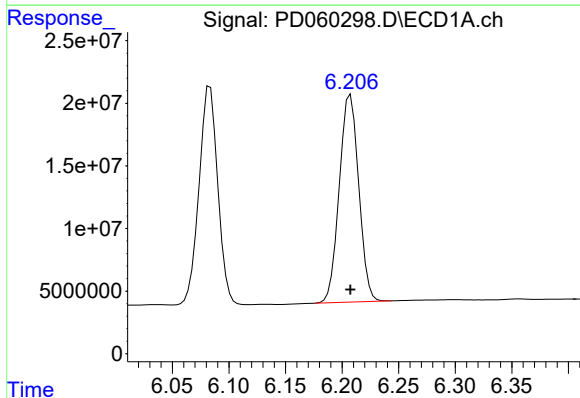


#16 4,4'-DDD

R.T.: 6.207 min
Delta R.T.: 0.000 min
Response: 198083104
Conc: 150.17 ng/ml

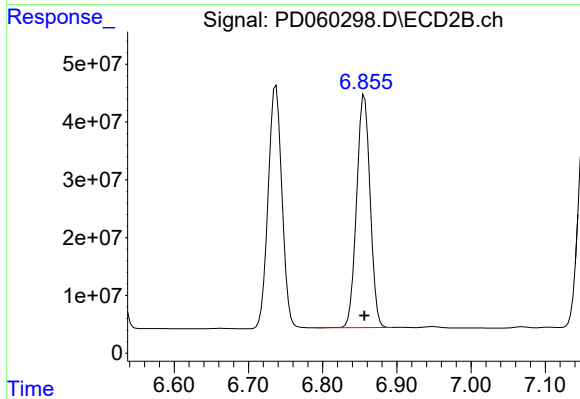

#16 4,4'-DDD


R.T.: 6.856 min
Delta R.T.: 0.000 min
Response: 510052187
Conc: 156.40 ng/ml

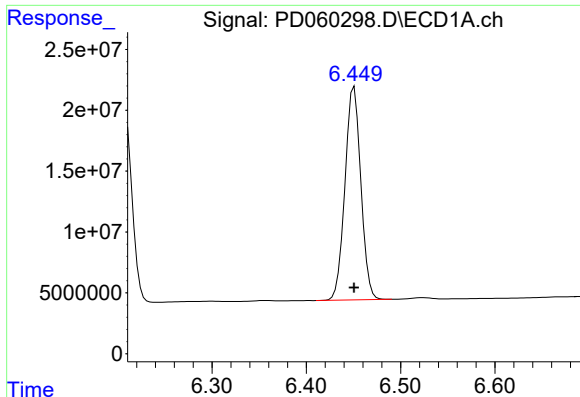

#17 4,4'-DDT


R.T.: 6.451 min
Delta R.T.: 0.000 min
Response: 205181703
Conc: 156.38 ng/ml

Instrument :
ECD_D
ClientSampleId :

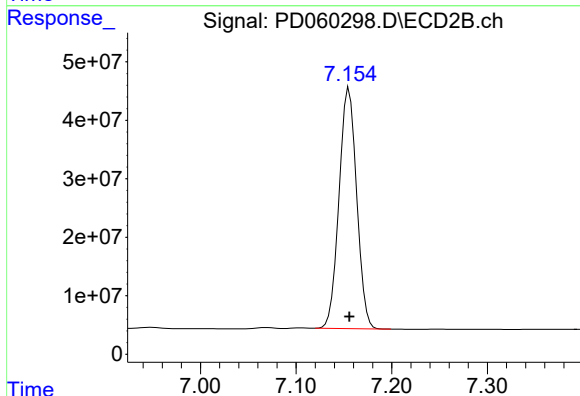


#17 4,4'-DDT

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 527941949
Conc: 159.49 ng/ml

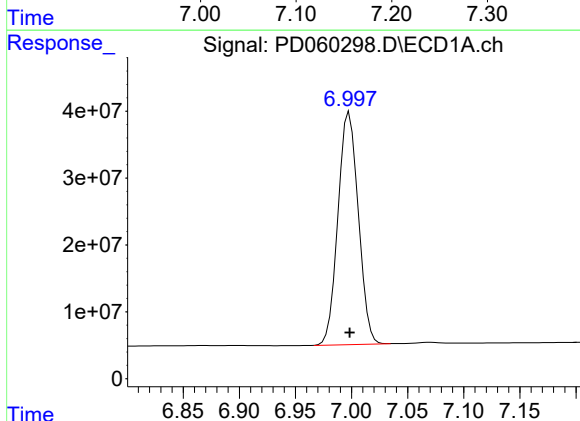


#20 Methoxychlor

R.T.: 6.998 min
Delta R.T.: 0.000 min
Response: 438751881
Conc: 689.31 ng/ml

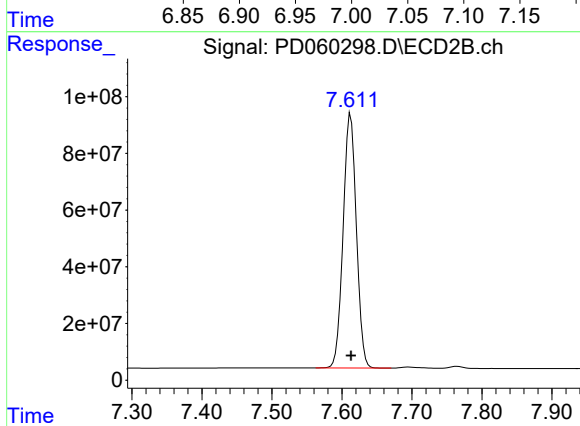

#20 Methoxychlor


R.T.: 7.613 min
Delta R.T.: 0.000 min
Response: 1178700900
Conc: 686.50 ng/ml

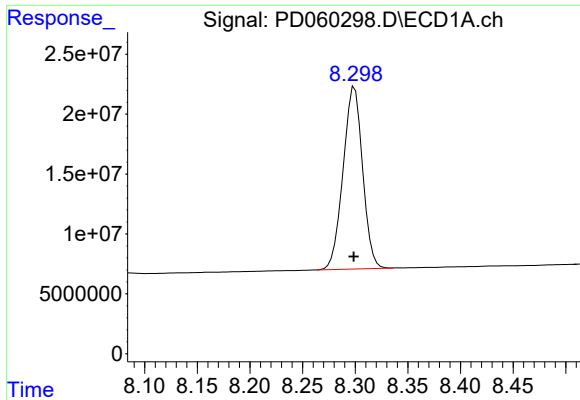

#27 Decachlorobiphenyl

R.T.: 8.300 min
Delta R.T.: 0.000 min
Response: 196740887
Conc: 147.76 ng/ml

Instrument :
ECD_D
ClientSampleId :

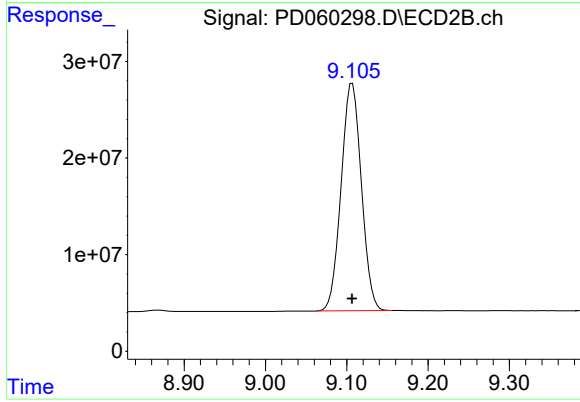

#27 Decachlorobiphenyl

R.T.: 9.107 min
Delta R.T.: 0.000 min
Response: 407069322
Conc: 142.49 ng/ml