

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
 Data File : PD060298.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Nov 2020 13:01
 Operator : DD\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA501

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 25 13:12:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Nov 25 12:52:17 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.504	4.023	83949146	277.5E6	75.594	76.093
27)	SA Decachlor...	8.300	9.107	196.7E6	407.1E6	147.757	142.491
Target Compounds							
2)	A alpha-BHC	3.945	4.413	135.2E6	428.4E6	77.901	79.383
3)	MA gamma-BHC...	4.231	4.699	125.8E6	389.5E6	76.672	79.946
4)	MA Heptachlor	4.538	5.211	120.7E6	373.0E6	75.290	78.846
9)	A Endosulfan I	5.578	6.261	106.7E6	294.9E6	74.931	77.128
13)	MA Dieldrin	5.824	6.519	243.8E6	651.0E6	150.801	156.262
14)	MA Endrin	6.083	6.737	201.3E6	542.8E6	146.419	155.181
16)	A 4,4'-DDD	6.207	6.856	198.1E6	510.1E6	150.173	156.399
17)	MA 4,4'-DDT	6.451	7.155	205.2E6	527.9E6	156.382	159.489
20)	A Methoxychlor	6.998	7.613	438.8E6	1178.7E6	689.306	686.503

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD112520\
Data File : PD060298.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Nov 2020 13:01
Operator : DD\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 25 13:12:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD112520CLP.M
Quant Title : GC Extractables
QLast Update : Wed Nov 25 12:52:17 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

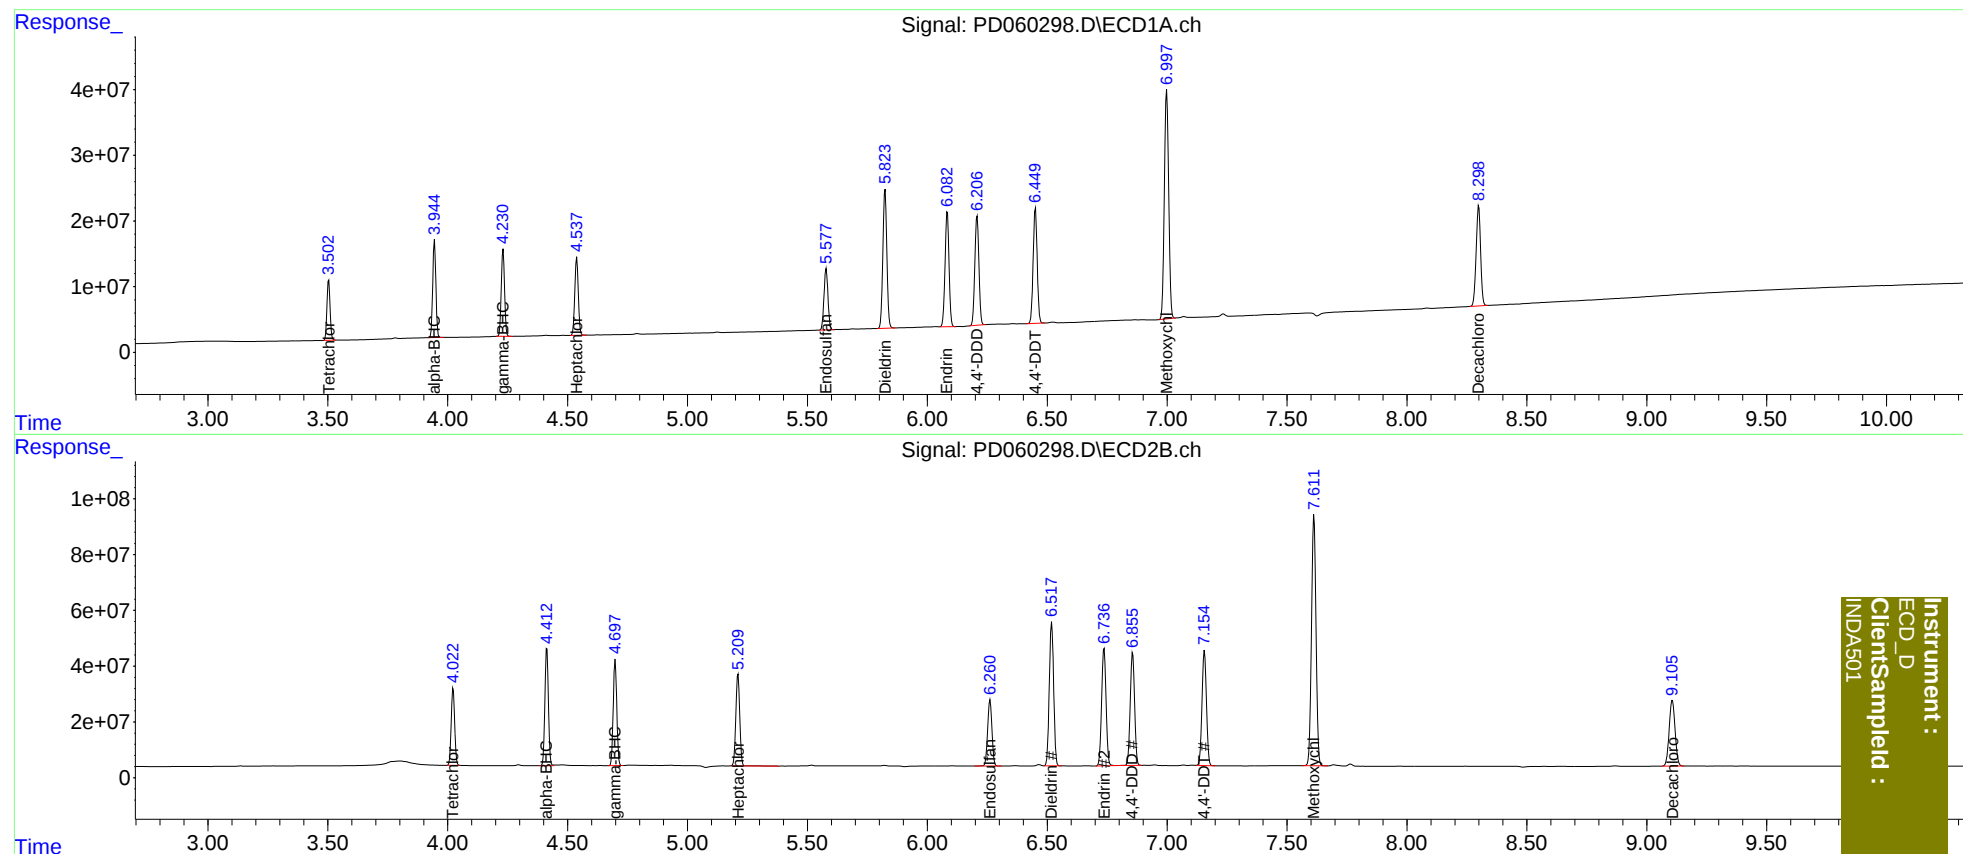

Instrument :
ECD_D
ClientSample :
INDA501